

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
 Data File : BM026266.D
 Acq On : 04 Jun 2020 20:26
 Operator : JU/CG
 Sample : L2844-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Quant Time: Jun 05 01:24:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 05 01:05:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	139514	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	564160	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	330571	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	702676	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	757394	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	807653	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	23183	5.01	ng/uL	0.00
5) Phenol-d5	6.66	99	84877	6.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	241776	27.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	225078	22.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	158305	16.60	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	134436	29.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	142910	31.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	263418	28.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	15990	1.73	ng/ul	0.01
44) Dimethylphthalate-d6	13.53	166	910229	34.34	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	1041042	33.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	27105	5.77	ng/ul	0.01
58) Fluorene-d10	15.11	176	780622	33.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	133416	32.56	ng/ul	0.00
71) Anthracene-d10	16.96	188	1254973	36.24	ng/ul	0.00
79) Pyrene-d10	19.26	212	1435661	36.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	1342904	31.24	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.58	163	87468	3.143	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
Data File : BM026266.D
Acq On : 04 Jun 2020 20:26
Operator : JU/CG
Sample : L2844-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Time: Jun 05 01:24:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 05 01:05:40 2020
Response via : Initial Calibration

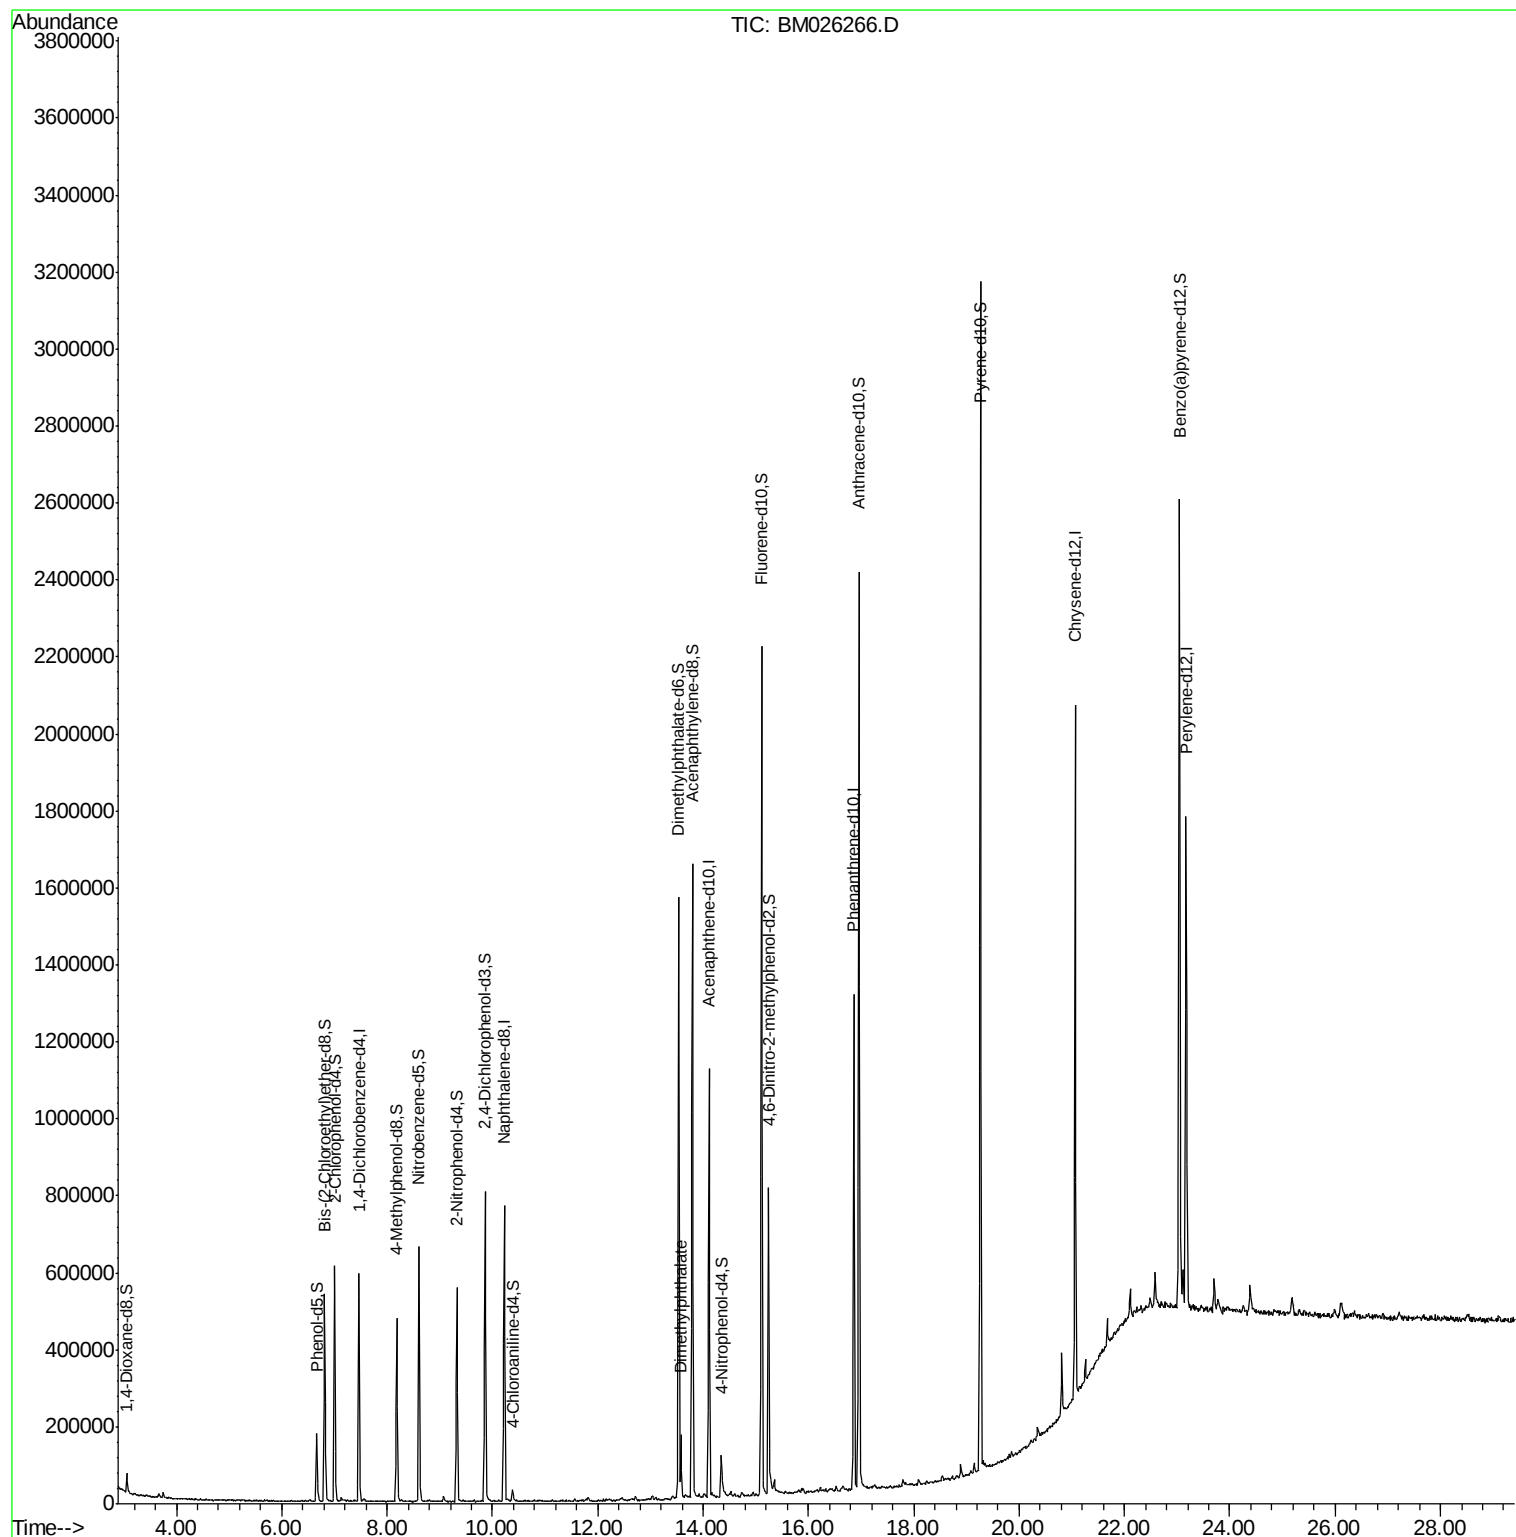

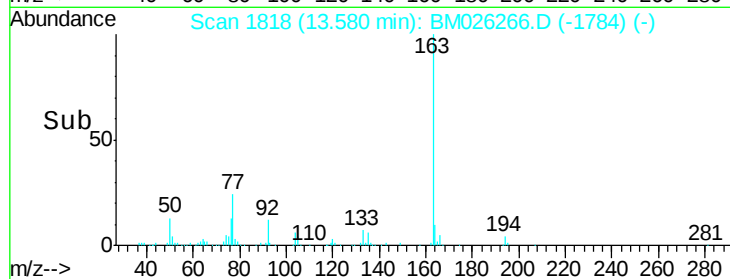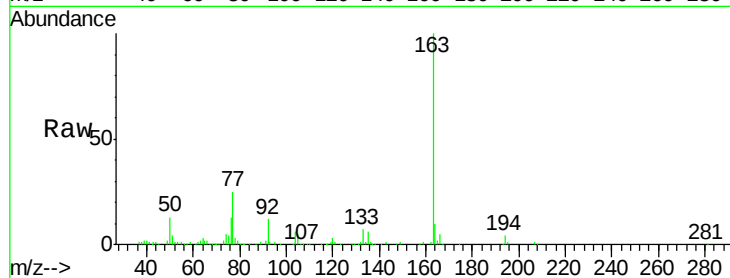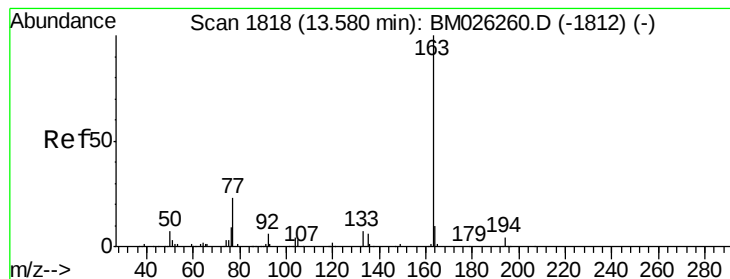

#45

Dimethylphthalate

Concen: 3.143 ng/ul

RT: 13.58 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM026266.D

Acq: 04 Jun 2020 20:26

Instrument :

BNA_M

ClientSampleId :

C0AF4

Tot Ion:163 Resp: 87468

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.4 8.0 12.0

