

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045856.D
 Acq On : 05 Jun 2024 18:56
 Operator : MA/JU
 Sample : P2586-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D30

Quant Time: Jun 06 01:13:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 31 13:01:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.463	152	274688	20.000	ng/ul	0.00
20) Naphthalene-d8	10.233	136	1113354	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.104	164	604408	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.851	188	1010974	20.000	ng/ul	0.00
79) Chrysene-d12	21.062	240	780390	20.000	ng/ul	0.00
88) Perylene-d12	23.786	264	886917	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.058	96	21987	3.103	ng/uL	0.00
4) Pyridine-d5	3.469	84	321686	17.634	ng/ul	0.00
7) Phenol-d5	6.722	99	470193	20.149	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.828	67	320358	19.118	ng/ul	0.00
11) 2-Chlorophenol-d4	7.028	132	365232	20.953	ng/ul	0.00
15) 4-Methylphenol-d8	8.234	113	361342	20.496	ng/ul	0.00
21) Nitrobenzene-d5	8.628	128	182699	20.988	ng/ul	0.00
24) 2-Nitrophenol-d4	9.339	143	183870	20.870	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.892	165	329701	19.957	ng/ul	0.00
31) 4-Chloroaniline-d4	10.410	131	465783	20.371	ng/ul	-0.01
46) Dimethylphthalate-d6	13.557	166	923634	22.074	ng/ul	0.00
49) Acenaphthylene-d8	13.798	160	1024167	21.078	ng/ul	0.00
54) 4-Nitrophenol-d4	14.410	143	111516	12.349	ng/ul	0.00
60) Fluorene-d10	15.104	176	725966	20.337	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.245	200	52791	10.226	ng/ul	0.00
73) Anthracene-d10	16.951	188	933491	21.240	ng/ul	0.00
81) Pyrene-d10	19.251	212	981986	20.234	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.597	264	901153	21.740	ng/ul	0.00
Target Compounds						
					Qvalue	
18) 4-Methylphenol	8.292	108	42463	2.316	ng/ul	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045856.D
Acq On : 05 Jun 2024 18:56
Operator : MA/JU
Sample : P2586-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4D30

Quant Time: Jun 06 01:13:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 31 13:01:11 2024
Response via : Initial Calibration

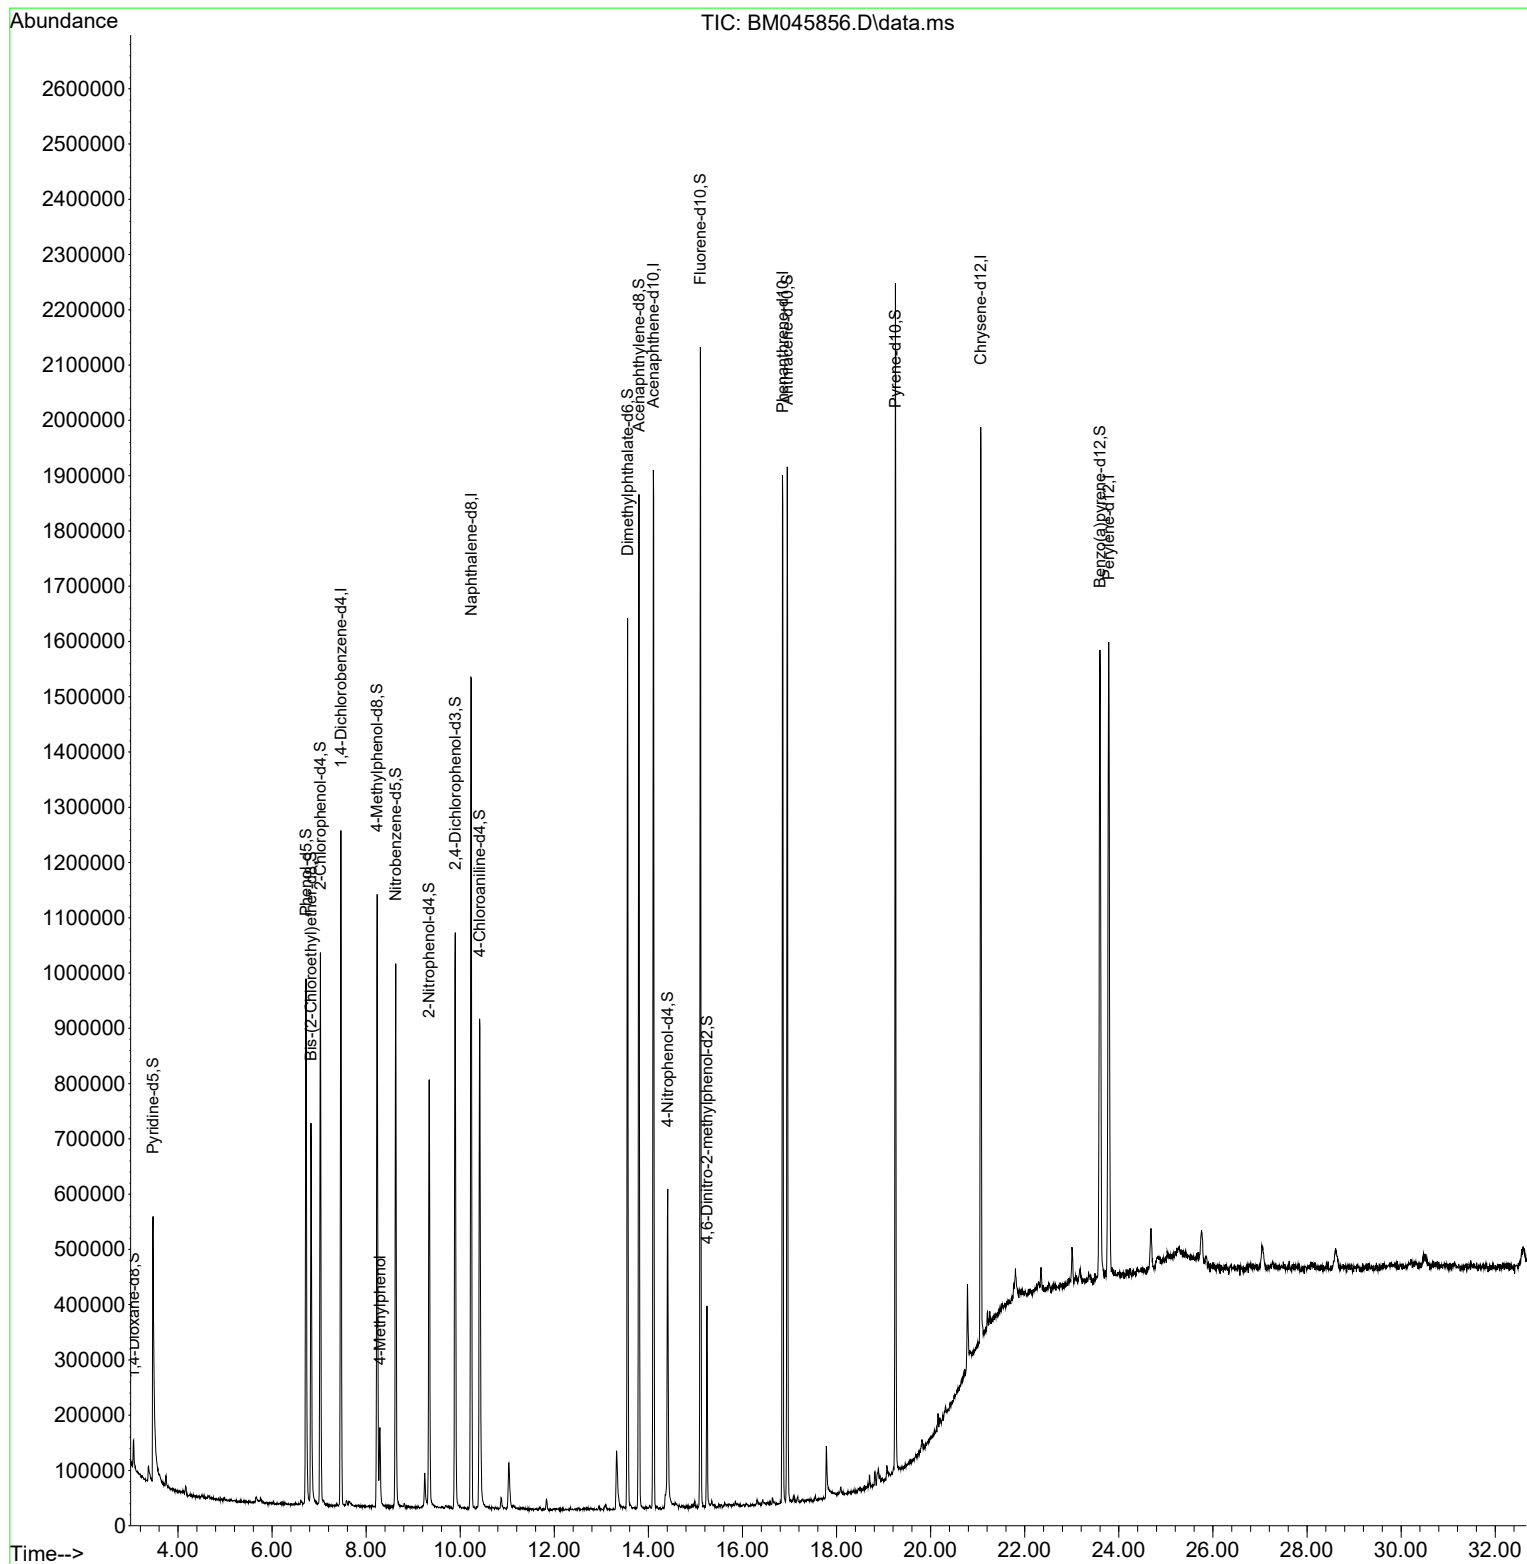

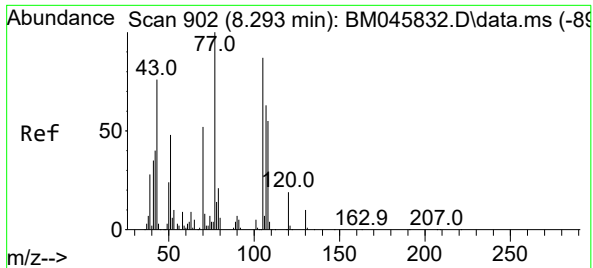

#18
 4-Methylphenol
 Concen: 2.316 ng/ul
 RT: 8.292 min Scan# 90
 Delta R.T. -0.006 min
 Lab File: BM045856.D
 Acq: 05 Jun 2024 18:56

Instrument :
 BNA_M
 ClientSampleId :
 A4D30

Tgt Ion:108 Resp: 42463
 Ion Ratio Lower Upper
 108 100
 107 129.1 90.6 136.0

