

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045828.D
 Acq On : 04 Jun 2024 22:31
 Operator : MA/JU
 Sample : P2589-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6D1

Quant Time: Jun 04 23:07:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 31 13:01:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.463	152	273770	20.000	ng/u1	0.00
20) Naphthalene-d8	10.234	136	1173354	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.110	164	740950	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.857	188	1484112	20.000	ng/u1	0.00
79) Chrysene-d12	21.062	240	1092429	20.000	ng/u1	0.00
88) Perylene-d12	23.786	264	948059	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.058	96	22440	3.178	ng/uL	0.00
4) Pyridine-d5	3.470	84	301667	16.592	ng/u1	0.00
7) Phenol-d5	6.722	99	517216	22.239	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.834	67	353124	21.144	ng/u1	0.00
11) 2-Chlorophenol-d4	7.028	132	402392	23.162	ng/u1	0.00
15) 4-Methylphenol-d8	8.234	113	392308	22.327	ng/u1	0.00
21) Nitrobenzene-d5	8.634	128	201974	22.016	ng/u1	0.00
24) 2-Nitrophenol-d4	9.346	143	223375	24.058	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.893	165	413532	23.751	ng/u1	0.00
31) 4-Chloroaniline-d4	10.416	131	558688	23.185	ng/u1	0.00
46) Dimethylphthalate-d6	13.557	166	1430580	27.889	ng/u1	0.00
49) Acenaphthylene-d8	13.798	160	1521362	25.541	ng/u1	0.00
54) 4-Nitrophenol-d4	14.404	143	221384	19.998	ng/u1	0.00
60) Fluorene-d10	15.110	176	1201004	27.445	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.245	200	94616	12.485	ng/u1	0.00
73) Anthracene-d10	16.951	188	1829736	28.360	ng/u1	0.00
81) Pyrene-d10	19.251	212	2098210	30.885	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.603	264	1314972	29.677	ng/u1	0.00
Target Compounds					Qvalue	
72) Phenanthrene	16.892	178	84292	1.078	ng/u1	98
80) Fluoranthene	18.916	202	211940	2.573	ng/u1	100
82) Pyrene	19.280	202	190687	2.253	ng/u1	99
87) Chrysene	21.104	228	88178	1.264	ng/u1	96
90) Benzo(b)fluoranthene	22.933	252	95221	1.634	ng/u1#	95
93) Benzo(a)pyrene	23.651	252	54500	1.065	ng/u1#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045828.D
Acq On : 04 Jun 2024 22:31
Operator : MA/JU
Sample : P2589-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6D1

Quant Time: Jun 04 23:07:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 31 13:01:11 2024
Response via : Initial Calibration

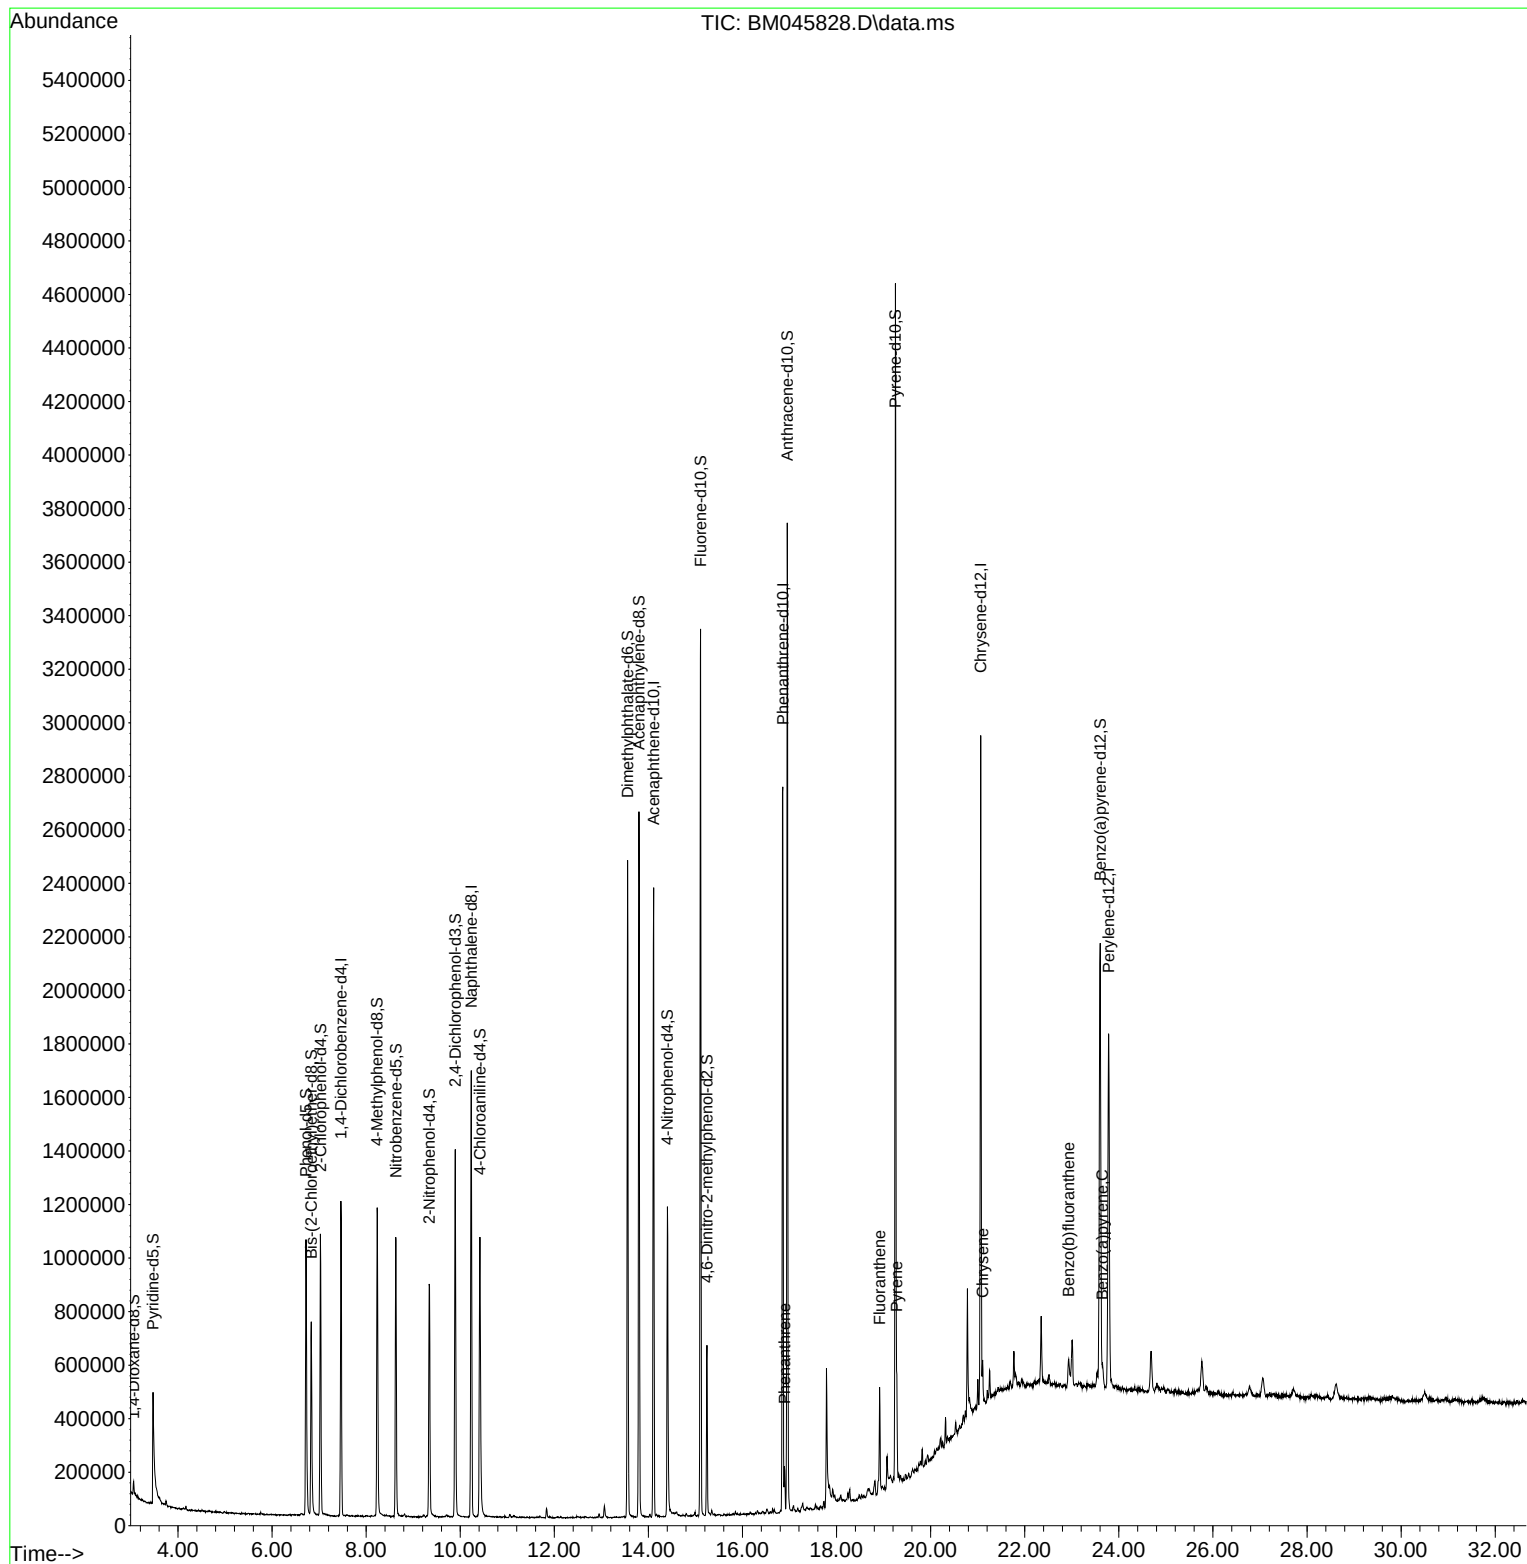

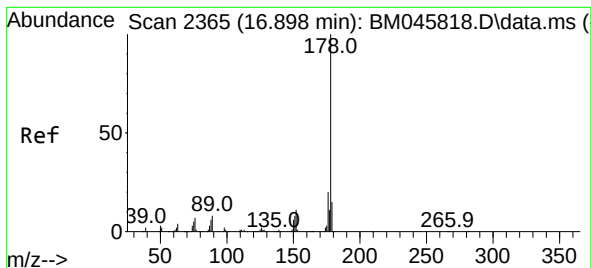

#72

Phenanthrene

Concen: 1.078 ng/ul

RT: 16.892 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM045828.D

Acq: 04 Jun 2024 22:31

Instrument :

BNA_M

ClientSampleId :

BH6D1





Tgt Ion:178 Resp: 84292

Ion Ratio Lower Upper

178 100

179 16.1 12.4 18.6

176 20.0 15.3 22.9

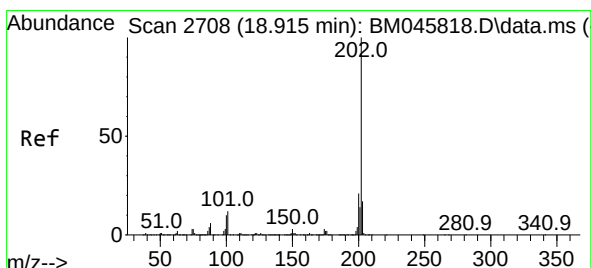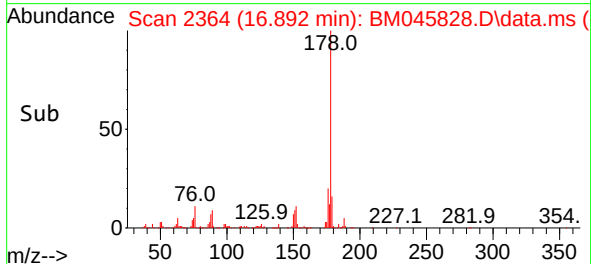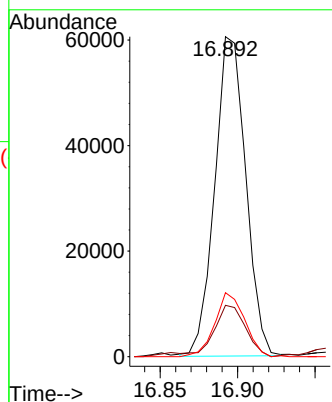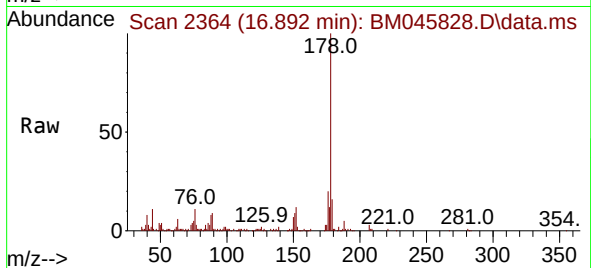

#80

Fluoranthene

Concen: 2.573 ng/ul

RT: 18.916 min Scan# 2708

Delta R.T. -0.006 min

Lab File: BM045828.D

Acq: 04 Jun 2024 22:31




Tgt Ion:202 Resp: 211940


Ion Ratio Lower Upper

202 100

101 10.9 8.9 13.3

100 8.5 6.6 10.0

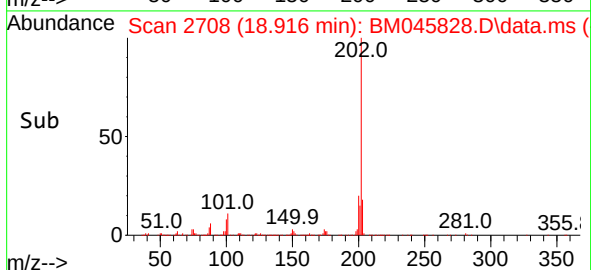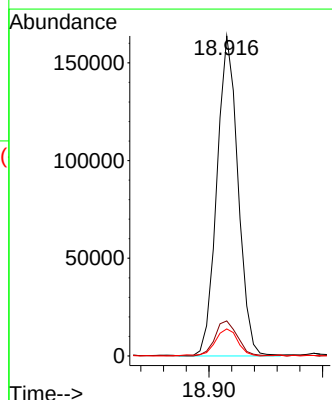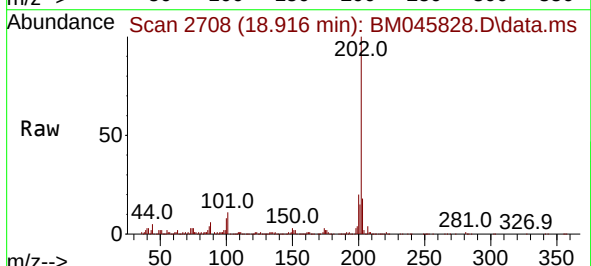

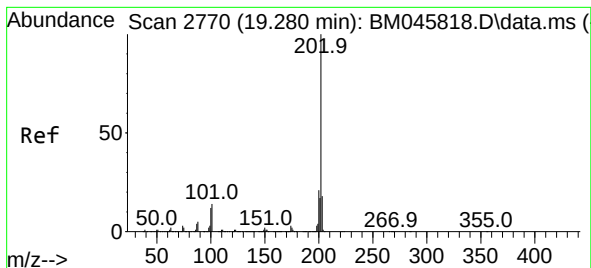

#82

Pyrene

Concen: 2.253 ng/ul

RT: 19.280 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM045828.D

Acq: 04 Jun 2024 22:31

Instrument :

BNA_M

ClientSampleId :

BH6D1





Tgt Ion:202 Resp: 190687

Ion Ratio Lower Upper

202 100

101 13.3 10.5 15.7

100 10.3 8.6 12.8

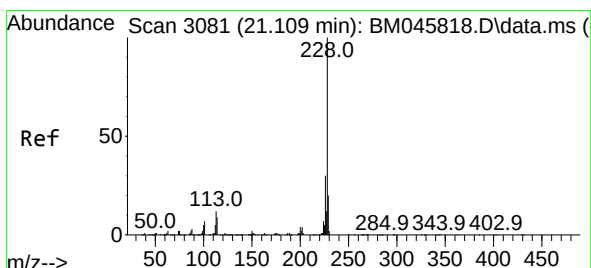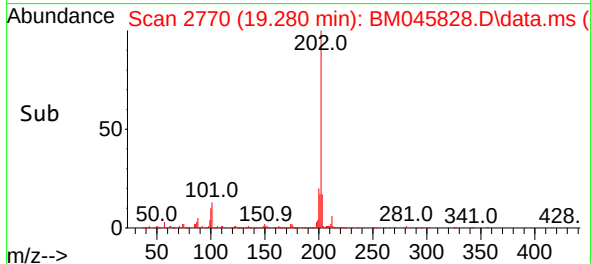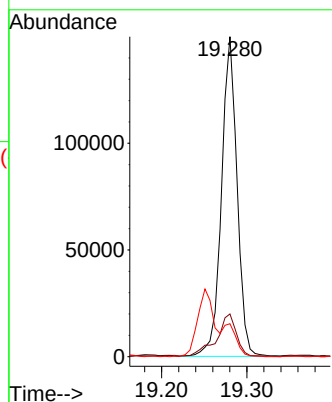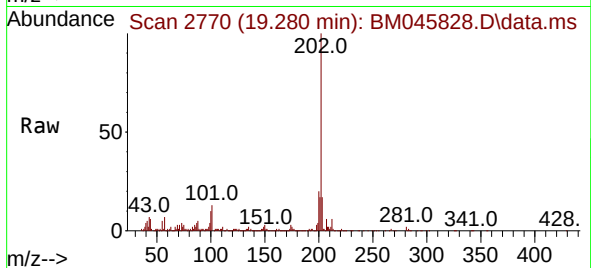

#87

Chrysene

Concen: 1.264 ng/ul

RT: 21.104 min Scan# 3080

Delta R.T. -0.006 min

Lab File: BM045828.D

Acq: 04 Jun 2024 22:31




Tgt Ion:228 Resp: 88178


Ion Ratio Lower Upper

228 100

226 31.1 24.2 36.2

229 22.5 15.2 22.8


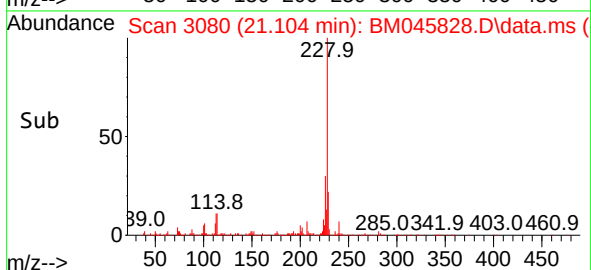
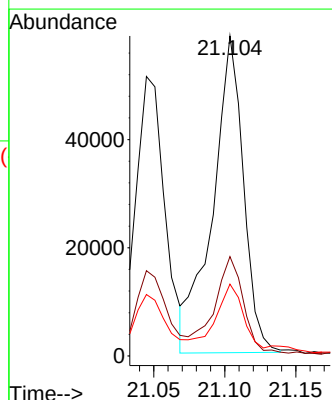
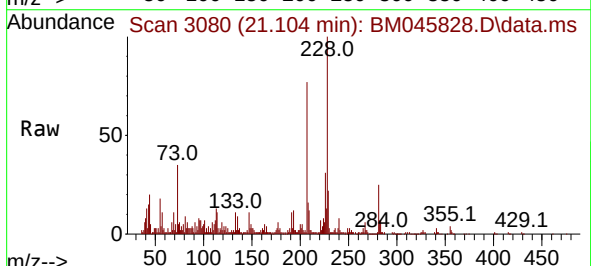


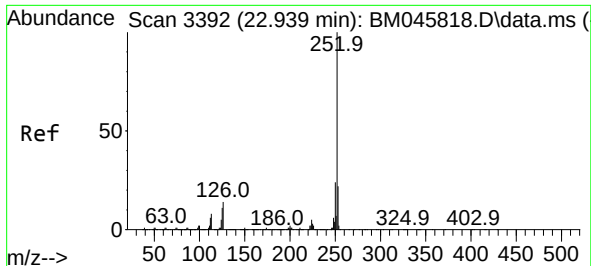

#90
Benzo(b)fluoranthene
Concen: 1.634 ng/u1
RT: 22.933 min Scan# 31
Delta R.T. -0.006 min
Lab File: BM045828.D
Acq: 04 Jun 2024 22:31

Instrument :
BNA_M
ClientSampleId :
BH6D1

Tgt Ion:252 Resp: 95221
Ion Ratio Lower Upper
252 100
253 24.4 17.8 26.6
125 13.3 8.4 12.6#

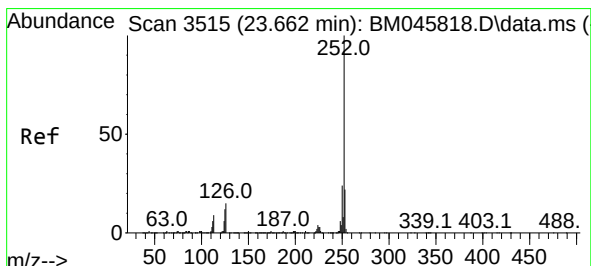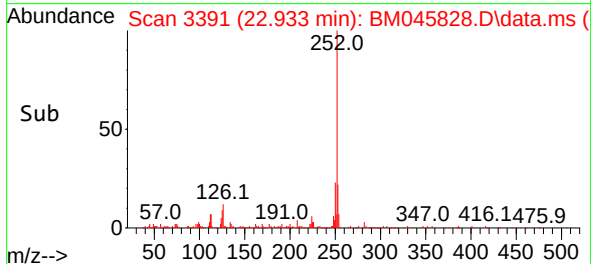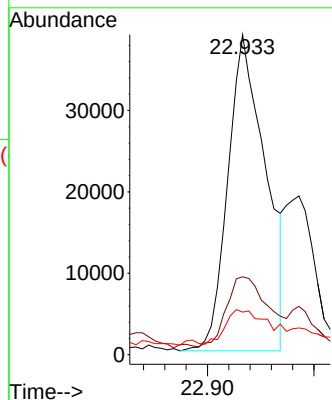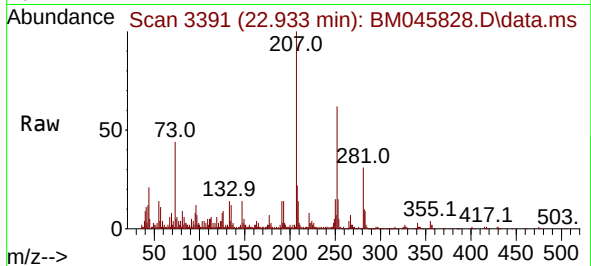

#93
Benzo(a)pyrene
Concen: 1.065 ng/u1
RT: 23.651 min Scan# 3513
Delta R.T. -0.012 min
Lab File: BM045828.D
Acq: 04 Jun 2024 22:31

Tgt Ion:252 Resp: 54500
Ion Ratio Lower Upper
252 100
253 26.3 17.5 26.3#
125 16.7 9.3 13.9#

