

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045852.D
 Acq On : 05 Jun 2024 16:16
 Operator : MA/JU
 Sample : P2586-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4C56

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/06/2024
 Supervised By :mohammad ahmed 06/07/2024

Quant Time: Jun 06 01:59:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 31 13:01:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.463	152	267854	20.000	ng/u1	0.00
20) Naphthalene-d8	10.234	136	1054242	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.104	164	567101	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.851	188	1000525	20.000	ng/u1	0.00
79) Chrysene-d12	21.062	240	815820	20.000	ng/u1	0.00
88) Perylene-d12	23.786	264	929176	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	28080	4.064	ng/uL	0.00
4) Pyridine-d5	3.463	84	346642	19.487	ng/u1	0.00
7) Phenol-d5	6.722	99	567253	24.929	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.828	67	402378	24.626	ng/u1	0.00
11) 2-Chlorophenol-d4	7.028	132	459987	27.062	ng/u1	0.00
15) 4-Methylphenol-d8	8.234	113	412725	24.008	ng/u1	0.00
21) Nitrobenzene-d5	8.628	128	223721	27.142	ng/u1	0.00
24) 2-Nitrophenol-d4	9.339	143	239339	28.690	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.892	165	401871	25.689	ng/u1	0.00
31) 4-Chloroaniline-d4	10.416	131	496755	22.944	ng/u1	0.00
46) Dimethylphthalate-d6	13.557	166	1060389	27.009	ng/u1	0.00
49) Acenaphthylene-d8	13.798	160	1218021	26.717	ng/u1	0.00
54) 4-Nitrophenol-d4	14.410	143	142715	16.844	ng/u1	0.00
60) Fluorene-d10	15.104	176	852271	25.446	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.245	200	77478	15.165	ng/u1	0.00
73) Anthracene-d10	16.951	188	1168105	26.856	ng/u1	0.00
81) Pyrene-d10	19.251	212	1270514	25.042	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.603	264	1155018	26.597	ng/u1	0.00
Target Compounds					Qvalue	
72) Phenanthrene	16.892	178	171786	3.259	ng/u1	99
80) Fluoranthene	18.915	202	336059	5.464	ng/u1	99
82) Pyrene	19.280	202	288646	4.568	ng/u1	99
85) Benzo(a)anthracene	21.045	228	138370	2.456	ng/u1	97
87) Chrysene	21.103	228	148904	2.857	ng/u1	97
90) Benzo(b)fluoranthene	22.933	252	195020	3.415	ng/u1#	95
91) Benzo(k)fluoranthene	22.986	252	59054m	1.059	ng/u1	
93) Benzo(a)pyrene	23.656	252	121864	2.429	ng/u1#	93
94) Indeno(1,2,3-cd)pyrene	26.780	276	89005	1.624	ng/u1	98
96) Benzo(g,h,i)perylene	27.721	276	86006	1.782	ng/u1	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045852.D
 Acq On : 05 Jun 2024 16:16
 Operator : MA/JU
 Sample : P2586-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 A4C56

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 06/06/2024
 Supervised By :mohammad ahmed 06/07/2024


Quant Time: Jun 06 01:59:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 31 13:01:11 2024
 Response via : Initial Calibration

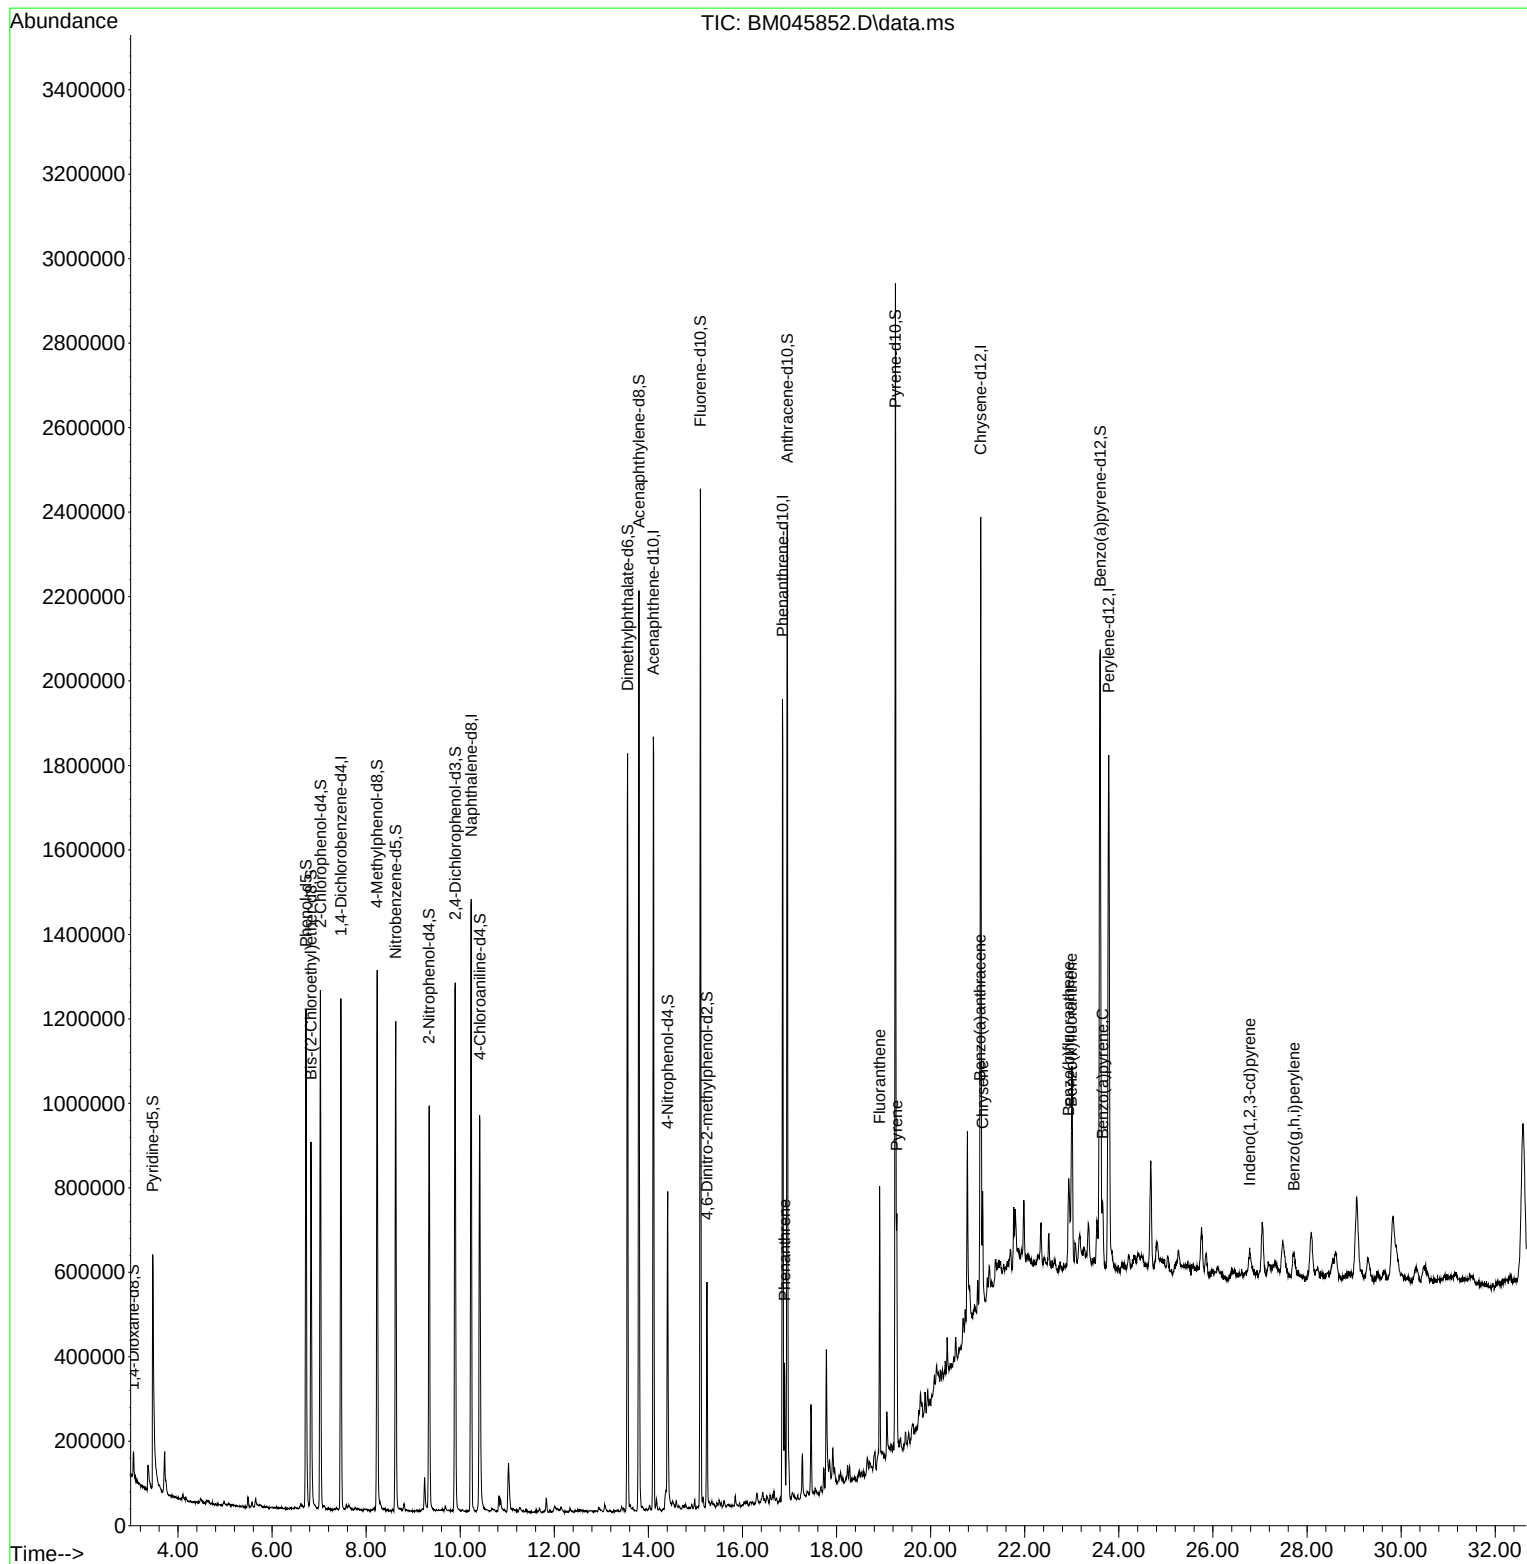



#72
Phenanthrene
Concen: 3.259 ng/ul
RT: 16.892 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM045852.D
Acq: 05 Jun 2024 16:16




Instrument :
BNA_M
ClientSampleId :
A4C56




Tgt Ion:178 Resp: 171780
Ion Ratio Lower Upper
178 100
179 15.7 12.4 18.6
176 20.1 15.3 22.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/06/2024
Supervised By :mohammad ahmed 06/07/2024

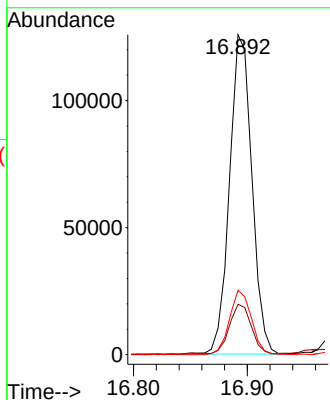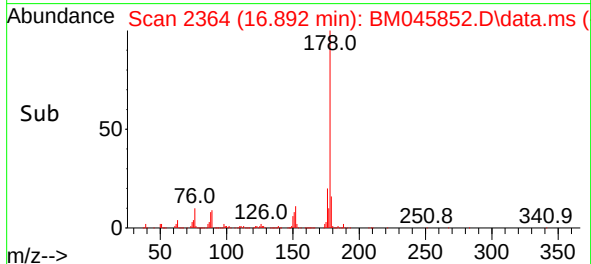


#80
Fluoranthene
Concen: 5.464 ng/ul
RT: 18.915 min Scan# 2708
Delta R.T. -0.006 min
Lab File: BM045852.D
Acq: 05 Jun 2024 16:16

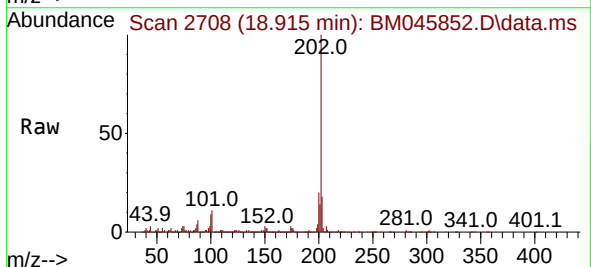

Tgt Ion:202 Resp: 336059
Ion Ratio Lower Upper
202 100
101 10.9 8.9 13.3
100 8.7 6.6 10.0

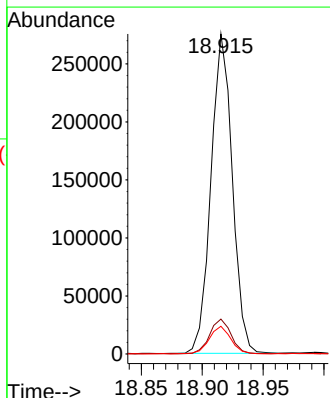



#82

Pyrene

Concen: 4.568 ng/ul

RT: 19.280 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Instrument :

BNA_M

ClientSampleId :

A4C56

Tgt Ion:202 Resp: 288640

Ion Ratio Lower Upper

202 100





101 13.6 10.5 15.7

100 10.9 8.6 12.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 06/06/2024
Supervised By :mohammad ahmed 06/07/2024

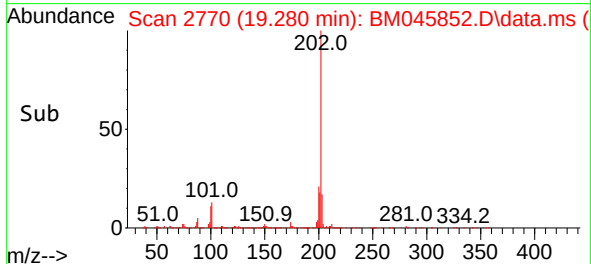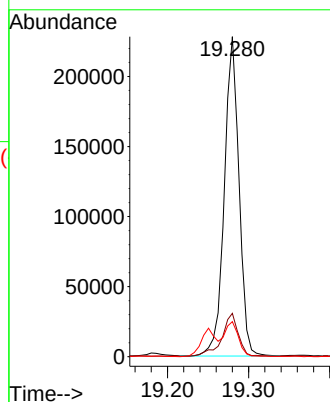

#85

Benzo(a)anthracene

Concen: 2.456 ng/ul

RT: 21.045 min Scan# 3070

Delta R.T. -0.006 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16




Tgt Ion:228 Resp: 138370


Ion Ratio Lower Upper

228 100

229 19.5 15.8 23.8

226 28.9 21.4 32.0

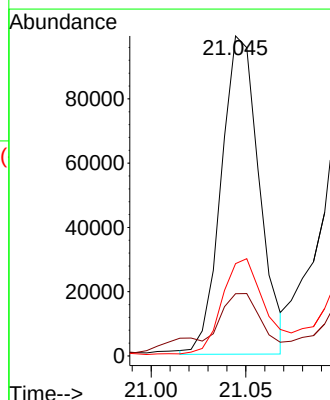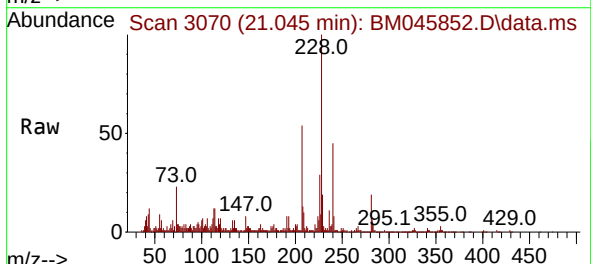



#87

Chrysene

Concen: 2.857 ng/ul

RT: 21.103 min Scan# 3080

Delta R.T. -0.006 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Instrument :

BNA_M

ClientSampleId :





A4C56

Tgt Ion:228	Resp: 148904
Ion Ratio	Lower Upper
228 100	
226 30.4	24.2 36.2
229 21.7	15.2 22.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 06/06/2024
Supervised By :mohammad ahmed 06/07/2024

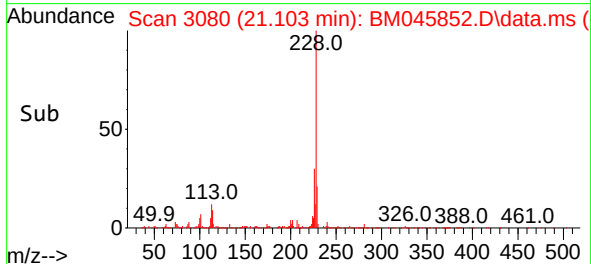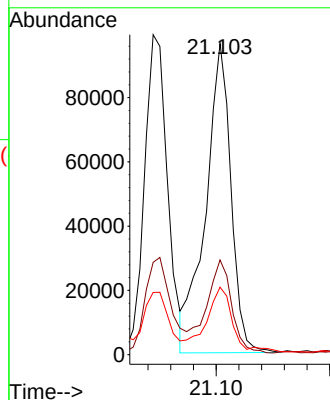

#90

Benzo(b)fluoranthene

Concen: 3.415 ng/ul




RT: 22.933 min Scan# 3391


Delta R.T. -0.006 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Tgt Ion:252	Resp: 195020
Ion Ratio	Lower Upper
252 100	
253 24.5	17.8 26.6
125 12.8	8.4 12.6

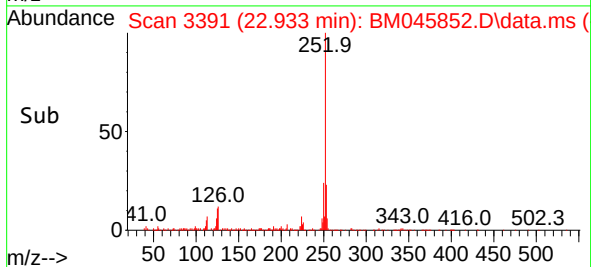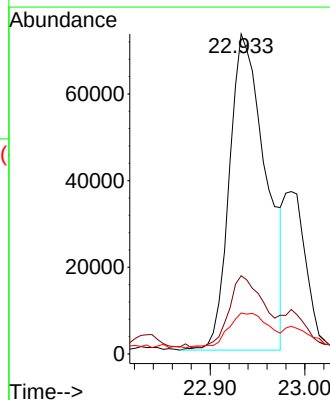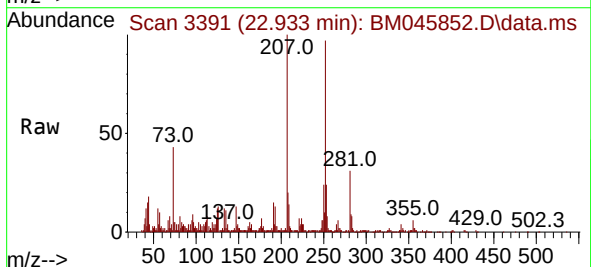



#91

Benzo(k)fluoranthene

Concen: 1.059 ng/ul m

RT: 22.986 min Scan# 3401

Delta R.T. -0.012 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Instrument :

BNA_M

ClientSampleId :





A4C56

Tgt Ion:	252	Resp:	59054
Ion Ratio	Lower	Upper	
252	100		
253	27.4	16.8	25.2
125	17.1	8.2	12.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 06/06/2024
Supervised By :mohammad ahmed 06/07/2024

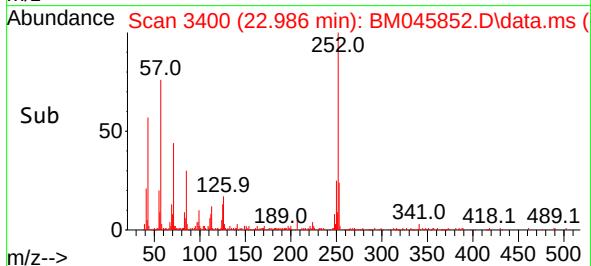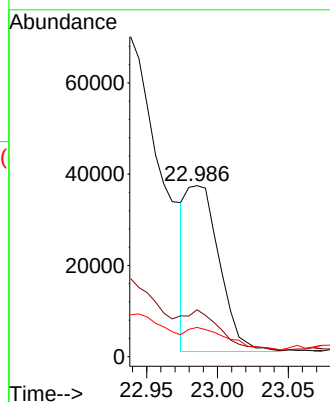

#93

Benzo(a)pyrene

Concen: 2.429 ng/ul




RT: 23.656 min Scan# 3514


Delta R.T. -0.006 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Tgt Ion:	252	Resp:	121864
Ion Ratio	Lower	Upper	
252	100		
253	24.5	17.5	26.3
125	15.1	9.3	13.9

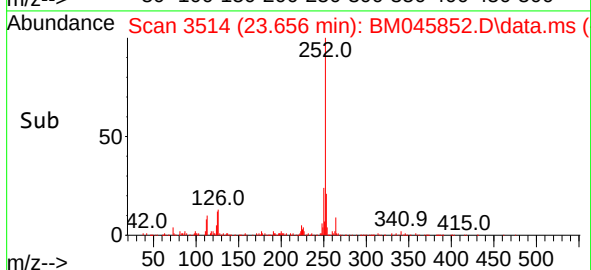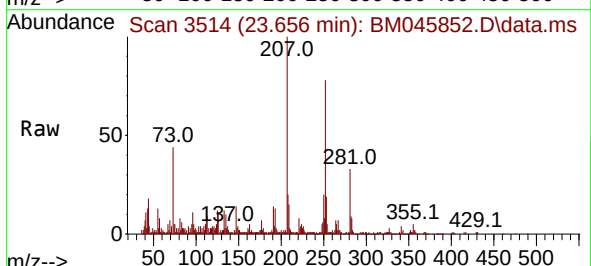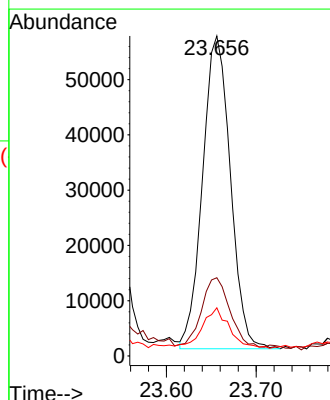



#94

Indeno(1,2,3-cd)pyrene

Concen: 1.624 ng/ul

RT: 26.780 min Scan# 4047

Delta R.T. -0.012 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Instrument :

BNA_M

ClientSampleId :





A4C56

Tgt Ion:	276	Resp:	8900
Ion Ratio	Lower	Upper	
276	100		
138	21.1	17.9	26.9
277	23.6	19.0	28.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 06/06/2024
Supervised By :mohammad ahmed 06/07/2024

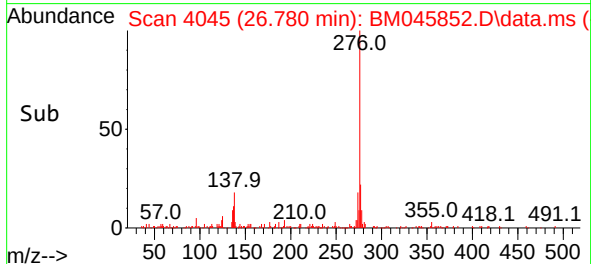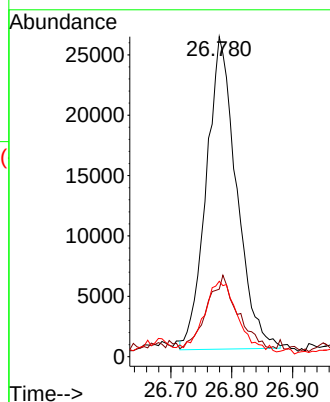

#96

Benzo(g,h,i)perylene

Concen: 1.782 ng/ul

RT: 27.721 min Scan# 4205

Delta R.T. -0.006 min

Lab File: BM045852.D

Acq: 05 Jun 2024 16:16

Tgt Ion:	276	Resp:	8600
Ion Ratio	Lower	Upper	
276	100		
138	25.5	18.6	27.8
277	21.8	18.7	28.1

