

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045819.D
 Acq On : 04 Jun 2024 16:33
 Operator : MA/JU
 Sample : PB161139BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK139

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	8	11	29	rVB	82614	161479	2.59%	0.216%
2	3.463	79	81	103	rBV	632600	1554589	24.91%	2.080%
3	4.169	198	201	206	rVB2	31505	42939	0.69%	0.057%
4	6.616	613	617	620	rBV6	6170	10277	0.16%	0.014%
5	6.716	628	634	648	rBV	1260237	2182655	34.97%	2.921%
6	6.834	648	654	670	rVV	962743	1687586	27.04%	2.258%
7	7.028	680	687	698	rBV	1378822	2122608	34.01%	2.840%
8	7.463	755	761	772	rBV	1267016	1972952	31.61%	2.640%
9	8.234	884	892	907	rBV	1584470	2543212	40.75%	3.403%
10	8.628	951	959	972	rBV	1392397	2282645	36.57%	3.055%
11	9.245	1059	1064	1071	rBV8	5444	11503	0.18%	0.015%
12	9.345	1073	1081	1094	rBV	1077827	1814535	29.07%	2.428%
13	9.892	1167	1174	1187	rBV	1479608	2525638	40.46%	3.380%
14	10.233	1225	1232	1242	rBV	1770454	2771595	44.40%	3.709%
15	10.416	1256	1263	1287	rBV	1282314	2711946	43.45%	3.629%
16	11.839	1499	1505	1511	rBV3	27408	45292	0.73%	0.061%
17	12.904	1681	1686	1692	rBV10	3904	8415	0.13%	0.011%
18	13.069	1708	1714	1722	rBV2	15259	35224	0.56%	0.047%
19	13.563	1791	1798	1809	rBV	2624053	3986435	63.87%	5.334%
20	13.798	1831	1838	1848	rBV2	3121376	4395384	70.42%	5.882%
21	14.110	1884	1891	1899	rBV	2614379	3650360	58.48%	4.885%
22	14.404	1932	1941	1953	rBV	1226027	2000752	32.05%	2.677%
23	15.110	2054	2061	2070	rBV	3770481	5315891	85.17%	7.113%
24	15.245	2077	2084	2098	rBV	1207496	1622542	25.99%	2.171%
25	15.345	2098	2101	2106	rVB5	15555	25858	0.41%	0.035%
26	16.645	2319	2322	2325	rBV4	7680	9222	0.15%	0.012%
27	16.857	2351	2358	2368	rBV	3083968	4244077	67.99%	5.679%
28	16.951	2368	2374	2387	rBV	4052041	5718730	91.62%	7.653%
29	17.257	2423	2426	2431	rVB5	4912	6860	0.11%	0.009%
30	17.615	2482	2487	2491	rBV8	4713	7674	0.12%	0.010%
31	17.851	2525	2527	2531	rBV5	5125	7255	0.12%	0.010%
32	18.521	2636	2641	2642	rBV5	4300	7633	0.12%	0.010%
33	18.815	2687	2691	2697	rVB4	45464	61929	0.99%	0.083%
34	18.886	2699	2703	2709	rBV	48720	61264	0.98%	0.082%
35	19.251	2759	2765	2775	rVB	4933953	6241751	100.00%	8.352%
36	21.068	3068	3074	3084	rBV	3038491	3998405	64.06%	5.350%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045819.D
Acq On : 04 Jun 2024 16:33
Operator : MA/JU
Sample : PB161139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK139

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	23.603	3497	3505	3519	rBV2	2279066	4944758	79.22%	6.617%
38	23.786	3528	3536	3548	rVB	1775434	3937972	63.09%	5.270%




Sum of corrected areas: 74729842

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045819.D
Acq On : 04 Jun 2024 16:33
Operator : MA/JU
Sample : PB161139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK139

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

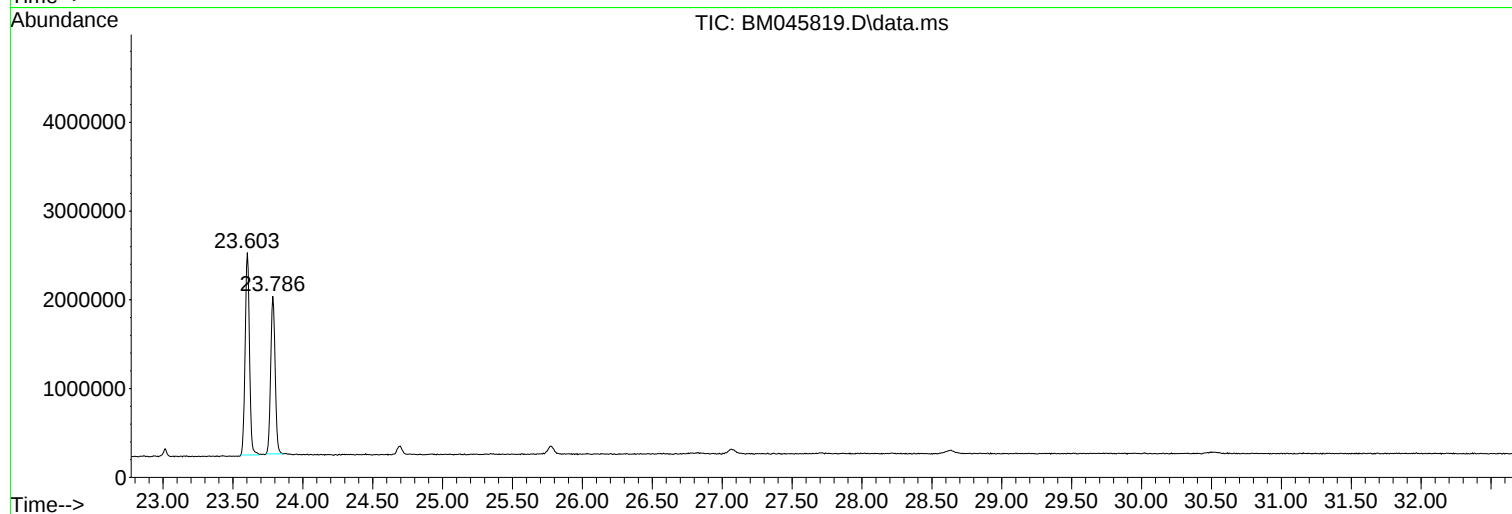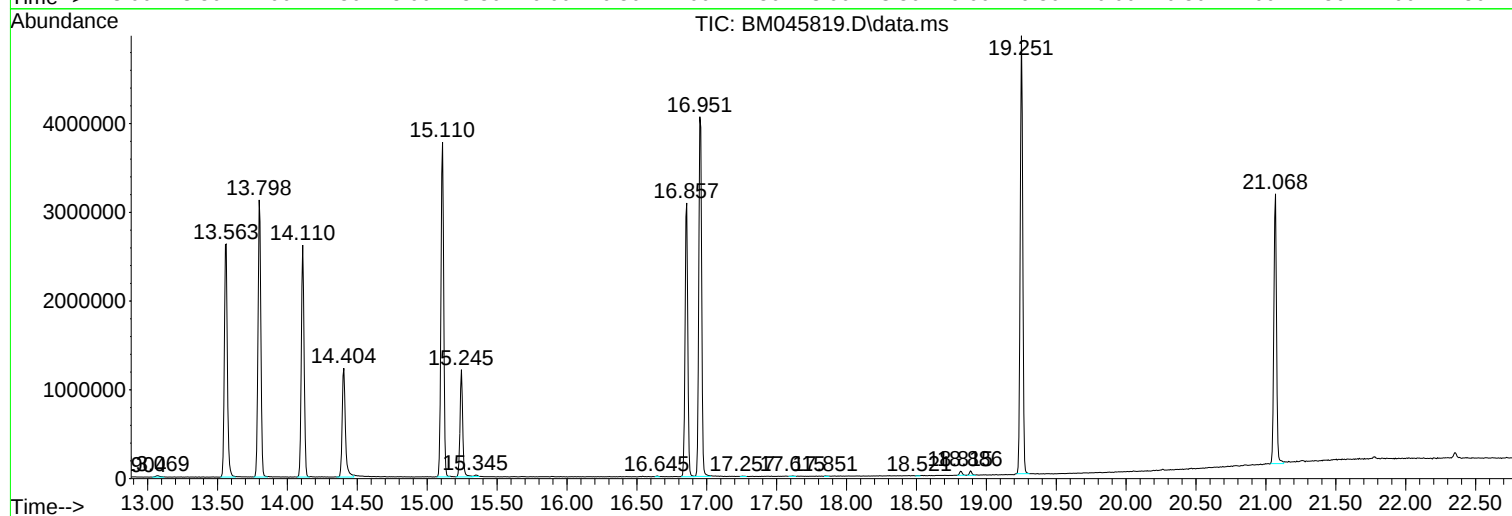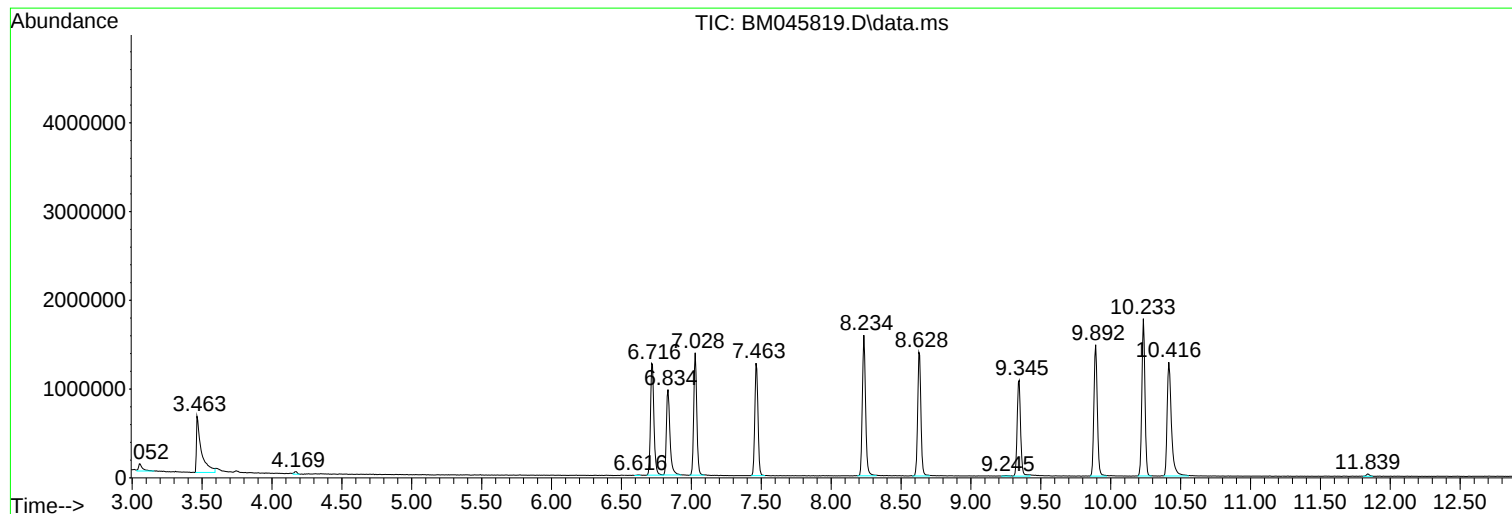

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045819.D
Acq On : 04 Jun 2024 16:33
Operator : MA/JU
Sample : PB161139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK139

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045819.D
Acq On : 04 Jun 2024 16:33
Operator : MA/JU
Sample : PB161139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK139

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------