

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045822.D
 Acq On : 04 Jun 2024 18:33
 Operator : MA/JU
 Sample : P2589-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	9	12	21	rVB2	44088	74681	1.40%	0.122%
2	3.475	81	83	105	rBV	304846	835897	15.67%	1.366%
3	4.169	199	201	207	rVB5	17981	25039	0.47%	0.041%
4	6.628	614	619	622	rBV6	6071	11285	0.21%	0.018%
5	6.722	628	635	648	rBV	856808	1526809	28.62%	2.496%
6	6.834	648	654	670	rVB	630960	1128240	21.15%	1.844%
7	7.028	681	687	697	rBV	913312	1432826	26.86%	2.342%
8	7.463	755	761	772	rBV	1145309	1813803	34.00%	2.965%
9	8.234	885	892	906	rBV	988562	1678890	31.47%	2.744%
10	8.634	952	960	969	rBV	920771	1515940	28.42%	2.478%
11	8.828	989	993	994	rBV3	6129	5448	0.10%	0.009%
12	9.245	1057	1064	1067	rBV7	6119	11918	0.22%	0.019%
13	9.345	1072	1081	1090	rBV	731554	1200123	22.50%	1.962%
14	9.892	1167	1174	1186	rBV	1043793	1777126	33.32%	2.905%
15	10.234	1225	1232	1244	rBV	1614599	2572543	48.23%	4.205%
16	10.422	1254	1264	1286	rBV	817765	1736482	32.55%	2.838%
17	11.069	1368	1374	1377	rBV4	15141	31701	0.59%	0.052%
18	11.145	1383	1387	1390	rBV6	5259	7042	0.13%	0.012%
19	11.286	1408	1411	1418	rVB8	2673	5843	0.11%	0.010%
20	11.451	1435	1439	1444	rBV6	3492	5757	0.11%	0.009%
21	11.704	1478	1482	1489	rVB7	5361	7749	0.15%	0.013%
22	11.839	1501	1505	1513	rVB4	22661	42669	0.80%	0.070%
23	12.133	1552	1555	1561	rVB8	4325	6578	0.12%	0.011%
24	12.957	1691	1695	1699	rVB3	9965	14484	0.27%	0.024%
25	13.069	1709	1714	1724	rBV3	26851	57602	1.08%	0.094%
26	13.433	1772	1776	1779	rVB5	5354	7207	0.14%	0.012%
27	13.486	1779	1785	1788	rBV8	4879	9401	0.18%	0.015%
28	13.563	1791	1798	1807	rVV	1835882	2645314	49.59%	4.324%
29	13.657	1811	1814	1819	rVB7	6432	10227	0.19%	0.017%
30	13.798	1831	1838	1849	rBV	2117383	3051358	57.20%	4.988%
31	14.039	1875	1879	1884	rBV6	8372	13340	0.25%	0.022%
32	14.110	1884	1891	1899	rVV	2418235	3270469	61.31%	5.346%
33	14.175	1899	1902	1906	rVB5	8216	10606	0.20%	0.017%
34	14.404	1935	1941	1956	rBV	818689	1289630	24.18%	2.108%
35	14.510	1956	1959	1962	rVV5	11698	22025	0.41%	0.036%
36	14.569	1966	1969	1971	rVV4	9274	12218	0.23%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045822.D
 Acq On : 04 Jun 2024 18:33
 Operator : MA/JU
 Sample : P2589-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6C5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

37	14.592	1971	1973	1981	rVV8	9838	20050	0.38%	0.033%
38	14.969	2034	2037	2038	rBV2	7389	7331	0.14%	0.012%
39	14.992	2038	2041	2045	rVB5	14731	17060	0.32%	0.028%
40	15.110	2054	2061	2068	rBV	2635171	3682703	69.04%	6.020%
41	15.163	2068	2070	2076	rVB5	12179	11969	0.22%	0.020%
42	15.245	2078	2084	2093	rBV	814798	1059562	19.86%	1.732%
43	15.351	2099	2102	2109	rVB6	11873	16895	0.32%	0.028%
44	15.851	2183	2187	2190	rBV4	13565	17061	0.32%	0.028%
45	15.892	2192	2194	2197	rVB3	7894	6551	0.12%	0.011%
46	16.169	2239	2241	2244	rVV4	6026	6240	0.12%	0.010%
47	16.321	2262	2267	2272	rBV7	12418	20753	0.39%	0.034%
48	16.445	2283	2288	2290	rBV6	7010	9554	0.18%	0.016%
49	16.521	2297	2301	2309	rVB6	13378	25897	0.49%	0.042%
50	16.639	2318	2321	2325	rBV4	14487	19220	0.36%	0.031%
51	16.674	2325	2327	2331	rVB3	8133	8119	0.15%	0.013%
52	16.810	2346	2350	2352	rBV4	13857	17787	0.33%	0.029%
53	16.857	2352	2358	2362	rVV	2682397	3746921	70.24%	6.125%
54	16.892	2362	2364	2369	rVV	185976	235404	4.41%	0.385%
55	16.951	2369	2374	2386	rVB2	2682226	3917631	73.44%	6.404%
56	17.086	2394	2397	2401	rVB6	15404	20312	0.38%	0.033%
57	17.180	2409	2413	2417	rBV6	10932	14209	0.27%	0.023%
58	17.280	2423	2430	2434	rBV4	24713	47402	0.89%	0.077%
59	17.380	2443	2447	2450	rBV6	11966	15119	0.28%	0.025%
60	17.551	2474	2476	2488	rVB6	15194	26865	0.50%	0.044%
61	17.668	2492	2496	2501	rBV7	14231	25184	0.47%	0.041%
62	17.733	2503	2507	2511	rVV	39276	53371	1.00%	0.087%
63	17.786	2511	2516	2524	rVV2	210031	369871	6.93%	0.605%
64	17.851	2524	2527	2534	rVV3	42486	90449	1.70%	0.148%
65	17.915	2534	2538	2543	rVV2	56727	106887	2.00%	0.175%
66	17.957	2543	2545	2551	rVB	30334	43669	0.82%	0.071%
67	18.239	2589	2593	2596	rBV	32970	41106	0.77%	0.067%
68	18.280	2597	2600	2606	rVB5	28289	37588	0.70%	0.061%
69	18.480	2632	2634	2640	rVB6	16174	21535	0.40%	0.035%
70	18.533	2640	2643	2646	rBV3	17234	23737	0.44%	0.039%
71	18.651	2660	2663	2669	rBV5	34814	71087	1.33%	0.116%
72	18.704	2669	2672	2677	rVB6	24006	40234	0.75%	0.066%
73	18.815	2684	2691	2696	rBV4	48701	96405	1.81%	0.158%
74	18.886	2700	2703	2704	rBV	42020	41101	0.77%	0.067%
75	18.915	2704	2708	2715	rVB	475707	620946	11.64%	1.015%
76	19.074	2731	2735	2738	rBV3	37261	46912	0.88%	0.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045822.D
 Acq On : 04 Jun 2024 18:33
 Operator : MA/JU
 Sample : P2589-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

77	19.209	2755	2758	2759	rBV3	17741	18386	0.34%	0.030%
78	19.251	2759	2765	2775	rVV2	3665521	5334282	100.00%	8.719%
79	19.462	2799	2801	2808	rVB2	23342	31217	0.59%	0.051%
80	19.615	2822	2827	2834	rBV4	37784	91428	1.71%	0.149%
81	19.745	2846	2849	2852	rBV4	30139	50602	0.95%	0.083%
82	19.780	2853	2855	2859	rVV2	48297	58053	1.09%	0.095%
83	19.821	2859	2862	2866	rVB	48070	50973	0.96%	0.083%
84	19.880	2870	2872	2876	rBV2	26382	30608	0.57%	0.050%
85	19.939	2878	2882	2887	rVV2	50930	72334	1.36%	0.118%
86	20.315	2944	2946	2950	rBV2	57134	61253	1.15%	0.100%
87	20.533	2980	2983	2988	rBV2	45939	63401	1.19%	0.104%
88	20.786	3021	3026	3032	rBV3	265800	471804	8.84%	0.771%
89	21.003	3060	3063	3067	rBV	99971	133977	2.51%	0.219%
90	21.062	3067	3073	3078	rVV	2737610	4064556	76.20%	6.644%
91	21.103	3078	3080	3087	rVB	220396	281228	5.27%	0.460%
92	22.350	3288	3292	3299	rVB2	225445	360688	6.76%	0.590%
93	22.933	3387	3391	3398	rBV	118179	313072	5.87%	0.512%
94	23.603	3497	3505	3512	rBV2	1635265	3505121	65.71%	5.729%
95	23.786	3528	3536	3554	rVB	1561998	3615963	67.79%	5.911%


Sum of corrected areas: 61177913

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045822.D
Acq On : 04 Jun 2024 18:33
Operator : MA/JU
Sample : P2589-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

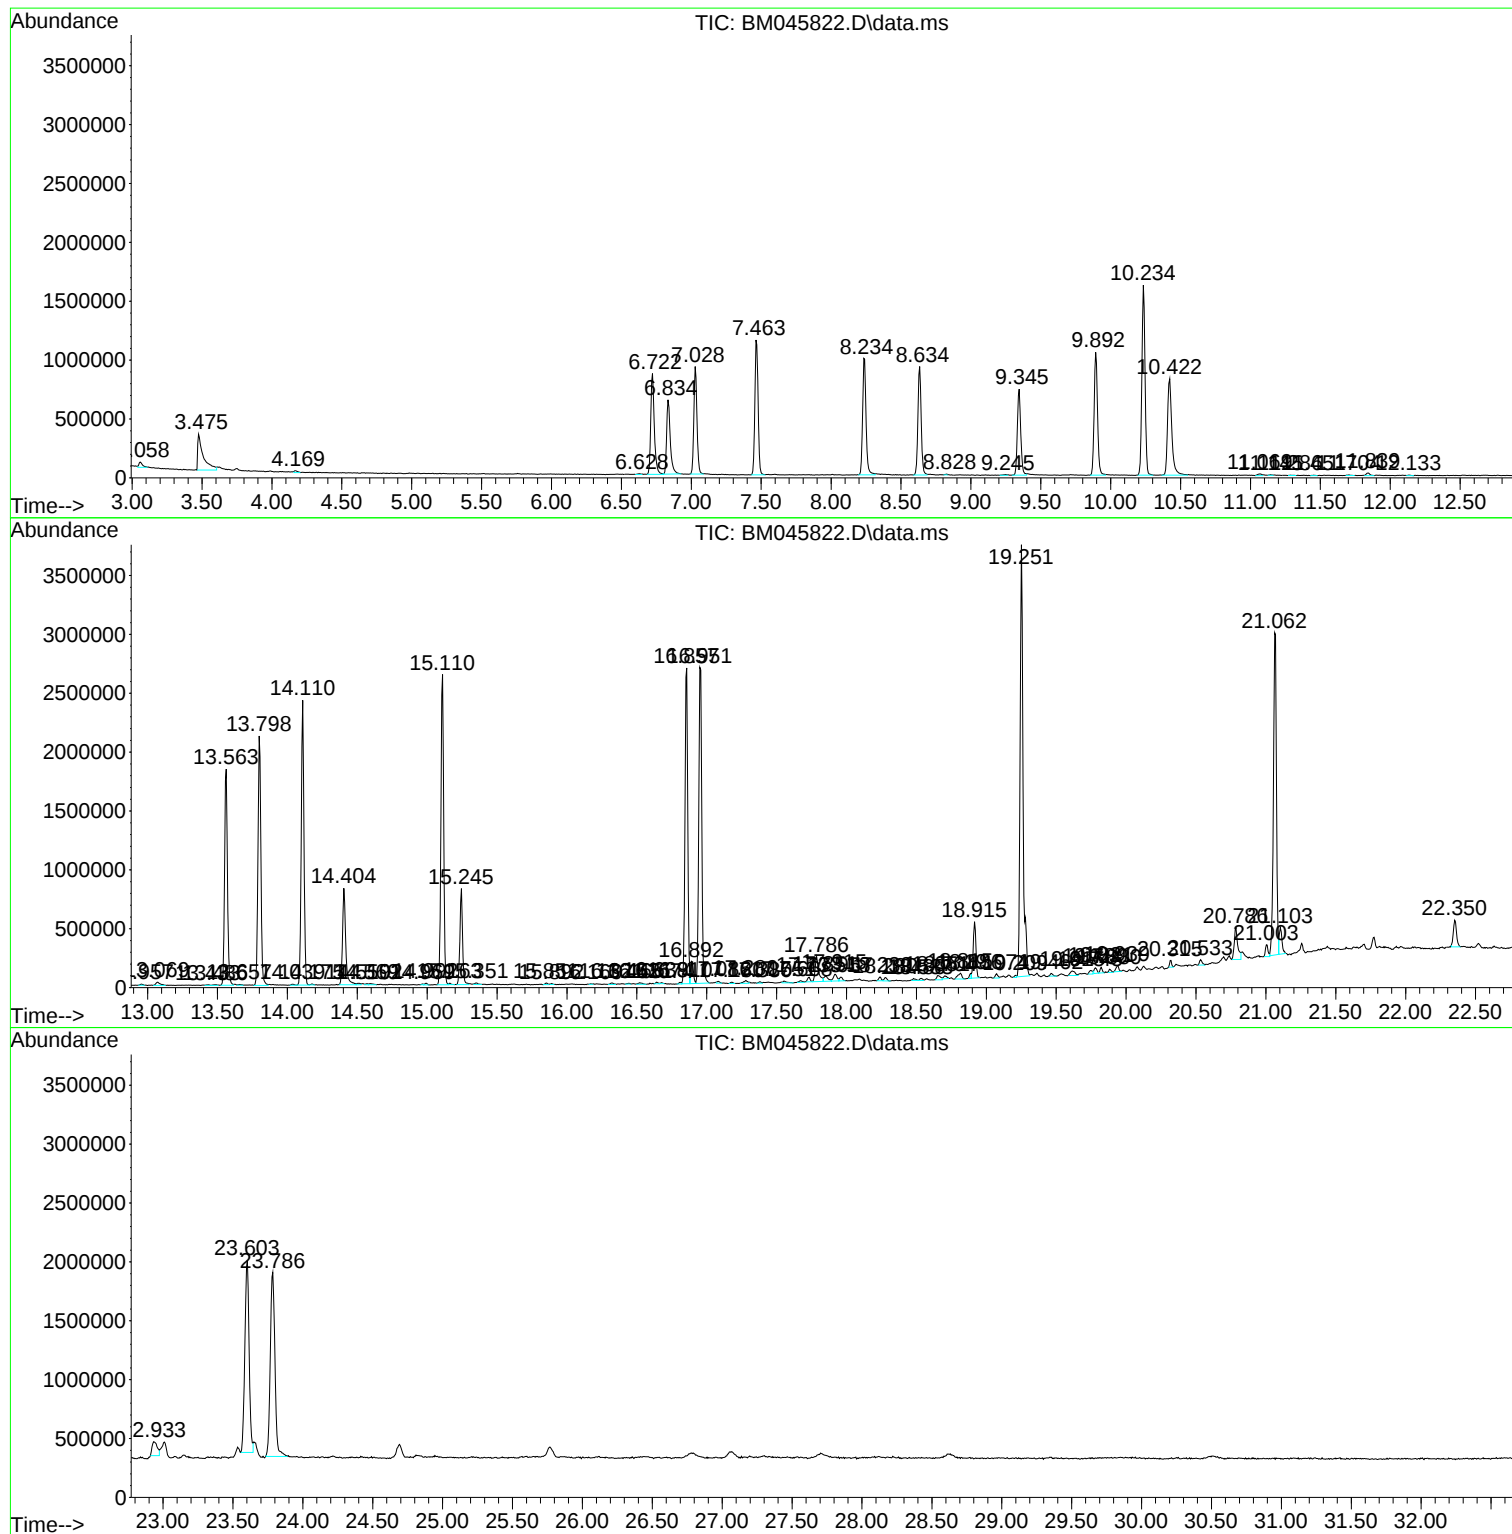

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045822.D
Acq On : 04 Jun 2024 18:33
Operator : MA/JU
Sample : P2589-11
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
BH6C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
20.786	2.32 ng/ul	471804	Chrysene-d12			21.068
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-		280	C20H40	074685-30-6	98
2	3-Eicosene, (E)-		280	C20H40	074685-33-9	96
3	9-Eicosene, (E)-		280	C20H40	074685-29-3	90
4	Oxalic acid, allyl octadecyl ester		382	C23H42O4	1000309-24-5	87
5	Hexacosyl heptafluorobutyrate		578	C30H53F7O2	1000351-83-3	83

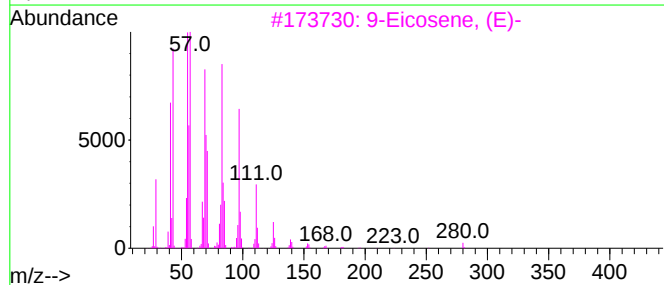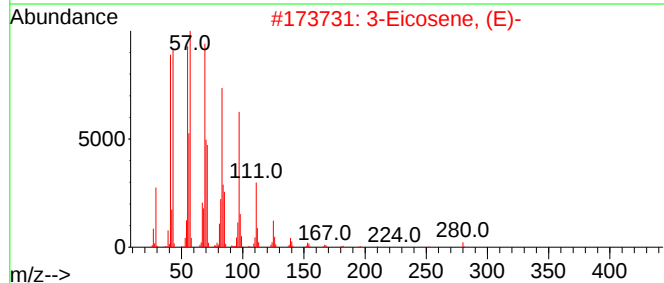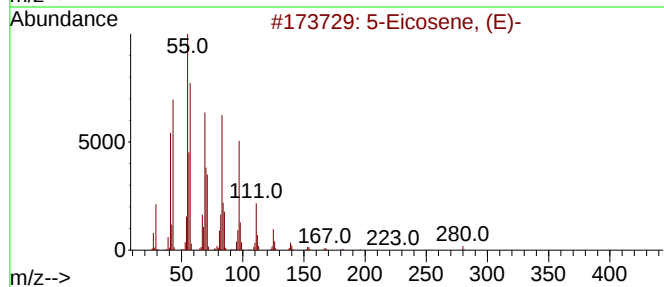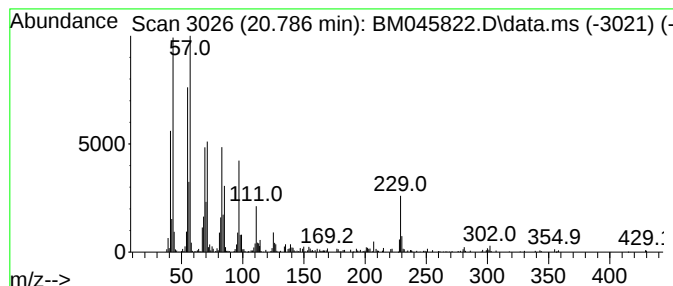

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045822.D
Acq On : 04 Jun 2024 18:33
Operator : MA/JU
Sample : P2589-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.786	2.3	ng/u1	471804	5	21.068	4064560	20.0