

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045823.D
 Acq On : 04 Jun 2024 19:12
 Operator : MA/JU
 Sample : P2589-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	10	12	21	rVB2	29258	45455	1.26%	0.100%
2	3.481	81	84	101	rBV	161137	449260	12.43%	0.993%
3	3.746	127	129	137	rVB3	19862	27469	0.76%	0.061%
4	3.987	168	170	173	rVB4	8966	8494	0.24%	0.019%
5	4.652	279	283	286	rBV5	4667	6143	0.17%	0.014%
6	5.705	461	462	465	rBV3	4225	4318	0.12%	0.010%
7	6.622	613	618	620	rBV5	5049	7060	0.20%	0.016%
8	6.722	629	635	649	rVV	553137	1001464	27.71%	2.213%
9	6.834	649	654	667	rVV	393709	733563	20.30%	1.621%
10	7.028	681	687	699	rBV	592851	945422	26.16%	2.089%
11	7.469	753	762	771	rBV	1043330	1663231	46.02%	3.675%
12	8.240	886	893	908	rBV	645162	1097316	30.36%	2.425%
13	8.634	953	960	968	rBV	630192	1008142	27.89%	2.228%
14	8.828	988	993	1000	rVB10	9830	18701	0.52%	0.041%
15	9.093	1035	1038	1042	rBV5	4519	4764	0.13%	0.011%
16	9.252	1062	1065	1068	rBV5	5043	7266	0.20%	0.016%
17	9.346	1074	1081	1096	rBV	478408	799944	22.13%	1.768%
18	9.710	1141	1143	1145	rBV3	5044	4922	0.14%	0.011%
19	9.893	1167	1174	1189	rBV	700013	1197981	33.14%	2.647%
20	10.175	1219	1222	1224	rBV4	3743	5204	0.14%	0.011%
21	10.234	1224	1232	1245	rVV	1408166	2337312	64.67%	5.165%
22	10.340	1248	1250	1254	rBV4	3424	4933	0.14%	0.011%
23	10.422	1254	1264	1281	rBV	531558	1163764	32.20%	2.571%
24	11.063	1370	1373	1382	rVV8	9565	23155	0.64%	0.051%
25	11.140	1382	1386	1388	rVV5	3533	6418	0.18%	0.014%
26	11.698	1477	1481	1483	rBV5	4126	6073	0.17%	0.013%
27	11.763	1489	1492	1495	rVB4	2786	4217	0.12%	0.009%
28	11.798	1495	1498	1500	rBV4	3021	4332	0.12%	0.010%
29	11.840	1500	1505	1513	rVV6	16078	33688	0.93%	0.074%
30	11.910	1516	1517	1526	rVB9	3610	6768	0.19%	0.015%
31	12.140	1551	1556	1558	rVV5	4610	6572	0.18%	0.015%
32	12.181	1558	1563	1566	rVB7	4168	6895	0.19%	0.015%
33	12.522	1618	1621	1626	rVB5	2781	5083	0.14%	0.011%
34	12.669	1641	1646	1647	rBV4	4242	6539	0.18%	0.014%
35	12.957	1691	1695	1698	rBV4	6747	9857	0.27%	0.022%
36	13.075	1708	1715	1724	rBV2	33393	75732	2.10%	0.167%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045823.D
 Acq On : 04 Jun 2024 19:12
 Operator : MA/JU
 Sample : P2589-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

37	13.392	1765	1769	1771	rBV5	4517	5032	0.14%	0.011%
38	13.475	1781	1783	1788	rVB5	4048	6252	0.17%	0.014%
39	13.563	1791	1798	1811	rVV	1317132	1829757	50.62%	4.043%
40	13.739	1823	1828	1830	rBV6	2897	5828	0.16%	0.013%

41	13.798	1832	1838	1850	rVV2	1385386	2079553	57.54%	4.595%
42	14.039	1875	1879	1883	rVB6	6443	8833	0.24%	0.020%
43	14.110	1884	1891	1899	rVV	2018912	2927766	81.00%	6.469%
44	14.181	1899	1903	1906	rVV5	5023	8562	0.24%	0.019%
45	14.275	1917	1919	1926	rVB8	3249	4444	0.12%	0.010%

46	14.404	1934	1941	1957	rBV	525342	872587	24.14%	1.928%
47	14.598	1972	1974	1977	rVB3	5072	5826	0.16%	0.013%
48	14.734	1995	1997	2002	rBV6	3244	4753	0.13%	0.011%
49	14.969	2033	2037	2039	rBV5	5387	6210	0.17%	0.014%
50	14.992	2039	2041	2045	rVB5	7979	10286	0.28%	0.023%

51	15.110	2054	2061	2069	rBV	1825650	2569031	71.08%	5.677%
52	15.245	2078	2084	2095	rBV	522077	713650	19.74%	1.577%
53	15.322	2095	2097	2100	rVV4	6128	9095	0.25%	0.020%
54	15.351	2100	2102	2106	rVB5	7365	7362	0.20%	0.016%
55	15.510	2125	2129	2132	rVB6	4656	6469	0.18%	0.014%

56	15.545	2132	2135	2136	rBV3	4852	4143	0.11%	0.009%
57	15.604	2142	2145	2149	rBV6	3227	6472	0.18%	0.014%
58	15.675	2156	2157	2161	rBV4	3829	5369	0.15%	0.012%
59	15.857	2185	2188	2190	rBV3	7328	8037	0.22%	0.018%
60	15.892	2192	2194	2197	rVB4	5300	5068	0.14%	0.011%

61	16.033	2214	2218	2222	rVV6	4906	6993	0.19%	0.015%
62	16.322	2260	2267	2273	rBV7	14915	30488	0.84%	0.067%
63	16.522	2298	2301	2305	rBV6	5146	8433	0.23%	0.019%
64	16.645	2318	2322	2326	rBV6	12509	17056	0.47%	0.038%
65	16.810	2347	2350	2352	rBV3	11180	11925	0.33%	0.026%

66	16.857	2352	2358	2363	rVV	2492333	3378002	93.46%	7.464%
67	16.892	2363	2364	2368	rVV	80884	83897	2.32%	0.185%
68	16.951	2368	2374	2386	rVB	2012636	2723991	75.37%	6.019%
69	17.086	2393	2397	2402	rVB8	13065	20954	0.58%	0.046%
70	17.180	2410	2413	2418	rVB6	10085	12335	0.34%	0.027%

71	17.257	2422	2426	2427	rBV4	4427	6208	0.17%	0.014%
72	17.280	2427	2430	2437	rVB6	13342	26307	0.73%	0.058%
73	17.375	2444	2446	2449	rBV4	7284	8123	0.22%	0.018%
74	17.410	2449	2452	2454	rBV4	3884	4482	0.12%	0.010%
75	17.557	2473	2477	2481	rBV7	11957	19707	0.55%	0.044%

76	17.663	2491	2495	2502	rBV7	13642	29447	0.81%	0.065%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045823.D
 Acq On : 04 Jun 2024 19:12
 Operator : MA/JU
 Sample : P2589-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

77	17.727	2502	2506	2510	rBV3	23930	36700	1.02%	0.081%
78	17.786	2511	2516	2524	rBV2	191055	332330	9.19%	0.734%
79	17.916	2534	2538	2543	rBV5	24721	41719	1.15%	0.092%
80	17.957	2543	2545	2551	rVB4	18814	28165	0.78%	0.062%
81	18.004	2551	2553	2555	rBV3	4402	4370	0.12%	0.010%
82	18.092	2565	2568	2572	rVB6	11863	15328	0.42%	0.034%
83	18.239	2590	2593	2597	rBV4	15827	18819	0.52%	0.042%
84	18.280	2597	2600	2605	rVB7	13159	17745	0.49%	0.039%
85	18.486	2631	2635	2639	rBV6	11741	15478	0.43%	0.034%
86	18.539	2641	2644	2648	rBV4	10894	16656	0.46%	0.037%
87	18.574	2648	2650	2652	rBV2	7622	8300	0.23%	0.018%
88	18.657	2660	2664	2668	rBV4	26700	43763	1.21%	0.097%
89	18.816	2685	2691	2697	rVB6	31892	58220	1.61%	0.129%
90	18.886	2699	2703	2705	rBV2	30697	42994	1.19%	0.095%
91	18.916	2705	2708	2715	rVB	200200	253328	7.01%	0.560%
92	19.074	2731	2735	2740	rBV4	37602	61328	1.70%	0.136%
93	19.251	2759	2765	2776	rBV	2668045	3614386	100.00%	7.986%
94	19.821	2859	2862	2865	rBV	28809	27406	0.76%	0.061%
95	20.316	2944	2946	2949	rBV4	35865	37685	1.04%	0.083%
96	20.786	3022	3026	3037	rBV3	167193	330066	9.13%	0.729%
97	21.063	3067	3073	3078	rBV	2632786	3578555	99.01%	7.907%
98	22.351	3288	3292	3301	rVB2	152004	245483	6.79%	0.542%
99	23.598	3497	3504	3513	rBV	1267417	2663877	73.70%	5.886%
100	23.786	3528	3536	3558	rVB	1515267	3528193	97.62%	7.796%




Sum of corrected areas: 45257084

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045823.D
Acq On : 04 Jun 2024 19:12
Operator : MA/JU
Sample : P2589-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

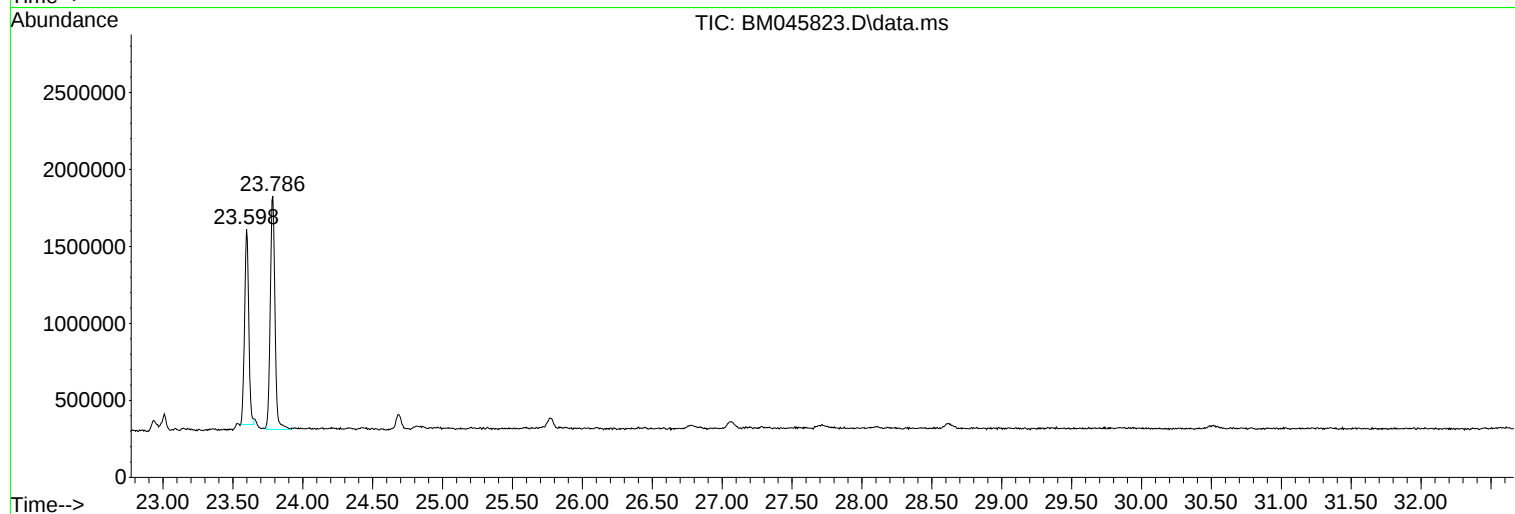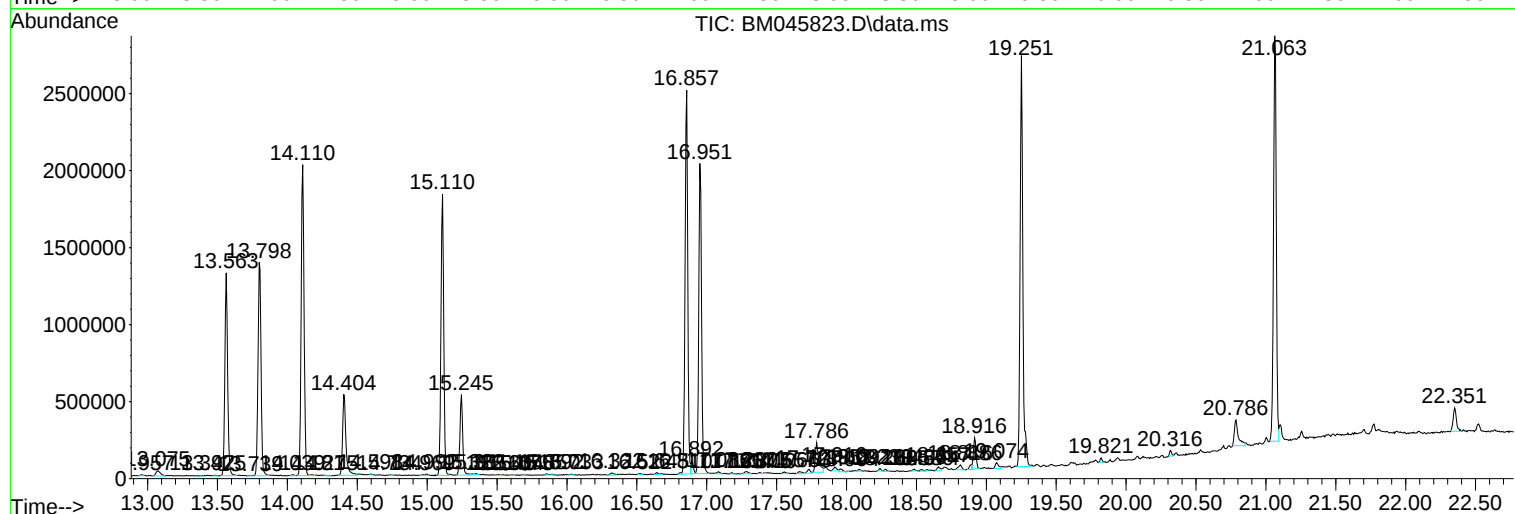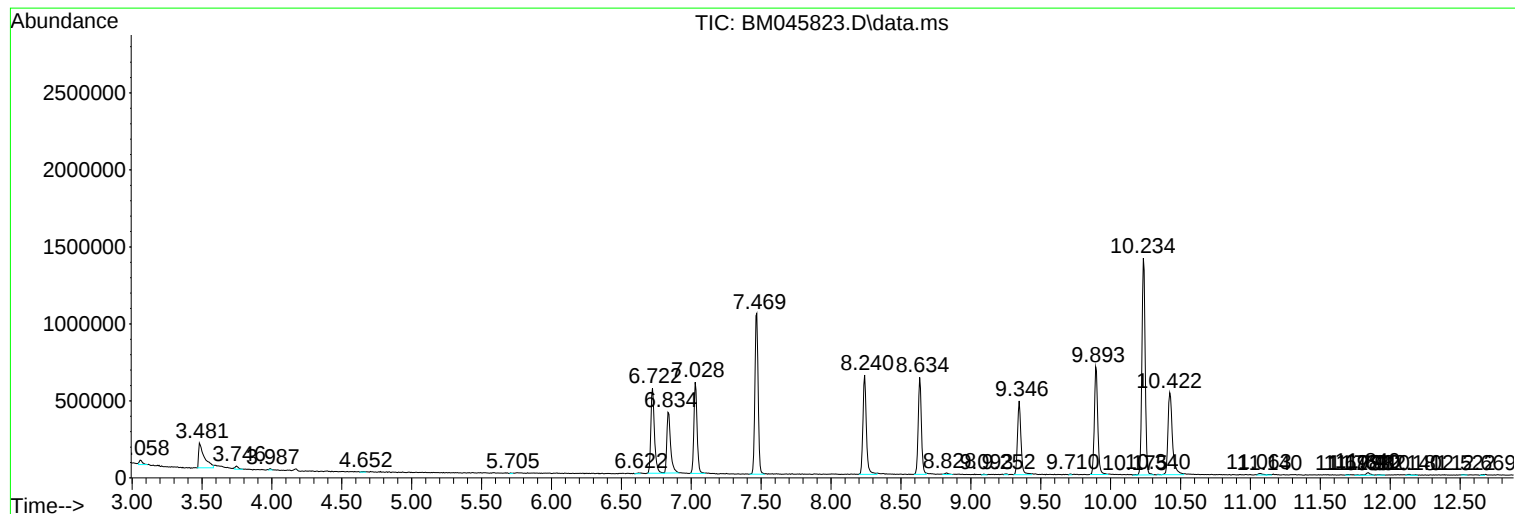

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045823.D
Acq On : 04 Jun 2024 19:12
Operator : MA/JU
Sample : P2589-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045823.D
Acq On : 04 Jun 2024 19:12
Operator : MA/JU
Sample : P2589-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------