

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045833.D
 Acq On : 05 Jun 2024 02:27
 Operator : MA/JU
 Sample : PB161208BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK208

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	8	11	22	rVB	96370	144456	2.78%	0.194%
2	3.463	78	81	102	rBV	896848	1851386	35.59%	2.491%
3	3.746	126	129	135	rVB2	23474	32130	0.62%	0.043%
4	4.169	197	201	206	rVB3	20194	32729	0.63%	0.044%
5	5.652	451	453	460	rVB8	3692	5792	0.11%	0.008%
6	6.610	612	616	617	rBV3	8358	9292	0.18%	0.013%
7	6.722	628	635	647	rBV	1508636	2536299	48.75%	3.412%
8	6.828	647	653	672	rVB	1117735	1895138	36.43%	2.550%
9	7.028	680	687	701	rVB	1595748	2496505	47.98%	3.359%
10	7.463	754	761	773	rVB	1511136	2283676	43.89%	3.072%
11	8.234	883	892	905	rBV	1827786	2964711	56.98%	3.989%
12	8.628	952	959	973	rBV	1612496	2587632	49.74%	3.481%
13	9.228	1058	1061	1065	rBV6	4562	8319	0.16%	0.011%
14	9.340	1072	1080	1096	rBV	1301414	2194812	42.19%	2.953%
15	9.892	1167	1174	1189	rBV	1715888	2973347	57.15%	4.000%
16	10.234	1223	1232	1240	rBV	1951918	3163744	60.81%	4.256%
17	10.416	1255	1263	1281	rBV	1428620	2976936	57.22%	4.005%
18	11.833	1500	1504	1514	rBV3	29907	52745	1.01%	0.071%
19	12.057	1539	1542	1547	rBV7	4621	8434	0.16%	0.011%
20	12.904	1685	1686	1691	rVB6	4793	6405	0.12%	0.009%
21	13.063	1707	1713	1722	rBV3	27977	57058	1.10%	0.077%
22	13.557	1790	1797	1807	rBV	2744938	3948094	75.89%	5.312%
23	13.798	1831	1838	1847	rBV	3206174	4564281	87.73%	6.141%
24	14.110	1883	1891	1898	rBV	2649061	3758055	72.23%	5.056%
25	14.233	1910	1912	1921	rVB8	3405	7173	0.14%	0.010%
26	14.404	1933	1941	1957	rBV	1191826	1894608	36.42%	2.549%
27	14.627	1977	1979	1987	rVB10	4162	9632	0.19%	0.013%
28	14.816	2006	2011	2013	rVV5	3712	6030	0.12%	0.008%
29	14.992	2038	2041	2045	rVB5	3796	6093	0.12%	0.008%
30	15.110	2054	2061	2070	rBV	3637047	5202686	100.00%	7.000%
31	15.245	2077	2084	2095	rBV	861604	1166221	22.42%	1.569%
32	15.351	2098	2102	2107	rVB3	20750	30452	0.59%	0.041%
33	15.680	2154	2158	2162	rVB7	5843	7222	0.14%	0.010%
34	15.810	2175	2180	2182	rBV5	4465	6693	0.13%	0.009%
35	16.533	2297	2303	2308	rBV10	6673	13193	0.25%	0.018%
36	16.645	2319	2322	2325	rVB4	10392	11894	0.23%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045833.D
Acq On : 05 Jun 2024 02:27
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK208

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	16.857	2351	2358	2366	rBV	2854277	3791903	72.88%	5.102%
38	16.951	2368	2374	2390	rVV2	3731916	5063024	97.32%	6.812%
39	17.598	2482	2484	2489	rBV6	3343	5792	0.11%	0.008%
40	17.663	2493	2495	2498	rVB4	5040	5385	0.10%	0.007%
41	18.815	2688	2691	2695	rVB3	43760	52155	1.00%	0.070%
42	18.886	2699	2703	2707	rBV	43091	59958	1.15%	0.081%
43	19.145	2745	2747	2750	rVB4	11684	9174	0.18%	0.012%
44	19.209	2756	2758	2759	rBV2	10152	7723	0.15%	0.010%
45	19.251	2759	2765	2773	rVB	4052158	5033674	96.75%	6.772%
46	21.062	3068	3073	3080	rBV	2428200	3167741	60.89%	4.262%
47	23.009	3401	3404	3413	rVB3	135319	235583	4.53%	0.317%
48	23.597	3497	3504	3520	rVB2	2060418	4334779	83.32%	5.832%
49	23.786	3528	3536	3548	rVB	1622469	3647073	70.10%	4.907%




Sum of corrected areas: 74327837

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045833.D
Acq On : 05 Jun 2024 02:27
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK208

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

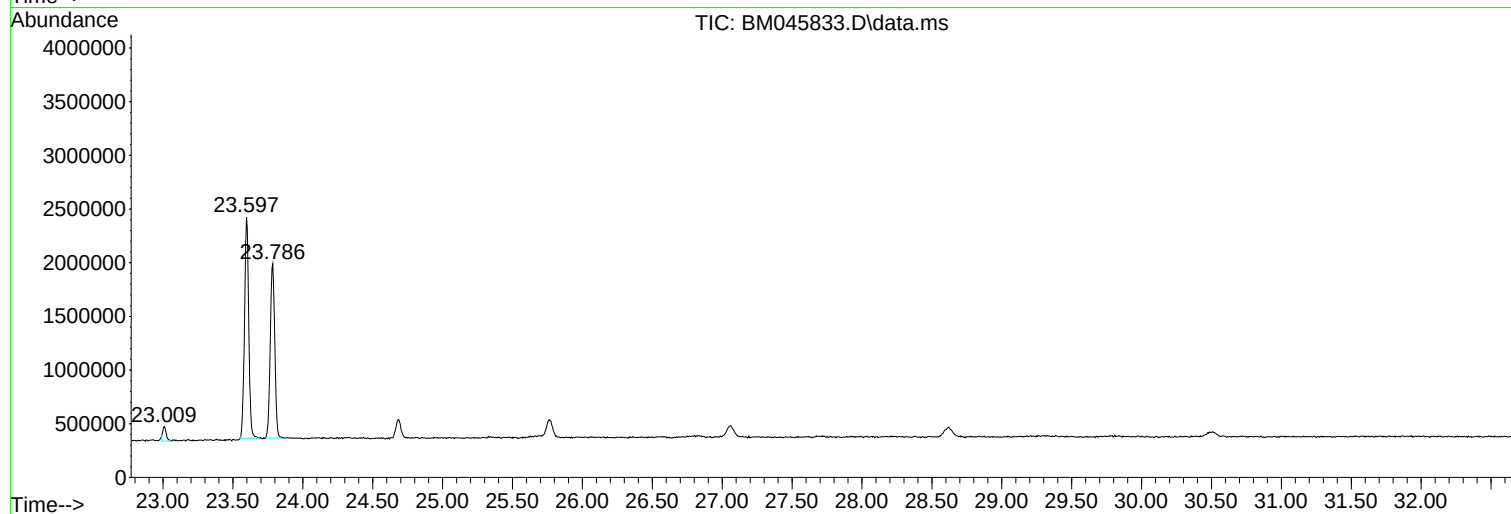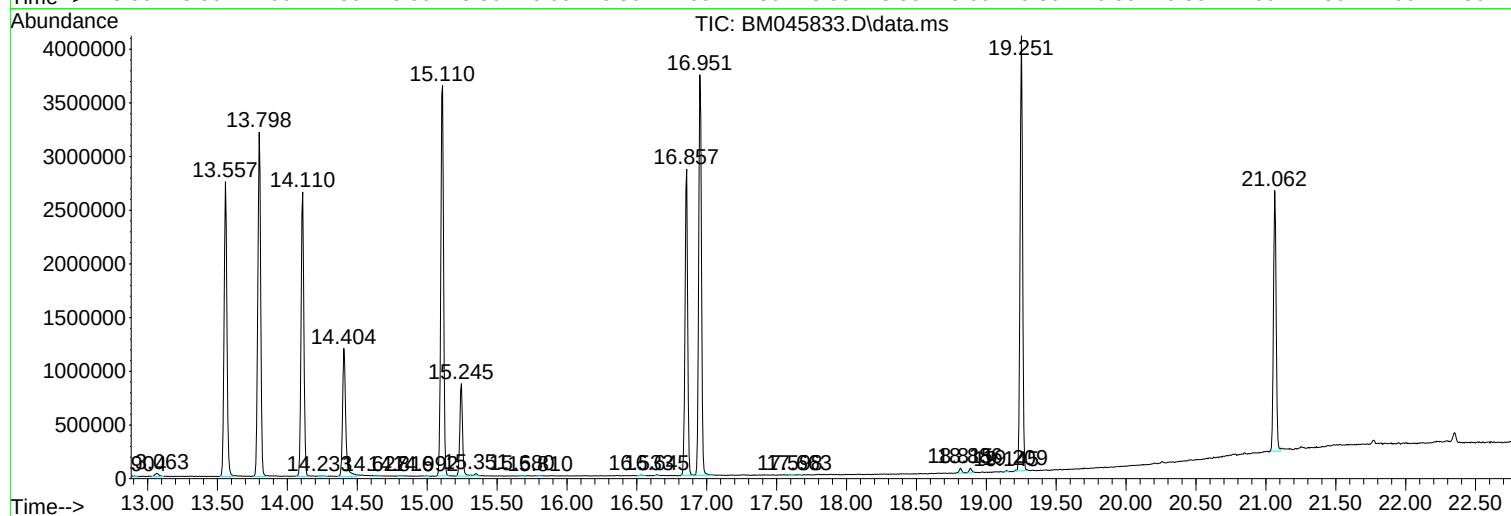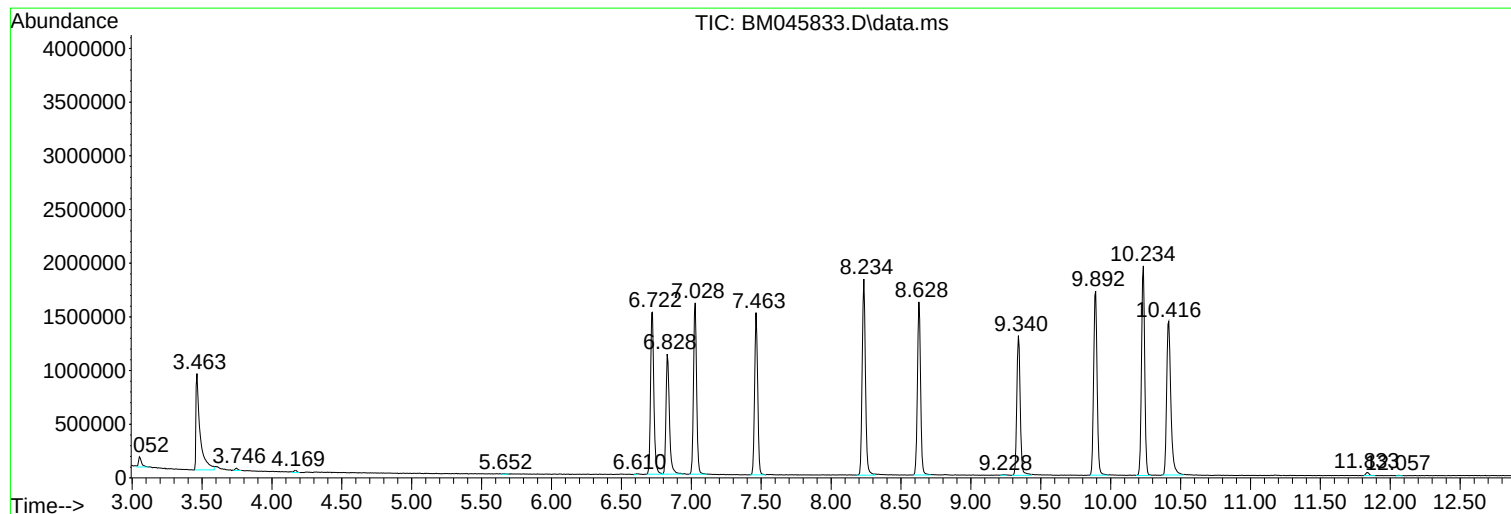

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045833.D
Acq On : 05 Jun 2024 02:27
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK208

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045833.D
Acq On : 05 Jun 2024 02:27
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK208

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc