

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045847.D
 Acq On : 05 Jun 2024 12:58
 Operator : MA/JU
 Sample : PB161208BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	8	11	19	rVB	77684	109388	2.32%	0.169%
2	3.463	78	81	101	rBV	789746	1670289	35.50%	2.578%
3	4.169	198	201	207	rVB	28319	39415	0.84%	0.061%
4	5.187	372	374	377	rBV4	5394	5291	0.11%	0.008%
5	6.616	614	617	621	rBV5	5169	6782	0.14%	0.010%
6	6.722	628	635	647	rBV	1390874	2353723	50.02%	3.633%
7	6.828	647	653	666	rVB	1011385	1655384	35.18%	2.555%
8	7.028	679	687	698	rBV	1458543	2291456	48.70%	3.537%
9	7.151	707	708	712	rVB4	5266	5214	0.11%	0.008%
10	7.463	753	761	769	rBV	1271205	1929043	41.00%	2.977%
11	8.234	883	892	904	rBV	1690032	2745371	58.34%	4.237%
12	8.628	952	959	972	rBV	1450846	2338240	49.69%	3.609%
13	9.339	1071	1080	1095	rBV	1219933	1998377	42.47%	3.084%
14	9.451	1097	1099	1105	rVB7	4647	7682	0.16%	0.012%
15	9.886	1166	1173	1189	rBV	1618639	2791017	59.31%	4.308%
16	10.228	1224	1231	1241	rBV	1646286	2715318	57.70%	4.191%
17	10.410	1255	1262	1285	rBV	1379513	2767726	58.82%	4.272%
18	11.051	1366	1371	1373	rVB6	4191	4725	0.10%	0.007%
19	11.545	1451	1455	1458	rBV5	2909	4761	0.10%	0.007%
20	11.833	1497	1504	1515	rVB2	29492	55730	1.18%	0.086%
21	13.063	1708	1713	1720	rBV3	19205	37115	0.79%	0.057%
22	13.557	1789	1797	1812	rBV	2589961	3633771	77.22%	5.609%
23	13.798	1830	1838	1845	rBV	2971602	4154815	88.30%	6.413%
24	14.104	1884	1890	1899	rVV	2256859	3269994	69.49%	5.047%
25	14.404	1935	1941	1959	rBV	1012782	1642805	34.91%	2.536%
26	14.798	2007	2008	2013	rVB4	6136	7173	0.15%	0.011%
27	15.104	2054	2060	2070	rVV	3355735	4705522	100.00%	7.263%
28	15.245	2078	2084	2092	rBV	757860	1010367	21.47%	1.559%
29	15.351	2098	2102	2107	rVB4	15445	21322	0.45%	0.033%
30	15.516	2127	2130	2135	rBV7	3127	6135	0.13%	0.009%
31	15.892	2191	2194	2198	rVB6	4003	5034	0.11%	0.008%
32	16.539	2301	2304	2307	rVB4	6086	6754	0.14%	0.010%
33	16.645	2318	2322	2326	rBV5	8736	9122	0.19%	0.014%
34	16.851	2351	2357	2368	rBV	2282071	3197386	67.95%	4.935%
35	16.951	2368	2374	2388	rVV	3384963	4509520	95.83%	6.960%
36	17.045	2388	2390	2392	rVB3	5656	5023	0.11%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045847.D
Acq On : 05 Jun 2024 12:58
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	18.204	2584	2587	2588	rBV2	3896	4938	0.10%	0.008%
38	18.815	2687	2691	2697	rVB3	35319	54328	1.15%	0.084%
39	18.886	2697	2703	2708	rBV	40049	67997	1.45%	0.105%
40	19.251	2759	2765	2775	rVB	3426989	4228450	89.86%	6.527%
41	21.062	3068	3073	3082	rBV	1756123	2510465	53.35%	3.875%
42	23.597	3497	3504	3516	rBV2	1672938	3515476	74.71%	5.426%
43	23.786	3529	3536	3547	rVB	1222053	2689448	57.16%	4.151%




Sum of corrected areas: 64787892

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045847.D
Acq On : 05 Jun 2024 12:58
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

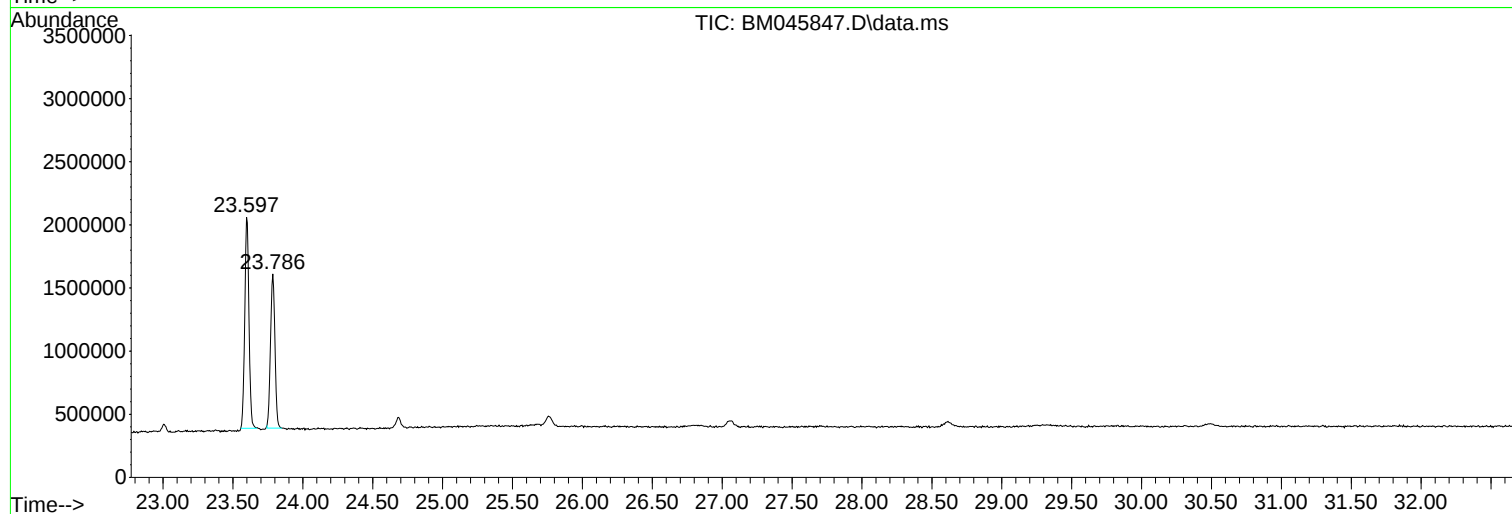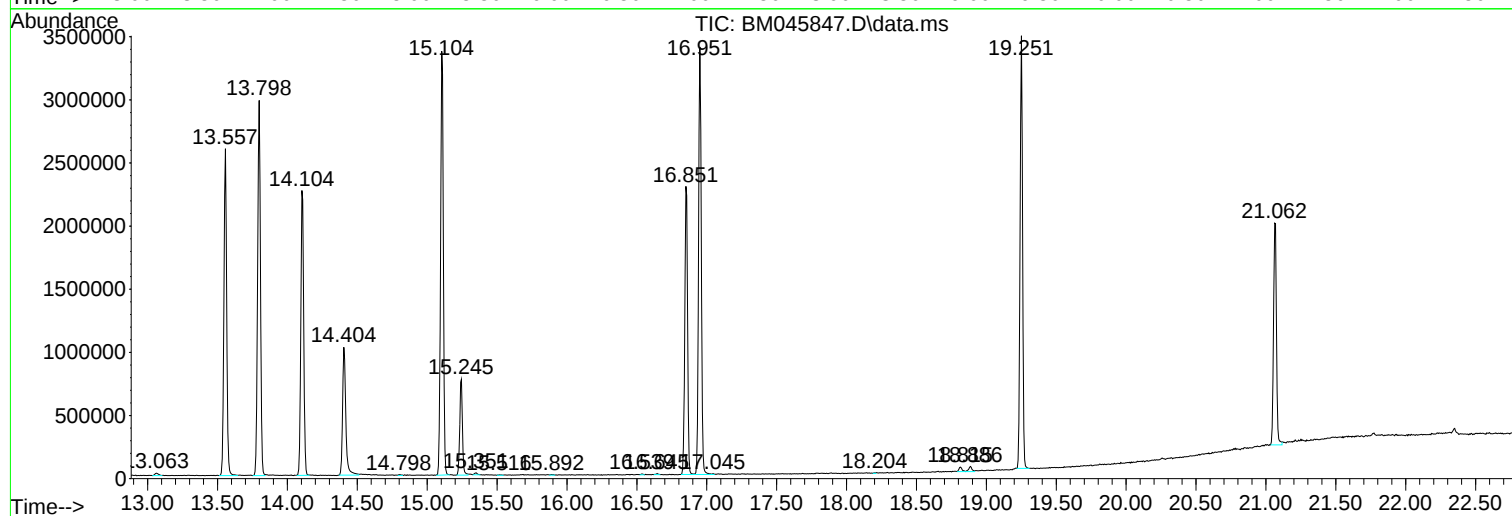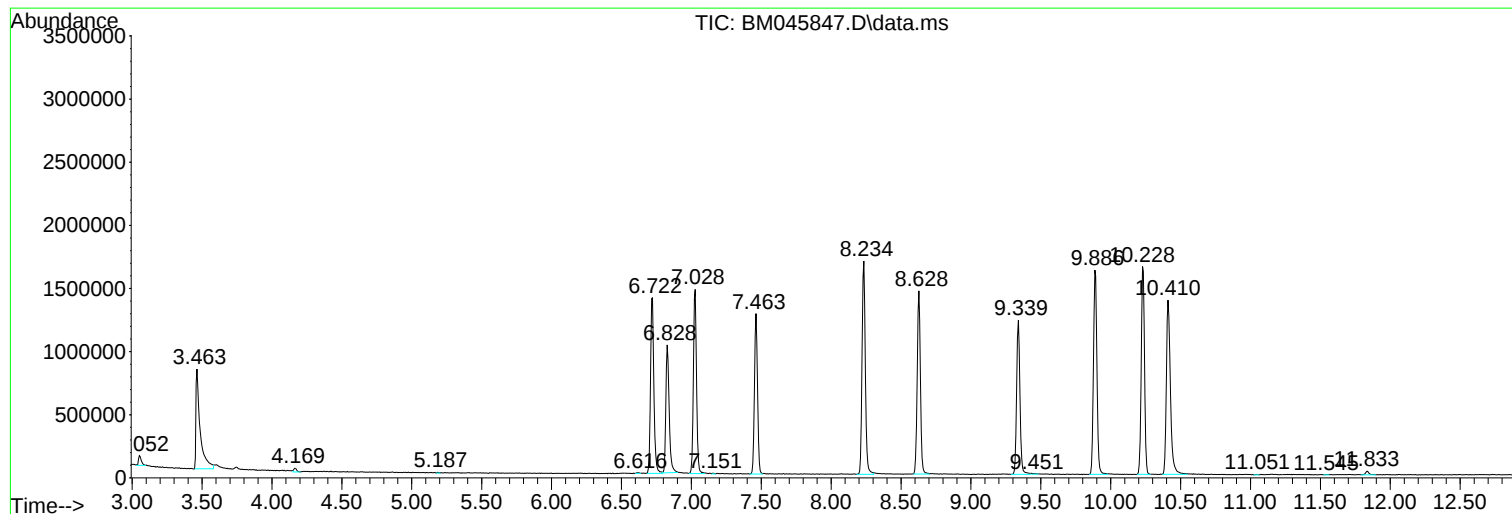

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045847.D
Acq On : 05 Jun 2024 12:58
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045847.D
Acq On : 05 Jun 2024 12:58
Operator : MA/JU
Sample : PB161208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc