

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045856.D
 Acq On : 05 Jun 2024 18:56
 Operator : MA/JU
 Sample : P2586-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	23	rVB	57242	97736	3.41%	0.207%
2	3.375	63	66	75	rBV	25142	52143	1.82%	0.111%
3	3.469	79	82	104	rBV	479120	1065702	37.16%	2.259%
4	3.746	126	129	136	rVB2	22157	32109	1.12%	0.068%
5	4.163	198	200	205	rVB	17611	23731	0.83%	0.050%
6	4.987	337	340	342	rVB4	5112	5416	0.19%	0.011%
7	5.663	451	455	459	rBV3	10005	19672	0.69%	0.042%
8	5.751	468	470	475	rVB5	7519	9845	0.34%	0.021%
9	5.916	497	498	500	rBV2	4138	4148	0.14%	0.009%
10	5.946	502	503	506	rVV3	4417	5708	0.20%	0.012%
11	6.275	558	559	563	rBV4	4360	4133	0.14%	0.009%
12	6.616	614	617	618	rBV3	6895	8228	0.29%	0.017%
13	6.722	628	635	647	rVV	949428	1587983	55.37%	3.366%
14	6.828	647	653	666	rVB	684030	1106373	38.58%	2.345%
15	7.028	680	687	695	rBV	996796	1522823	53.10%	3.228%
16	7.098	697	699	702	rVB4	5864	5841	0.20%	0.012%
17	7.298	731	733	737	rBV5	3024	4135	0.14%	0.009%
18	7.463	752	761	772	rBV	1222735	1866805	65.10%	3.958%
19	7.587	778	782	787	rVB6	8516	14524	0.51%	0.031%
20	7.634	787	790	792	rBV4	7138	9760	0.34%	0.021%
21	7.898	832	835	838	rVB5	3804	3967	0.14%	0.008%
22	8.128	872	874	877	rBV3	4123	4773	0.17%	0.010%
23	8.234	885	892	898	rBV	1108138	1770430	61.74%	3.753%
24	8.292	898	902	914	rVB	142457	254022	8.86%	0.539%
25	8.628	951	959	972	rVV	984222	1560822	54.43%	3.309%
26	8.804	986	989	993	rVB6	7653	11842	0.41%	0.025%
27	8.898	1002	1005	1008	rVV5	3730	5109	0.18%	0.011%
28	9.110	1038	1041	1046	rVB6	3664	4775	0.17%	0.010%
29	9.245	1058	1064	1073	rVV2	60412	116400	4.06%	0.247%
30	9.339	1073	1080	1091	rVB	769359	1255978	43.80%	2.663%
31	9.510	1106	1109	1114	rVB7	2569	4334	0.15%	0.009%
32	9.692	1136	1140	1143	rBV6	5282	9440	0.33%	0.020%
33	9.722	1143	1145	1148	rVV4	3734	4888	0.17%	0.010%
34	9.745	1148	1149	1154	rVB5	4190	5302	0.18%	0.011%
35	9.892	1165	1174	1185	rBV	1043013	1780651	62.09%	3.775%
36	10.228	1223	1231	1241	rBV	1504788	2548855	88.88%	5.404%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045856.D
 Acq On : 05 Jun 2024 18:56
 Operator : MA/JU
 Sample : P2586-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

37	10.357	1249	1253	1255	rBV5	3908	6378	0.22%	0.014%
38	10.410	1255	1262	1278	rBV	883523	1721200	60.02%	3.649%
39	10.622	1297	1298	1304	rVB6	4025	5490	0.19%	0.012%
40	10.869	1334	1340	1349	rBV6	20393	39395	1.37%	0.084%

41	11.033	1359	1368	1378	rBV2	83602	202868	7.07%	0.430%
42	11.133	1381	1385	1388	rVV5	6201	11958	0.42%	0.025%
43	11.692	1474	1480	1481	rBV6	6409	9423	0.33%	0.020%
44	11.833	1497	1504	1509	rBV5	18866	33933	1.18%	0.072%
45	12.327	1586	1588	1590	rBV3	3472	4008	0.14%	0.008%

46	12.504	1616	1618	1621	rBV3	4242	6098	0.21%	0.013%
47	12.951	1689	1694	1697	rBV7	7839	10969	0.38%	0.023%
48	12.998	1700	1702	1709	rVB8	2685	4763	0.17%	0.010%
49	13.086	1711	1717	1725	rVV8	9162	23522	0.82%	0.050%
50	13.322	1751	1757	1771	rBV2	104884	264518	9.22%	0.561%

51	13.427	1773	1775	1779	rVB5	4618	6555	0.23%	0.014%
52	13.469	1779	1782	1784	rBV4	4354	5692	0.20%	0.012%
53	13.557	1791	1797	1806	rBV	1610683	2207818	76.99%	4.681%
54	13.798	1830	1838	1847	rBV	1834955	2583533	90.09%	5.477%
55	14.027	1873	1877	1882	rVB5	5833	9396	0.33%	0.020%

56	14.104	1884	1890	1898	rVV	1878860	2779337	96.92%	5.892%
57	14.180	1901	1903	1908	rVB6	5027	5905	0.21%	0.013%
58	14.357	1928	1933	1935	rBV6	25075	36724	1.28%	0.078%
59	14.410	1935	1942	1961	rVV	574541	955205	33.31%	2.025%
60	14.533	1961	1963	1966	rVB4	4118	4246	0.15%	0.009%

61	14.569	1966	1969	1973	rBV6	6729	9155	0.32%	0.019%
62	14.657	1981	1984	1988	rBV5	6163	9407	0.33%	0.020%
63	14.927	2025	2030	2033	rBV5	7203	10367	0.36%	0.022%
64	14.963	2033	2036	2037	rVV3	5498	4198	0.15%	0.009%
65	14.986	2037	2040	2044	rVB7	11779	13448	0.47%	0.029%

66	15.104	2054	2060	2069	rVB	2098044	2867730	100.00%	6.080%
67	15.245	2079	2084	2095	rBV	362967	494382	17.24%	1.048%
68	15.333	2096	2099	2100	rVV3	3866	4468	0.16%	0.009%
69	15.345	2100	2101	2106	rVB5	9220	9177	0.32%	0.019%
70	15.427	2112	2115	2117	rVB3	4589	4579	0.16%	0.010%

71	15.492	2123	2126	2127	rBV3	5061	4072	0.14%	0.009%
72	15.551	2132	2136	2139	rVB4	5744	9373	0.33%	0.020%
73	15.621	2145	2148	2150	rVV4	6635	7241	0.25%	0.015%
74	15.716	2162	2164	2168	rBV5	3393	4106	0.14%	0.009%
75	15.851	2183	2187	2190	rVV5	7700	9385	0.33%	0.020%

76	16.074	2223	2225	2229	rBV4	5103	7196	0.25%	0.015%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045856.D
 Acq On : 05 Jun 2024 18:56
 Operator : MA/JU
 Sample : P2586-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

77	16.310	2260	2265	2269	rBV8	10271	16240	0.57%	0.034%
78	16.433	2281	2286	2290	rBV8	9343	16171	0.56%	0.034%
79	16.592	2310	2313	2316	rBV4	6476	6974	0.24%	0.015%
80	16.633	2317	2320	2324	rBV5	12162	17863	0.62%	0.038%
81	16.804	2347	2349	2352	rBV4	4031	3917	0.14%	0.008%
82	16.851	2352	2357	2367	rVV	1859468	2636254	91.93%	5.589%
83	16.951	2368	2374	2384	rVV	1871944	2570635	89.64%	5.450%
84	17.092	2393	2398	2399	rVV4	9071	12916	0.45%	0.027%
85	17.174	2406	2412	2416	rBV8	10385	18018	0.63%	0.038%
86	17.268	2425	2428	2429	rBV3	4113	5256	0.18%	0.011%
87	17.457	2458	2460	2463	rVB4	4664	3979	0.14%	0.008%
88	17.551	2474	2476	2479	rVB3	8197	6810	0.24%	0.014%
89	17.780	2511	2515	2522	rBV	94336	163769	5.71%	0.347%
90	18.092	2564	2568	2575	rVB9	14009	27167	0.95%	0.058%
91	18.457	2628	2630	2634	rBV5	6966	10451	0.36%	0.022%
92	18.592	2651	2653	2654	rVB2	7726	4303	0.15%	0.009%
93	18.698	2669	2671	2675	rVB4	21131	23329	0.81%	0.049%
94	18.815	2688	2691	2696	rVB5	24522	34070	1.19%	0.072%
95	19.068	2731	2734	2740	rBV7	25965	49533	1.73%	0.105%
96	19.251	2760	2765	2773	rBV	2144955	2678967	93.42%	5.679%
97	20.780	3022	3025	3031	rBV3	137759	199173	6.95%	0.422%
98	21.062	3068	3073	3079	rBV	1656659	2338373	81.54%	4.957%
99	23.597	3498	3504	3520	rVB2	1137023	2547375	88.83%	5.400%
100	23.786	3529	3536	3545	rVB	1140007	2583053	90.07%	5.476%


Sum of corrected areas: 47170217

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045856.D
Acq On : 05 Jun 2024 18:56
Operator : MA/JU
Sample : P2586-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4D30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

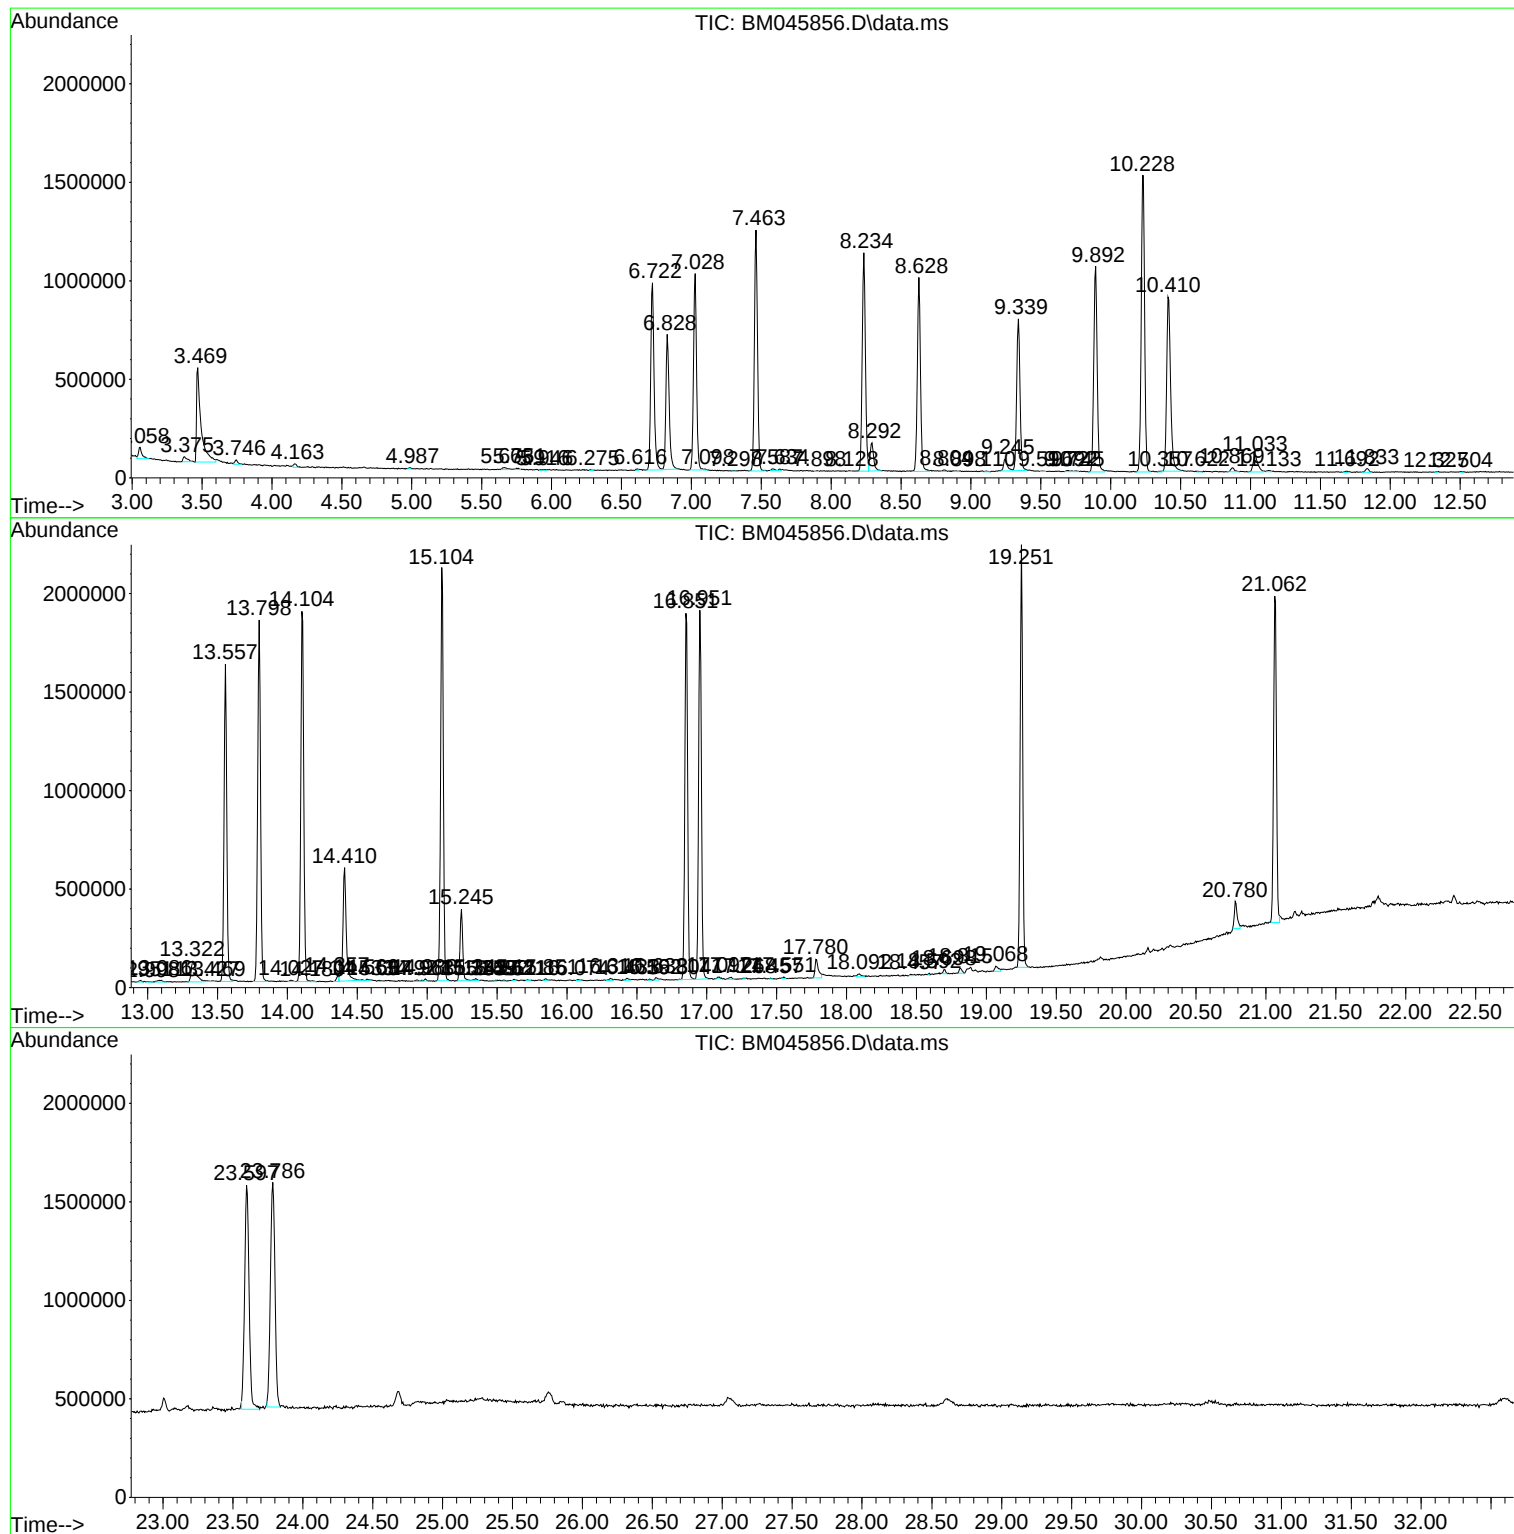

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045856.D
Acq On : 05 Jun 2024 18:56
Operator : MA/JU
Sample : P2586-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4D30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045856.D
Acq On : 05 Jun 2024 18:56
Operator : MA/JU
Sample : P2586-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4D30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------