

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045859.D
 Acq On : 05 Jun 2024 20:55
 Operator : MA/JU
 Sample : P2591-05DL2 30X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH5S8DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.169	198	201	204	rVB	20510	24311	0.92%	0.135%
2	4.399	238	240	242	rBV3	4150	3757	0.14%	0.021%
3	4.940	328	332	334	rBV4	5596	6065	0.23%	0.034%
4	5.110	359	361	364	rBV4	3400	4022	0.15%	0.022%
5	5.669	453	456	460	rBV6	4203	5809	0.22%	0.032%
6	6.428	584	585	588	rVV3	5189	3928	0.15%	0.022%
7	6.463	588	591	592	rVV3	4357	4277	0.16%	0.024%
8	6.498	595	597	599	rBV2	4295	3590	0.14%	0.020%
9	6.587	610	612	613	rBV2	5003	3687	0.14%	0.020%
10	6.622	613	618	622	rVV7	6826	11968	0.45%	0.066%
11	6.875	658	661	663	rVB4	3427	3681	0.14%	0.020%
12	6.951	672	674	676	rBV3	4389	4813	0.18%	0.027%
13	7.028	684	687	688	rBV3	4376	5241	0.20%	0.029%
14	7.040	688	689	694	rVB5	6673	5894	0.22%	0.033%
15	7.128	702	704	707	rVB4	4144	3968	0.15%	0.022%
16	7.463	754	761	771	rBV	1137968	1779263	67.05%	9.862%
17	7.534	771	773	779	rVV7	4986	8025	0.30%	0.044%
18	8.140	873	876	881	rBV7	3608	5562	0.21%	0.031%
19	8.263	893	897	900	rVV6	4668	7979	0.30%	0.044%
20	8.651	961	963	967	rBV5	4498	6793	0.26%	0.038%
21	8.816	989	991	994	rVB3	4006	4613	0.17%	0.026%
22	9.222	1057	1060	1062	rVB4	3804	3746	0.14%	0.021%
23	9.351	1078	1082	1083	rBV3	6001	4876	0.18%	0.027%
24	9.534	1109	1113	1117	rBV6	3640	6406	0.24%	0.036%
25	9.922	1177	1179	1181	rVV3	5265	4687	0.18%	0.026%
26	10.045	1197	1200	1203	rVB5	2526	3705	0.14%	0.021%
27	10.234	1223	1232	1248	rVB	1414389	2396810	90.32%	13.285%
28	10.345	1248	1251	1253	rBV4	2864	4015	0.15%	0.022%
29	10.557	1284	1287	1289	rBV4	3620	5440	0.21%	0.030%
30	10.892	1339	1344	1345	rBV5	3976	5481	0.21%	0.030%
31	11.169	1389	1391	1396	rVV6	2495	4102	0.15%	0.023%
32	11.692	1475	1480	1481	rVB5	4270	3597	0.14%	0.020%
33	11.910	1513	1517	1523	rVB5	10563	18422	0.69%	0.102%
34	11.963	1523	1526	1529	rBV5	3377	3806	0.14%	0.021%
35	12.133	1548	1555	1558	rVV8	8710	18028	0.68%	0.100%
36	12.945	1691	1693	1695	rBV2	3910	4715	0.18%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045859.D
 Acq On : 05 Jun 2024 20:55
 Operator : MA/JU
 Sample : P2591-05DL2 30X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH5S8DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

37	12.986	1698	1700	1702	rBV3	3954	3925	0.15%	0.022%
38	13.275	1745	1749	1750	rBV4	4287	4229	0.16%	0.023%
39	13.316	1753	1756	1760	rVB5	2863	4614	0.17%	0.026%
40	13.433	1770	1776	1780	rBV8	7986	12000	0.45%	0.067%
41	13.486	1780	1785	1789	rVB7	5917	10482	0.40%	0.058%
42	13.580	1798	1801	1806	rVB6	6832	11974	0.45%	0.066%
43	13.669	1812	1816	1823	rBV8	5474	11138	0.42%	0.062%
44	13.751	1827	1830	1834	rBV5	2596	4316	0.16%	0.024%
45	13.804	1834	1839	1842	rBV5	9644	17815	0.67%	0.099%
46	13.833	1842	1844	1849	rVV6	8081	10023	0.38%	0.056%
47	14.104	1883	1890	1898	rBV	1769812	2555454	96.30%	14.164%
48	14.169	1898	1901	1907	rVB2	30909	44188	1.67%	0.245%
49	14.516	1956	1960	1966	rVB	29400	45857	1.73%	0.254%
50	14.604	1970	1975	1976	rBV5	2682	3523	0.13%	0.020%
51	14.733	1994	1997	1999	rBV4	5856	7128	0.27%	0.040%
52	14.792	2004	2007	2008	rBV3	5085	4408	0.17%	0.024%
53	14.874	2017	2021	2024	rBV5	4246	4343	0.16%	0.024%
54	14.921	2024	2029	2036	rVB9	4312	10438	0.39%	0.058%
55	15.051	2047	2051	2053	rBV4	2972	3989	0.15%	0.022%
56	15.110	2057	2061	2065	rVV	13075	17948	0.68%	0.099%
57	15.163	2066	2070	2079	rVB2	32638	52038	1.96%	0.288%
58	15.286	2089	2091	2095	rVB5	4006	4851	0.18%	0.027%
59	15.321	2095	2097	2103	rBV7	5032	6917	0.26%	0.038%
60	15.404	2108	2111	2112	rBV3	5917	4584	0.17%	0.025%
61	15.463	2116	2121	2126	rBV6	14614	21861	0.82%	0.121%
62	15.616	2142	2147	2153	rVB5	13055	25014	0.94%	0.139%
63	15.704	2159	2162	2164	rVV4	3471	3871	0.15%	0.021%
64	15.810	2175	2180	2181	rVB5	4521	5799	0.22%	0.032%
65	15.857	2183	2188	2190	rBV5	6888	11601	0.44%	0.064%
66	16.174	2237	2242	2247	rVB8	7796	13869	0.52%	0.077%
67	16.286	2258	2261	2264	rBV5	3340	3610	0.14%	0.020%
68	16.315	2264	2266	2269	rBV4	3915	5040	0.19%	0.028%
69	16.398	2277	2280	2282	rBV4	4677	5560	0.21%	0.031%
70	16.439	2282	2287	2290	rBV7	7127	8838	0.33%	0.049%
71	16.515	2297	2300	2306	rVB2	30073	45022	1.70%	0.250%
72	16.598	2309	2314	2318	rVV7	6147	11140	0.42%	0.062%
73	16.651	2319	2323	2324	rVV4	3879	5650	0.21%	0.031%
74	16.674	2324	2327	2331	rVB	22391	29575	1.11%	0.164%
75	16.851	2351	2357	2362	rVV	1770235	2531751	95.41%	14.033%
76	16.892	2362	2364	2370	rVV	444056	570687	21.51%	3.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
 Data File : BM045859.D
 Acq On : 05 Jun 2024 20:55
 Operator : MA/JU
 Sample : P2591-05DL2 30X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH5S8DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

77	16.957	2372	2375	2376	rVV3	16698	20957	0.79%	0.116%
78	16.986	2376	2380	2385	rVV	84083	124361	4.69%	0.689%
79	17.062	2388	2393	2398	rVB7	6736	15762	0.59%	0.087%
80	17.280	2422	2430	2437	rBV2	50733	95874	3.61%	0.531%
81	17.374	2444	2446	2447	rBV2	5466	5054	0.19%	0.028%
82	17.439	2454	2457	2458	rBV2	6884	7595	0.29%	0.042%
83	17.727	2502	2506	2510	rBV	36644	51817	1.95%	0.287%
84	17.774	2510	2514	2523	rVB	51201	81480	3.07%	0.452%
85	17.857	2525	2528	2533	rBV5	12877	19488	0.73%	0.108%
86	17.921	2533	2539	2543	rBV3	51372	83739	3.16%	0.464%
87	18.092	2566	2568	2571	rVB4	10600	10360	0.39%	0.057%
88	18.239	2588	2593	2596	rBV	30467	44737	1.69%	0.248%
89	18.280	2596	2600	2604	rVB3	27006	38417	1.45%	0.213%
90	18.533	2639	2643	2647	rBV7	11171	15288	0.58%	0.085%
91	18.798	2684	2688	2693	rVB3	34373	54203	2.04%	0.300%
92	18.915	2703	2708	2714	rBV	544228	710093	26.76%	3.936%
93	19.280	2766	2770	2774	rVB	356859	464196	17.49%	2.573%
94	19.351	2780	2782	2791	rVB3	19584	33745	1.27%	0.187%
95	19.468	2799	2802	2807	rVB	28718	37646	1.42%	0.209%
96	19.609	2822	2826	2832	rBV5	26786	59027	2.22%	0.327%
97	20.533	2980	2983	2988	rBV	60538	69959	2.64%	0.388%
98	21.062	3067	3073	3078	rBV	1789471	2653567	100.00%	14.708%
99	21.103	3078	3080	3085	rVB	187919	204770	7.72%	1.135%
100	23.786	3529	3536	3551	rVB	1128007	2589473	97.58%	14.353%


Sum of corrected areas: 18041760

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045859.D
Acq On : 05 Jun 2024 20:55
Operator : MA/JU
Sample : P2591-05DL2 30X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH5S8DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

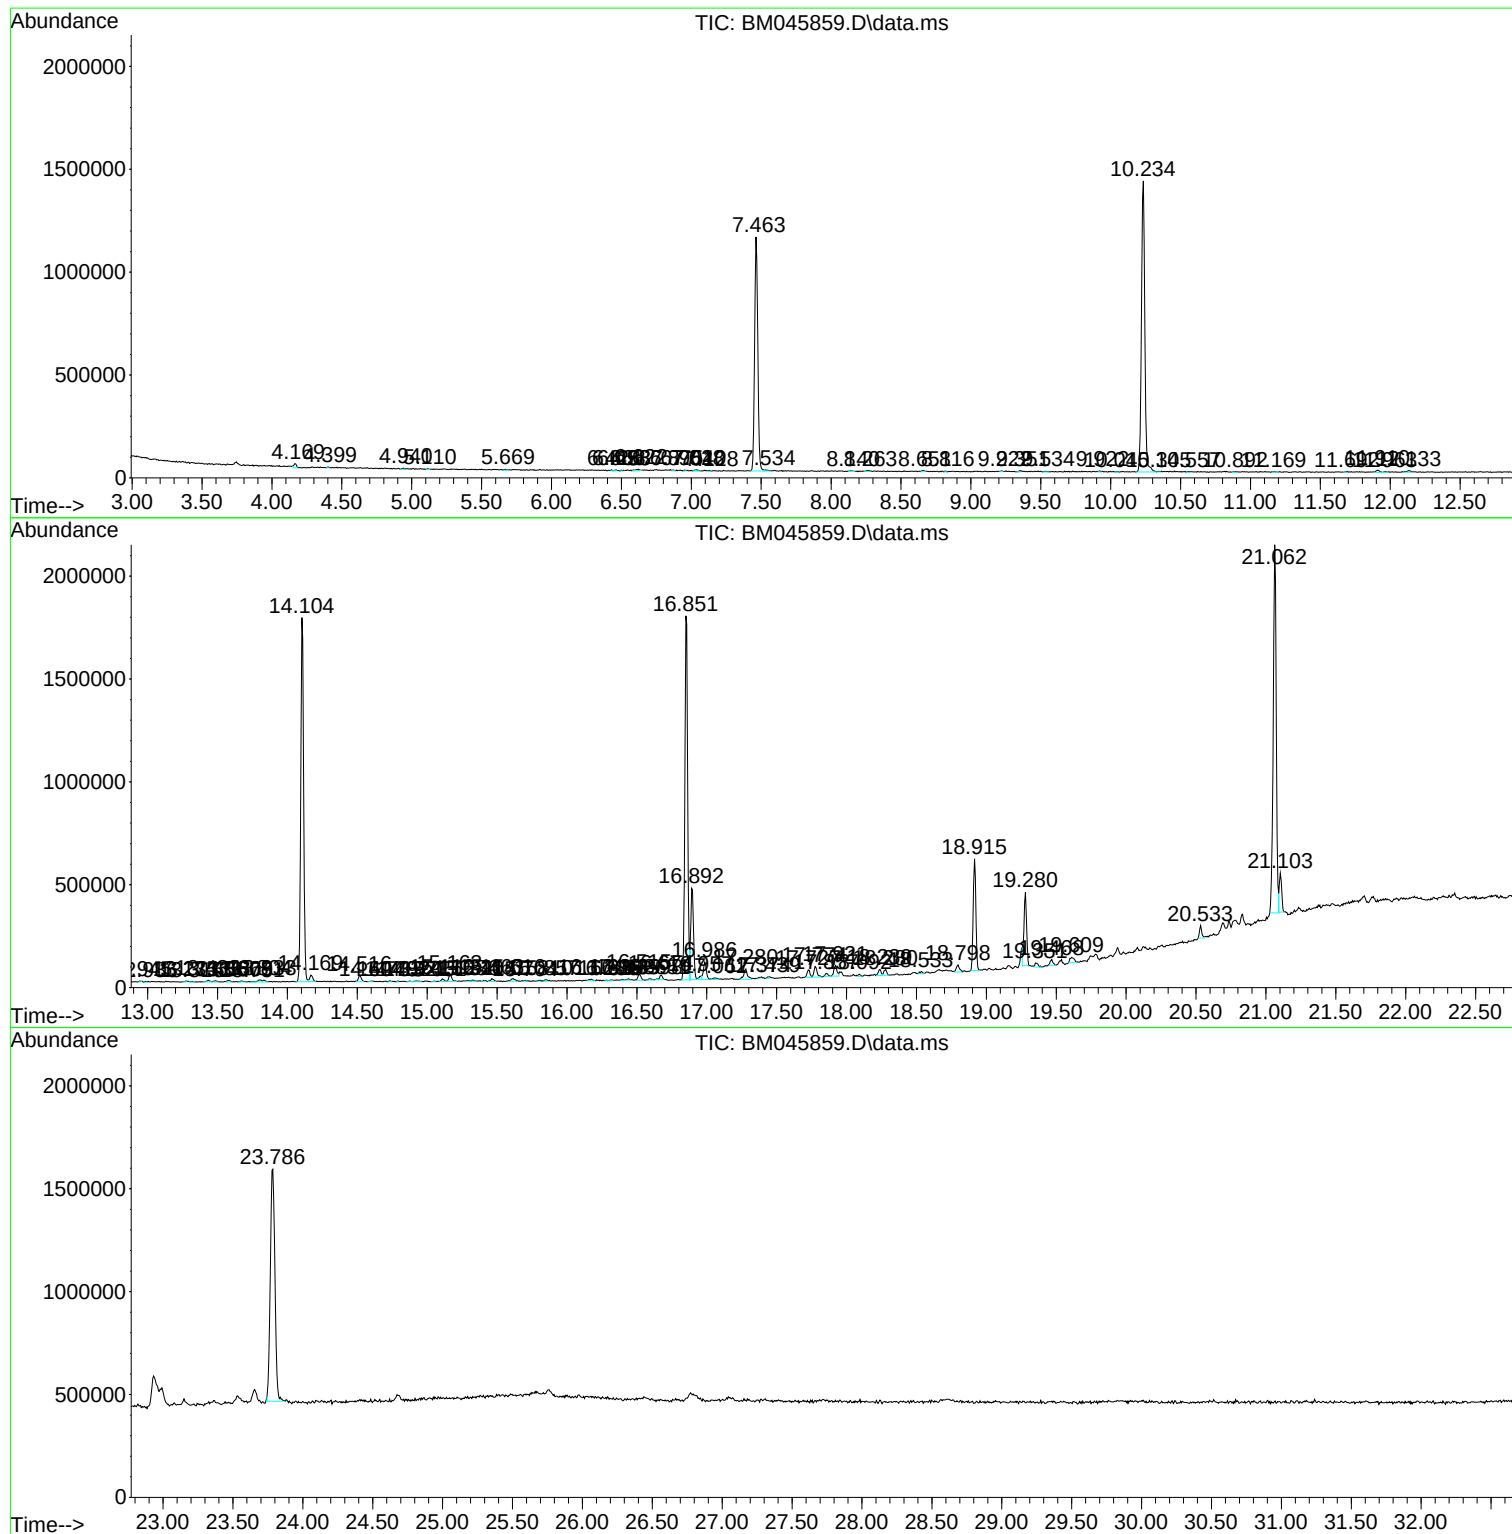

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045859.D
Acq On : 05 Jun 2024 20:55
Operator : MA/JU
Sample : P2591-05DL2 30X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH5S8DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060424\
Data File : BM045859.D
Acq On : 05 Jun 2024 20:55
Operator : MA/JU
Sample : P2591-05DL2 30X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH5S8DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------