


Data Path : Z:\HPCHEM1\BNA M\Data\BM060517\
Data File : BM010415.D
Acq On : 05 Jun 2017 09:20
Operator : SJ/MA
Sample : I3164-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG6

Manual Integrations
APPROVED

mohammad
6/6/2017 12:24:18 PM

Quant Time: Jun 05 18:54:51 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 04:03:07 2017
Response via : Initial Calibration

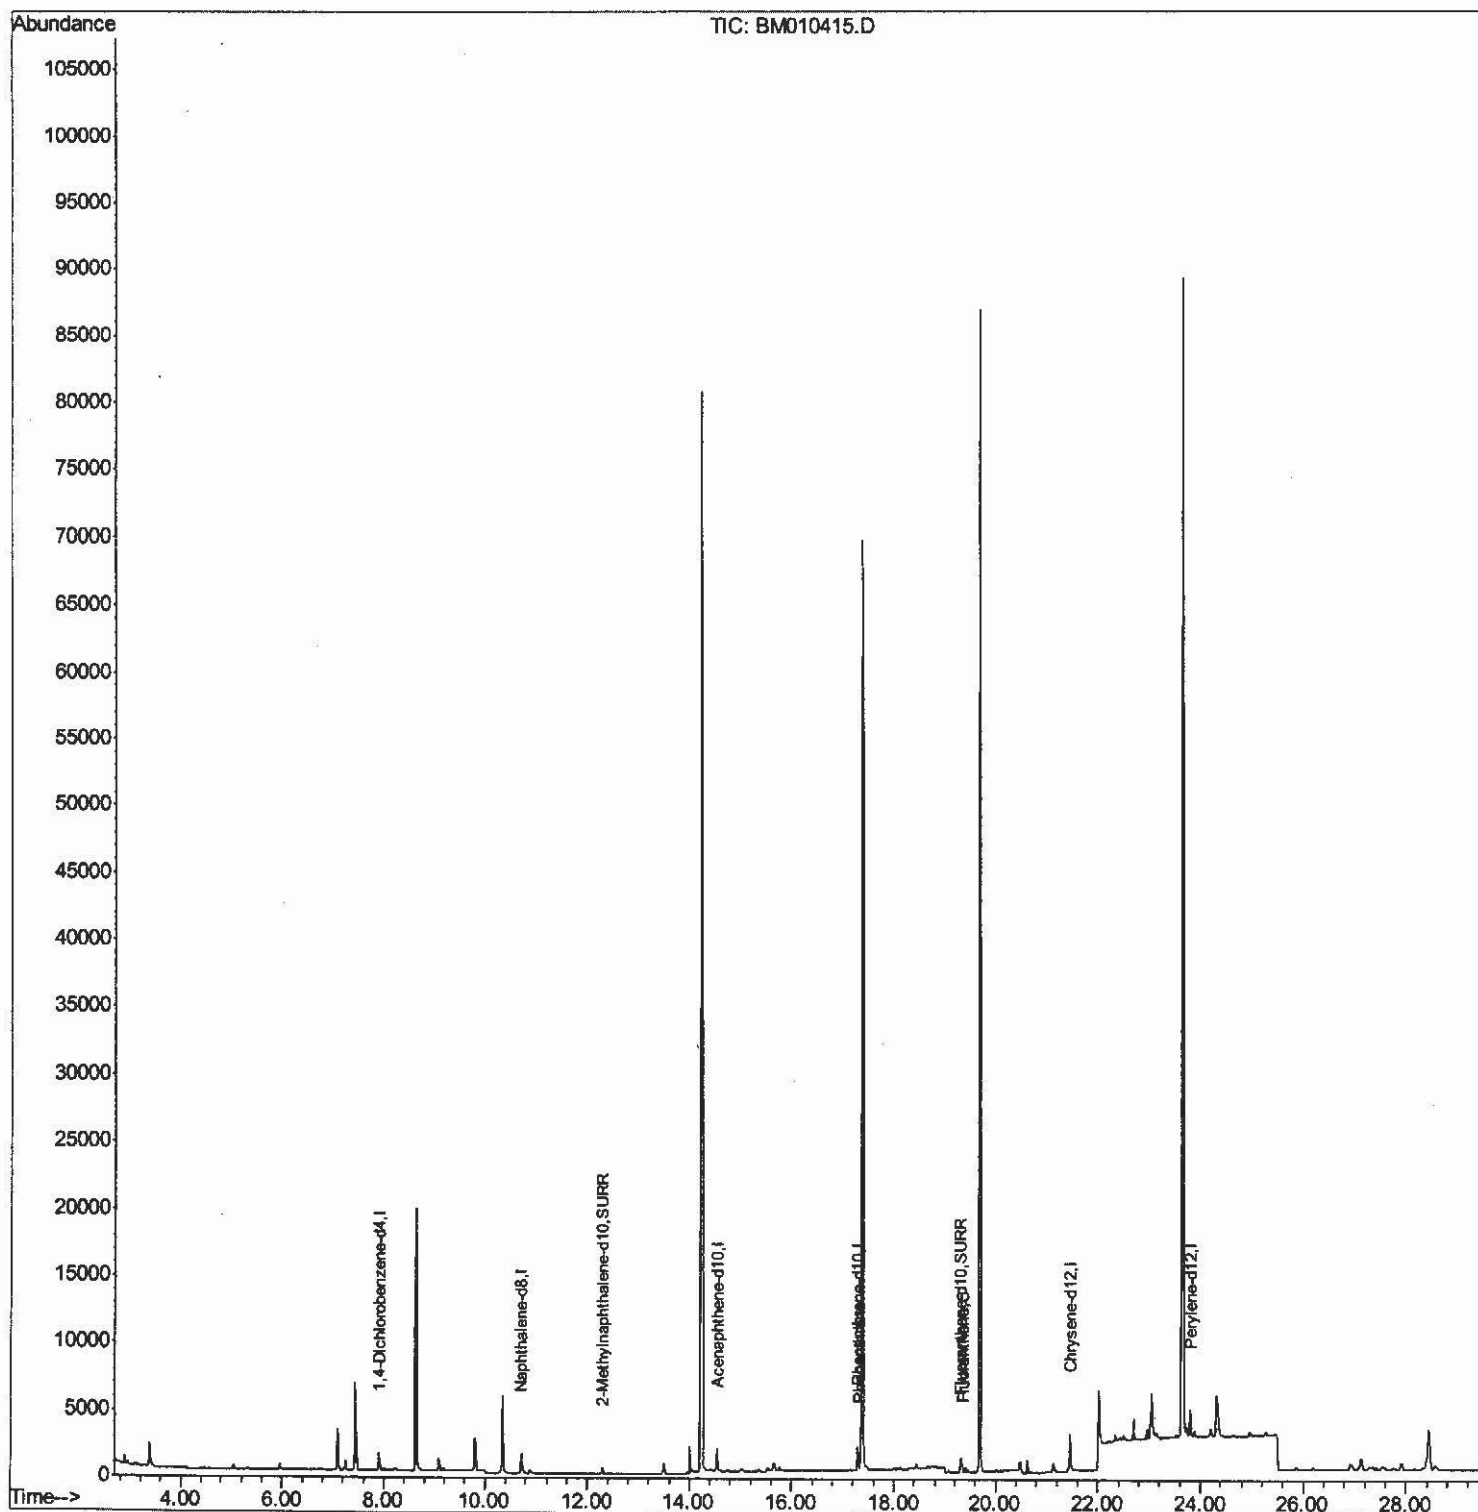


Data Path : Z:\HPCHEM1\BNA M\Data\BM060517\
Data File : BM010415.D
Acq On : 05 Jun 2017 09:20
Operator : SJ/MA
Sample : I3164-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG6

Manual Integrations
APPROVED

mohammad
6/6/2017 12:24:18 PM

Quant Time: Jun 05 13:24:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 04:03:07 2017
Response via : Initial Calibration

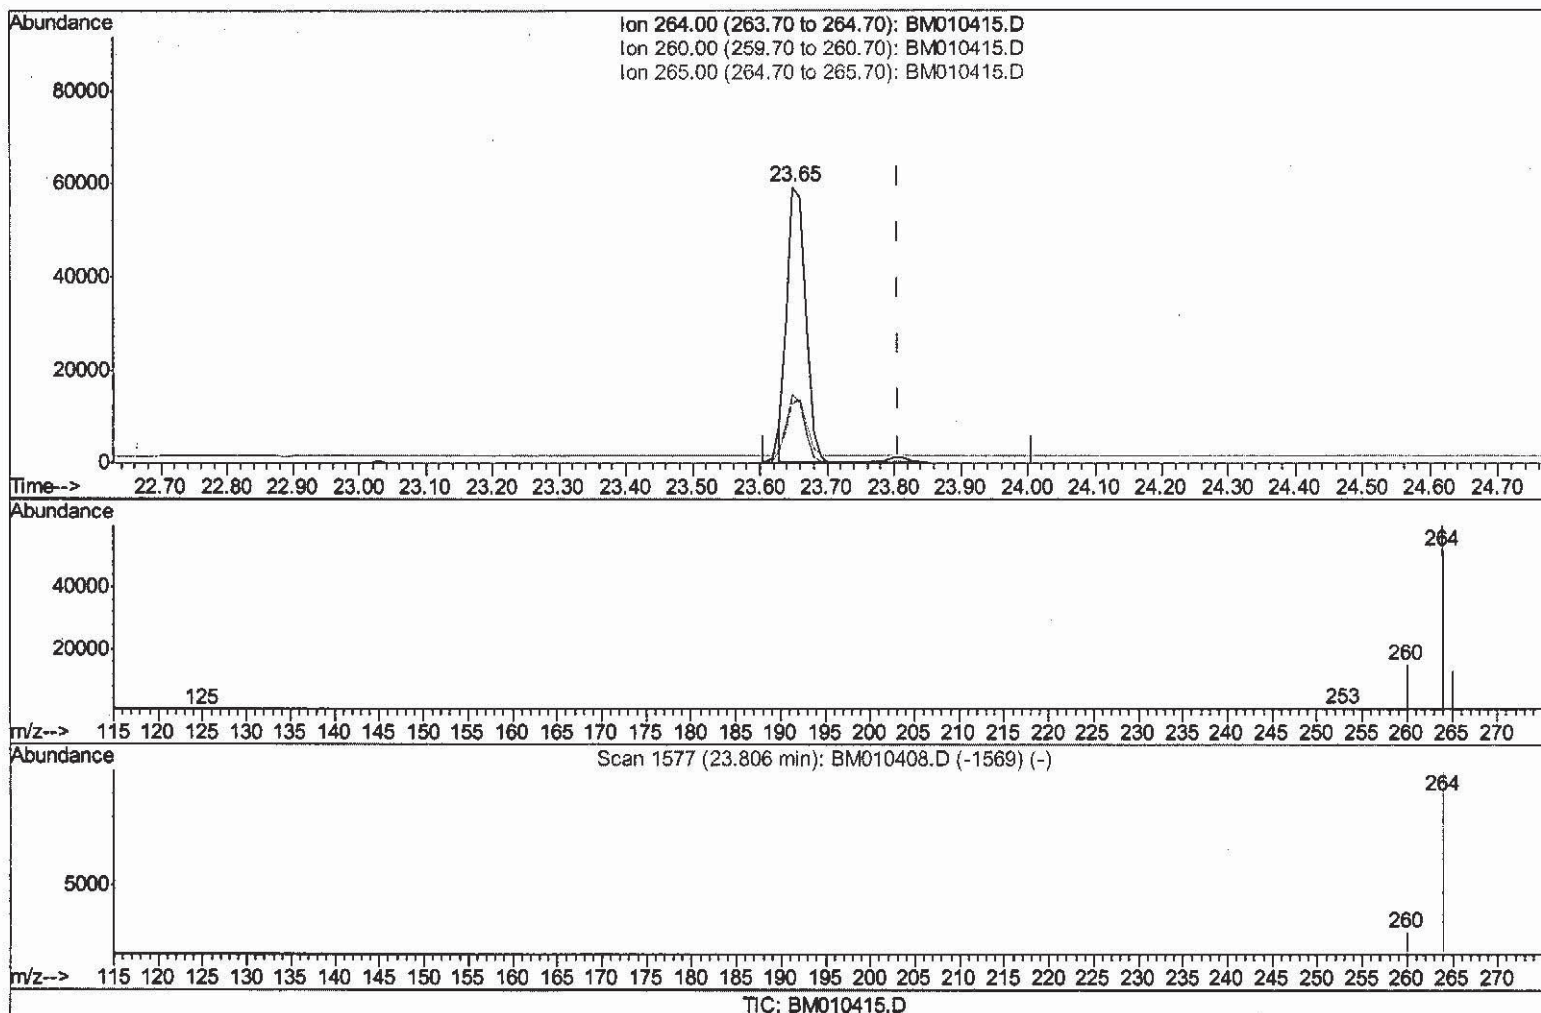

(20) Perylene-d12 (I)

23.649min (-0.157) 0.40ng/ul

response 113608

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.22
265.00	103.50	21.94#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM060517\
Data File : BM010415.D
Acq On : 05 Jun 2017 09:20
Operator : SJ/MA
Sample : I3164-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG6

Manual Integrations
APPROVED

mohammad
6/6/2017 12:24:18 PM

Quant Time: Jun 05 16:38:19 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 04:03:07 2017
Response via : Initial Calibration

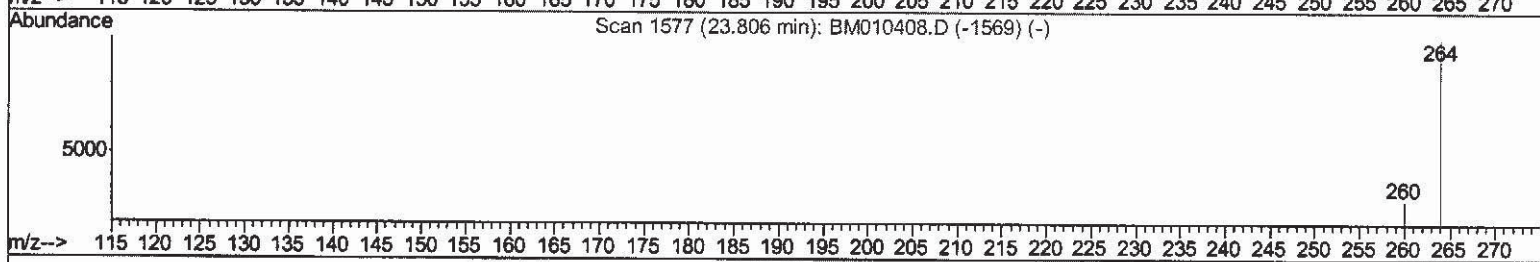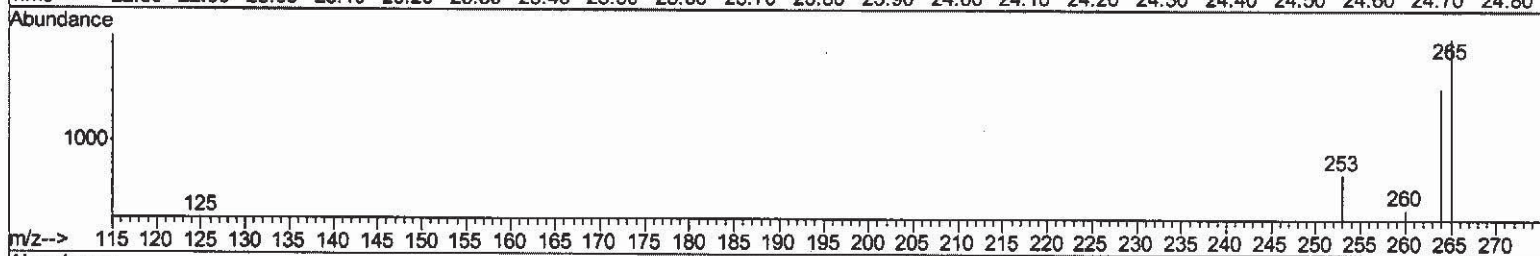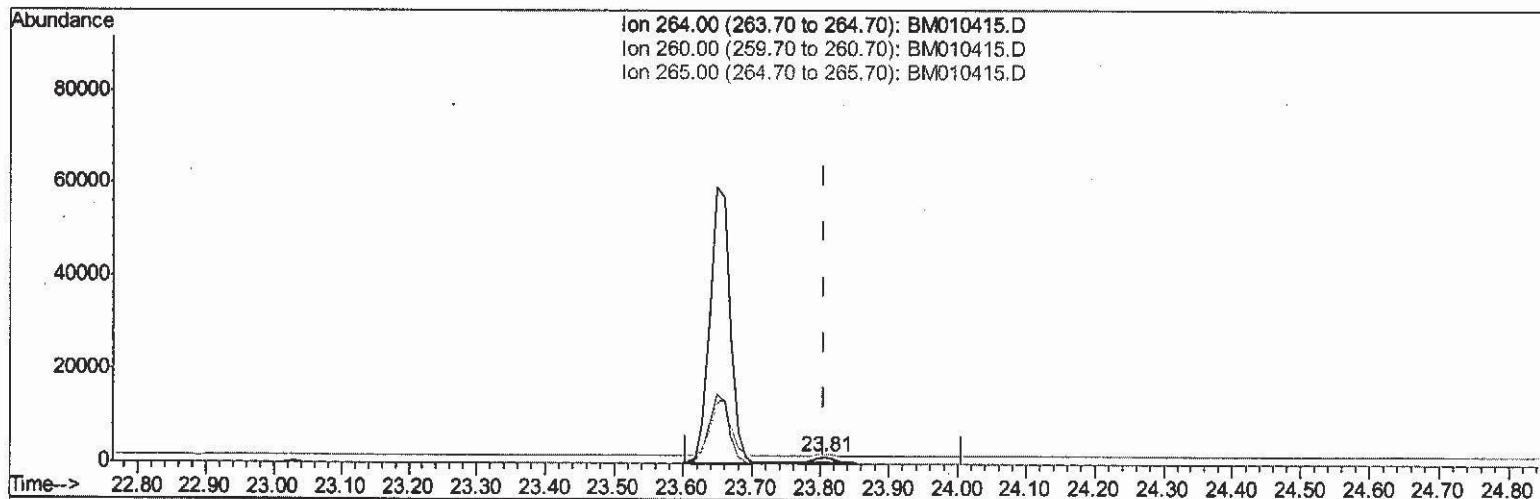

TIC: BM010415.D

(20) Perylene-d12 (I)

23.806min (-0.000) 0.40ng/ul m SJ 6/6/17

response 2605

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.90
265.00	103.50	128.36#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM060517\
Data File : BM010415.D
Acq On : 05 Jun 2017 09:20
Operator : SJ/MA
Sample : I3164-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG6

Manual Integrations
APPROVED

mohammad
6/6/2017 12:24:18 PM

Quant Time: Jun 05 18:54:51 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 04:03:07 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	712	0.40	ng/ul	0.00
2) Naphthalene-d8	10.72	136	2219	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	1216	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	2532	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	2523	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	2605m>	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	575	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	1350	0.20	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.33	178	470	0.06	ng/ul#	Ovalue 70
15) Fluoranthene	19.35	202	597	0.06	ng/ul#	57

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 6/6/17