


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060520\
 Data File : BM026272.D
 Acq On : 05 Jun 2020 10:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 18:05:40 2020

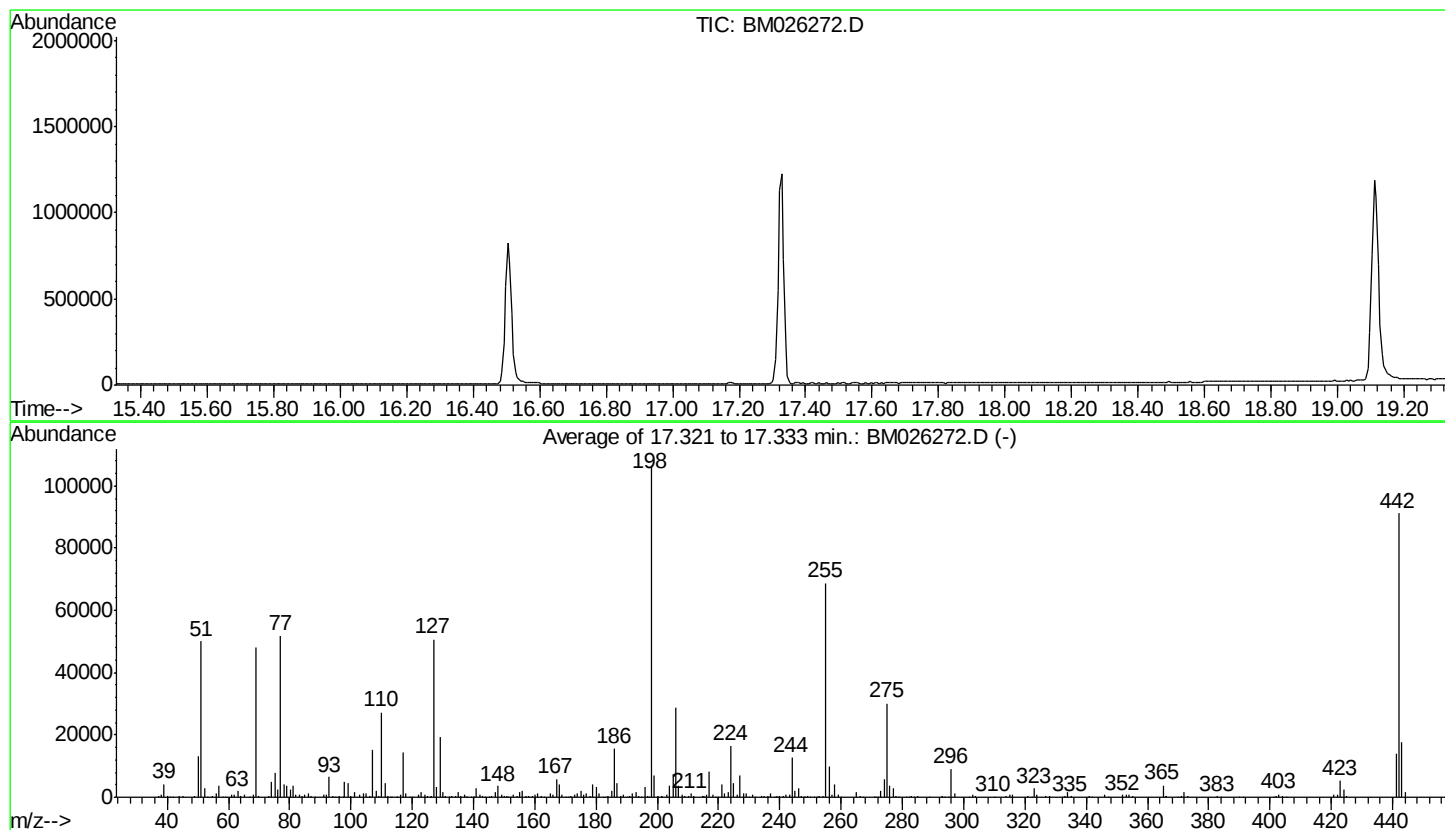

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	50036	PASS
68	69	0.00	2	1.8	879	PASS
69	198	0.00	100	45.1	48032	PASS
70	69	0.00	2	0.6	310	PASS
127	198	10	80	47.5	50578	PASS
197	198	0.00	2	0.4	405	PASS
198	198	100	100	100.0	106504	PASS
199	198	5	9	6.6	7041	PASS
275	198	10	60	28.3	30192	PASS
365	198	1	100	3.7	3919	PASS
441	198	0.01	100	13.0	13804	PASS
442	198	50	100	85.6	91210	PASS
443	442	15	24	19.4	17685	PASS