

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
 Data File : BM050197.D
 Acq On : 05 Jun 2025 11:17
 Operator : RC/JU
 Sample : SSTDICC020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC020

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 06/06/2025
 Supervised By :Jagrut Upadhyay 06/06/2025

Quant Time: Jun 05 14:58:25 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 14:55:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	277976	20.000	ng	0.00
21) Naphthalene-d8	10.575	136	1171357	20.000	ng	0.00
39) Acenaphthene-d10	14.416	164	720692	20.000	ng	0.00
64) Phenanthrene-d10	17.151	188	1364843	20.000	ng	0.00
76) Chrysene-d12	21.386	240	1240830	20.000	ng	0.00
86) Perylene-d12	24.374	264	1156806	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.369	112	662532	39.759	ng	0.00
7) Phenol-d6	6.946	99	899139	40.989	ng	0.00
23) Nitrobenzene-d5	8.934	82	917335	40.730	ng	0.00
42) 2,4,6-Tribromophenol	15.898	330	342402	41.770	ng	0.00
45) 2-Fluorobiphenyl	13.045	172	2208837	41.494	ng	0.00
79) Terphenyl-d14	19.780	244	2892092	44.169	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.293	88	143316	19.620	ng	99
3) Pyridine	3.681	79	380901	20.136	ng	99
4) n-Nitrosodimethylamine	3.593	42	77508	19.815	ng	# 97
6) Aniline	7.110	93	596745	20.578	ng	100
8) 2-Chlorophenol	7.352	128	373594	20.382	ng	99
9) Benzaldehyde	6.928	77	299039m	21.441	ng	
10) Phenol	6.975	94	475205	20.474	ng	100
11) bis(2-Chloroethyl)ether	7.210	93	383515	20.543	ng	99
12) 1,3-Dichlorobenzene	7.681	146	414543	20.230	ng	98
13) 1,4-Dichlorobenzene	7.822	146	434797	20.394	ng	99
14) 1,2-Dichlorobenzene	8.140	146	414769	20.407	ng	99
15) Benzyl Alcohol	8.022	79	320142	20.462	ng	99
16) 2,2'-oxybis(1-Chloropr...	8.316	45	270693	20.873	ng	98
17) 2-Methylphenol	8.222	107	314991	20.568	ng	97
18) Hexachloroethane	8.869	117	153532	19.885	ng	99
19) n-Nitroso-di-n-propyla...	8.593	70	297971	22.197	ng	98
20) 3+4-Methylphenols	8.546	107	426134	20.798	ng	98
22) Acetophenone	8.605	105	605945	20.706	ng	# 98
24) Nitrobenzene	8.975	77	420036	20.506	ng	97
25) Isophorone	9.504	82	802320	20.639	ng	100
26) 2-Nitrophenol	9.687	139	170594	19.294	ng	97
27) 2,4-Dimethylphenol	9.752	122	368697	20.275	ng	98
28) bis(2-Chloroethoxy)met...	9.993	93	523393	20.610	ng	99
29) 2,4-Dichlorophenol	10.222	162	338221	20.118	ng	99
30) 1,2,4-Trichlorobenzene	10.440	180	375562	20.074	ng	99
31) Naphthalene	10.628	128	1236626	20.419	ng	100
32) Benzoic acid	9.840	122	205878	18.032	ng	99
33) 4-Chloroaniline	10.728	127	531493	20.585	ng	99
34) Hexachlorobutadiene	10.922	225	221558	19.910	ng	99
35) Caprolactam	11.481	113	109175	20.483	ng	98
36) 4-Chloro-3-methylphenol	11.851	107	366554	20.433	ng	99
37) 2-Methylnaphthalene	12.240	142	752886	20.607	ng	98
38) 1-Methylnaphthalene	12.457	142	806687	20.803	ng	99
40) 1,2,4,5-Tetrachloroben...	12.610	216	421559	20.257	ng	100
41) Hexachlorocyclopentadiene	12.598	237	244251	19.326	ng	98
43) 2,4,6-Trichlorophenol	12.845	196	273306	19.971	ng	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
 Data File : BM050197.D
 Acq On : 05 Jun 2025 11:17
 Operator : RC/JU
 Sample : SSTDICC020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC020

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 06/06/2025
 Supervised By :Jagrut Upadhyay 06/06/2025

Quant Time: Jun 05 14:58:25 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 14:55:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,4,5-Trichlorophenol	12.910	196	305541	20.334	ng	98
46) 1,1'-Biphenyl	13.251	154	1091201	20.221	ng	98
47) 2-Chloronaphthalene	13.292	162	850349	20.269	ng	99
48) 2-Nitroaniline	13.481	65	181276	19.634	ng	96
49) Acenaphthylene	14.139	152	1398350	20.607	ng	99
50) Dimethylphthalate	13.875	163	1007787	20.677	ng	100
51) 2,6-Dinitrotoluene	13.981	165	204779	20.834	ng	96
52) Acenaphthene	14.481	154	854295	20.128	ng	99
53) 3-Nitroaniline	14.304	138	224884	20.528	ng	97
54) 2,4-Dinitrophenol	14.510	184	94248	19.130	ng	98
55) Dibenzofuran	14.816	168	1279459	20.605	ng	98
56) 4-Nitrophenol	14.604	139	191313	20.518	ng	100
57) 2,4-Dinitrotoluene	14.769	165	263119	20.293	ng	99
58) Fluorene	15.463	166	1004752	21.126	ng	100
59) 2,3,4,6-Tetrachlorophenol	15.034	232	266423	20.493	ng	92
60) Diethylphthalate	15.245	149	1020737	21.107	ng	99
61) 4-Chlorophenyl-phenyle...	15.463	204	480887	20.921	ng	99
62) 4-Nitroaniline	15.463	138	210030	20.456	ng	98
63) Azobenzene	15.751	77	1019944	21.101	ng	97
65) 4,6-Dinitro-2-methylph...	15.528	198	138015	18.514	ng	97
66) n-Nitrosodiphenylamine	15.669	169	872651	20.349	ng	99
67) 4-Bromophenyl-phenylether	16.351	248	293588	20.172	ng	99
68) Hexachlorobenzene	16.463	284	345929	20.343	ng	99
69) Atrazine	16.622	200	281360	20.591	ng	98
70) Pentachlorophenol	16.798	266	225494	20.396	ng	98
71) Phenanthrene	17.192	178	1583183	20.305	ng	99
72) Anthracene	17.286	178	1603637	20.560	ng	99
73) Carbazole	17.551	167	1450582	20.414	ng	99
74) Di-n-butylphthalate	18.133	149	1619797	20.950	ng	100
75) Fluoranthene	19.210	202	1679948	20.431	ng	99
77) Benzidine	19.392	184	704620	20.194	ng	99
78) Pyrene	19.569	202	1791963	21.427	ng	100
80) Butylbenzylphthalate	20.480	149	570581	20.453	ng	98
81) Benzo(a)anthracene	21.363	228	1610203	20.502	ng	100
82) 3,3'-Dichlorobenzidine	21.286	252	470294	19.636	ng	98
83) Chrysene	21.427	228	1519821	20.343	ng	99
84) Bis(2-ethylhexyl)phtha...	21.315	149	871329	20.277	ng	98
85) Di-n-octyl phthalate	22.457	149	1161953	18.223	ng	99
87) Indeno(1,2,3-cd)pyrene	27.739	276	1450383	19.472	ng	# 91
88) Benzo(b)fluoranthene	23.427	252	1393549	20.720	ng	99
89) Benzo(k)fluoranthene	23.492	252	1413975	20.594	ng	100
90) Benzo(a)pyrene	24.233	252	1284647	20.315	ng	98
91) Dibenzo(a,h)anthracene	27.809	278	1181274	19.538	ng	99
92) Benzo(g,h,i)perylene	28.791	276	1171360	19.358	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
 Data File : BM050197.D
 Acq On : 05 Jun 2025 11:17
 Operator : RC/JU
 Sample : SSTDICC020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SSTDICC020

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/06/2025

Supervised By :Jagrut Upadhyay 06/06/2025


Quant Time: Jun 05 14:58:25 2025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 05 14:55:18 2025

Response via : Initial Calibration

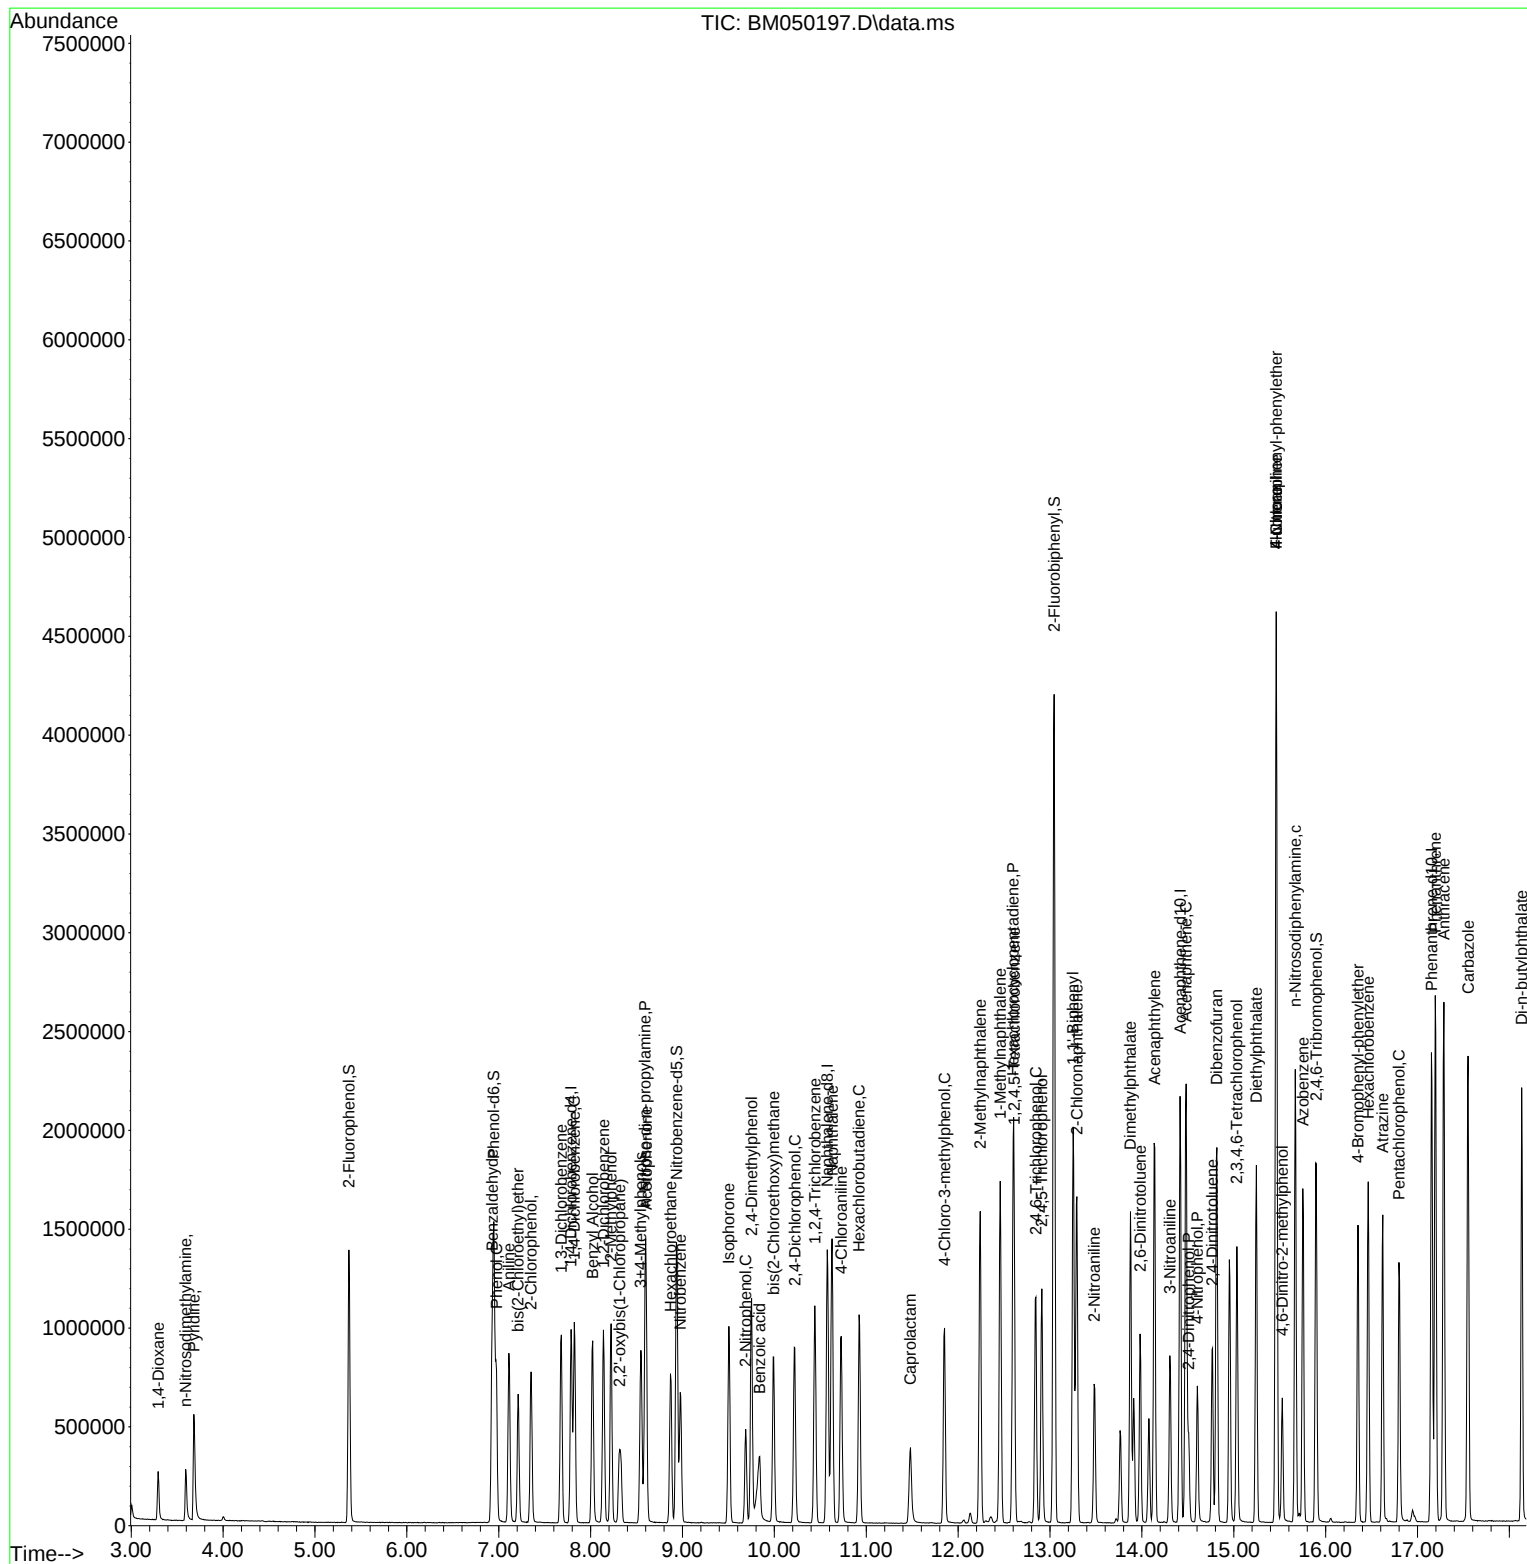

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050197.D
Acq On : 05 Jun 2025 11:17
Operator : RC/JU
Sample : SSTDICC020
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC020

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 06/06/2025
Supervised By :Jagrut Upadhyay 06/06/2025

Quant Time: Jun 05 14:58:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 14:55:18 2025
Response via : Initial Calibration

