

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
 Data File : BM050201.D
 Acq On : 05 Jun 2025 13:56
 Operator : RC/JU
 Sample : SSTDICC080
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC080

Quant Time: Jun 05 14:59:44 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 14:55:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	291644	20.000	ng	0.00
21) Naphthalene-d8	10.581	136	1166744	20.000	ng	0.00
39) Acenaphthene-d10	14.416	164	653677	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1121619	20.000	ng	0.00
76) Chrysene-d12	21.386	240	978835	20.000	ng	0.00
86) Perylene-d12	24.374	264	1062363	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	2682374	153.426	ng	0.00
7) Phenol-d6	6.957	99	3537202	153.692	ng	0.00
23) Nitrobenzene-d5	8.945	82	3567235	159.011	ng	0.00
42) 2,4,6-Tribromophenol	15.904	330	1121188	150.796	ng	0.00
45) 2-Fluorobiphenyl	13.051	172	7130886	147.690	ng	0.00
79) Terphenyl-d14	19.786	244	7496313	145.128	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.293	88	568907	74.235	ng	99
3) Pyridine	3.681	79	1547303	77.965	ng	99
4) n-Nitrosodimethylamine	3.599	42	329339	80.251	ng	97
6) Aniline	7.122	93	2369250	77.871	ng	100
8) 2-Chlorophenol	7.357	128	1502113	78.110	ng	98
10) Phenol	6.981	94	1866613	76.653	ng	100
11) bis(2-Chloroethyl)ether	7.216	93	1480567	75.590	ng	98
12) 1,3-Dichlorobenzene	7.681	146	1643168	76.431	ng	99
13) 1,4-Dichlorobenzene	7.828	146	1685110	75.334	ng	100
14) 1,2-Dichlorobenzene	8.140	146	1624137	76.165	ng	99
15) Benzyl Alcohol	8.028	79	1284953	78.279	ng	99
16) 2,2'-oxybis(1-Chloropr...	8.322	45	986129	72.476	ng	98
17) 2-Methylphenol	8.228	107	1245706	77.530	ng	100
18) Hexachloroethane	8.869	117	633589	78.215	ng	99
19) n-Nitroso-di-n-propyla...	8.604	70	1065330	75.641	ng	98
20) 3+4-Methylphenols	8.557	107	1677940	78.056	ng	100
22) Acetophenone	8.610	105	2192477	75.217	ng	100
24) Nitrobenzene	8.987	77	1617938	79.299	ng	99
25) Isophorone	9.516	82	3013669	77.831	ng	100
26) 2-Nitrophenol	9.692	139	788577	89.538	ng	98
27) 2,4-Dimethylphenol	9.757	122	1396376	77.093	ng	98
28) bis(2-Chloroethoxy)met...	9.998	93	1960708	77.513	ng	100
29) 2,4-Dichlorophenol	10.228	162	1350619	80.653	ng	99
30) 1,2,4-Trichlorobenzene	10.445	180	1456329	78.151	ng	100
31) Naphthalene	10.628	128	4521397	74.953	ng	100
32) Benzoic acid	9.916	122	1021552	89.827	ng	99
33) 4-Chloroaniline	10.734	127	1968786	76.553	ng	99
34) Hexachlorobutadiene	10.928	225	876137	79.043	ng	100
35) Caprolactam	11.522	113	417728	78.683	ng	97
36) 4-Chloro-3-methylphenol	11.857	107	1393503	77.985	ng	99
37) 2-Methylnaphthalene	12.239	142	2773230	76.205	ng	99
38) 1-Methylnaphthalene	12.463	142	2903763	75.179	ng	99
40) 1,2,4,5-Tetrachloroben...	12.610	216	1499750	79.455	ng	100
41) Hexachlorocyclopentadiene	12.598	237	1024557	89.378	ng	99
43) 2,4,6-Trichlorophenol	12.845	196	1035769	83.443	ng	100
44) 2,4,5-Trichlorophenol	12.916	196	1122919	82.394	ng	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
 Data File : BM050201.D
 Acq On : 05 Jun 2025 13:56
 Operator : RC/JU
 Sample : SSTDICC080
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC080

Quant Time: Jun 05 14:59:44 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 14:55:18 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) 1,1'-Biphenyl	13.257	154	3756723	76.752	ng	99
47) 2-Chloronaphthalene	13.292	162	2936913	77.180	ng	99
48) 2-Nitroaniline	13.486	65	725090	86.588	ng	98
49) Acenaphthylene	14.139	152	4768813	77.481	ng	100
50) Dimethylphthalate	13.886	163	3356061	75.915	ng	100
51) 2,6-Dinitrotoluene	13.986	165	743566	83.403	ng	98
52) Acenaphthene	14.486	154	2945563	76.514	ng	99
53) 3-Nitroaniline	14.316	138	820084	82.536	ng	98
54) 2,4-Dinitrophenol	14.516	184	419557	79.818	ng	95
55) Dibenzofuran	14.816	168	4229270	75.092	ng	99
56) 4-Nitrophenol	14.616	139	684831	80.978	ng	97
57) 2,4-Dinitrotoluene	14.774	165	994115	84.530	ng	97
58) Fluorene	15.463	166	3057322	70.874	ng	99
59) 2,3,4,6-Tetrachlorophenol	15.039	232	915334	77.626	ng	93
60) Diethylphthalate	15.251	149	3236518	73.786	ng	99
61) 4-Chlorophenyl-phenyle...	15.463	204	1497395	71.823	ng	98
62) 4-Nitroaniline	15.480	138	746446	80.153	ng	99
63) Azobenzene	15.757	77	3216935	73.375	ng	99
65) 4,6-Dinitro-2-methylph...	15.533	198	540790	88.276	ng	98
66) n-Nitrosodiphenylamine	15.674	169	2805368	79.603	ng	100
67) 4-Bromophenyl-phenylether	16.357	248	977940	81.762	ng	97
68) Hexachlorobenzene	16.468	284	1117623	79.976	ng	97
69) Atrazine	16.627	200	913622	81.362	ng	99
70) Pentachlorophenol	16.804	266	766580	84.374	ng	99
71) Phenanthrene	17.198	178	4793533	74.812	ng	100
72) Anthracene	17.286	178	4900912	76.458	ng	99
73) Carbazole	17.551	167	4417127	75.641	ng	100
74) Di-n-butylphthalate	18.133	149	4904225	77.184	ng	100
75) Fluoranthene	19.209	202	5027290	74.400	ng	99
77) Benzidine	19.392	184	2034794	73.924	ng	100
78) Pyrene	19.568	202	5224283	79.187	ng	99
80) Butylbenzylphthalate	20.480	149	1897236	86.212	ng	98
81) Benzo(a)anthracene	21.368	228	4797580	77.435	ng	99
82) 3,3'-Dichlorobenzidine	21.292	252	1627542	86.143	ng	100
83) Chrysene	21.433	228	4547461	77.162	ng	100
84) Bis(2-ethylhexyl)phtha...	21.321	149	2796211	82.490	ng	99
85) Di-n-octyl phthalate	22.462	149	4575834	90.971	ng	100
87) Indeno(1,2,3-cd)pyrene	27.762	276	5980793	87.435	ng	100
88) Benzo(b)fluoranthene	23.439	252	4811379	77.897	ng	99
89) Benzo(k)fluoranthene	23.503	252	4862610	77.118	ng	100
90) Benzo(a)pyrene	24.239	252	4719647	81.270	ng	100
91) Dibenzo(a,h)anthracene	27.821	278	4849919	87.349	ng	99
92) Benzo(g,h,i)perylene	28.815	276	4870648	87.646	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050201.D
Acq On : 05 Jun 2025 13:56
Operator : RC/JU
Sample : SSTDICC080
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC080

Quant Time: Jun 05 14:59:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 14:55:18 2025
Response via : Initial Calibration

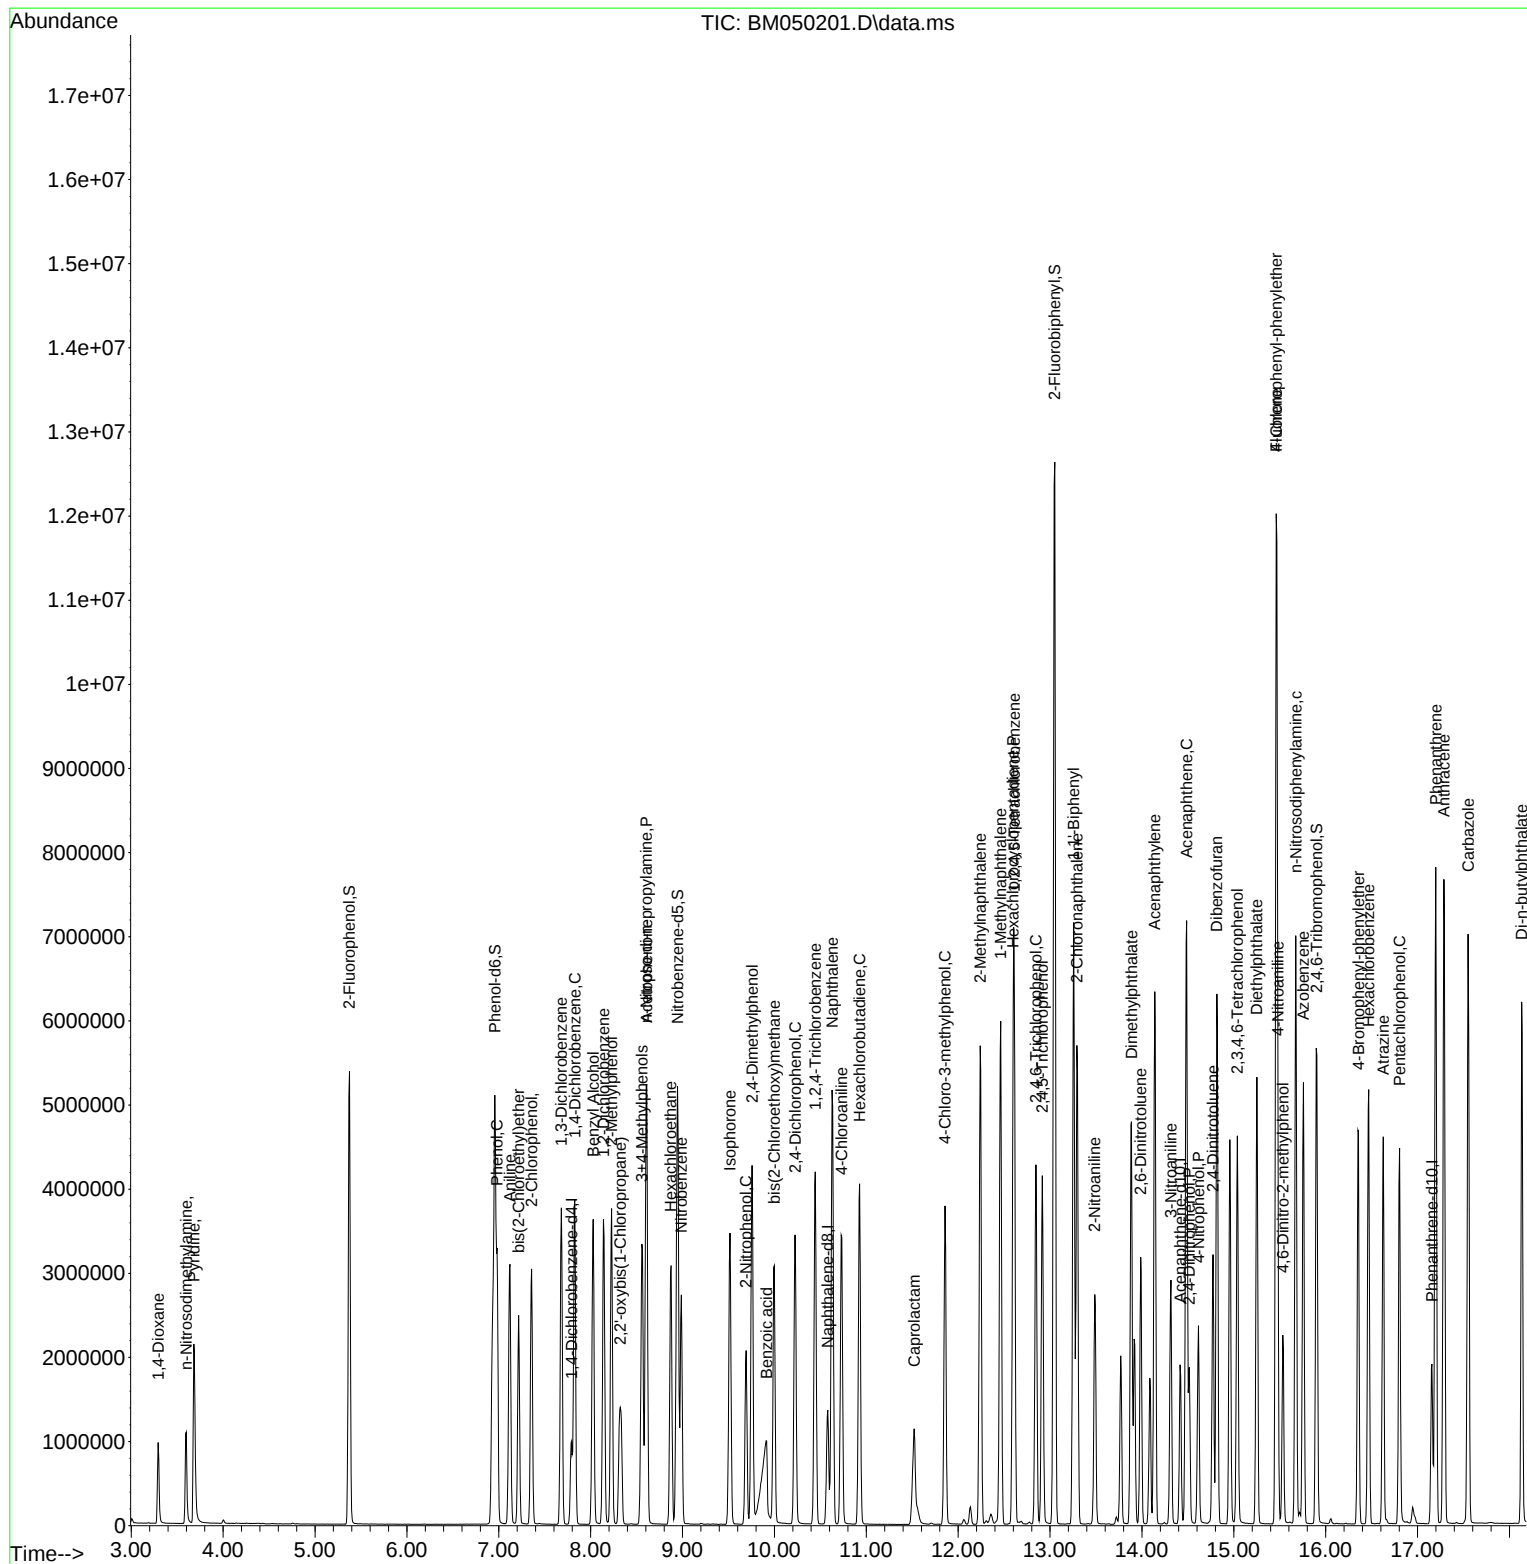

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050201.D
Acq On : 05 Jun 2025 13:56
Operator : RC/JU
Sample : SSTDICC080
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC080

Quant Time: Jun 05 14:59:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 14:55:18 2025
Response via : Initial Calibration

