
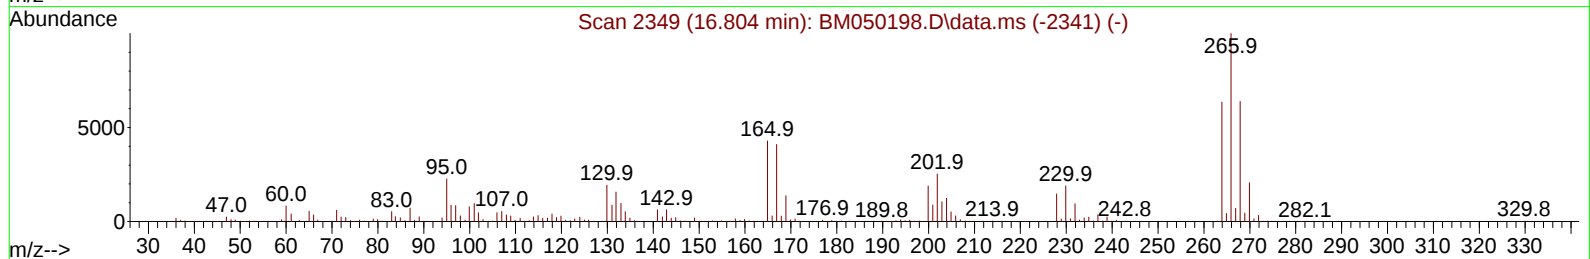
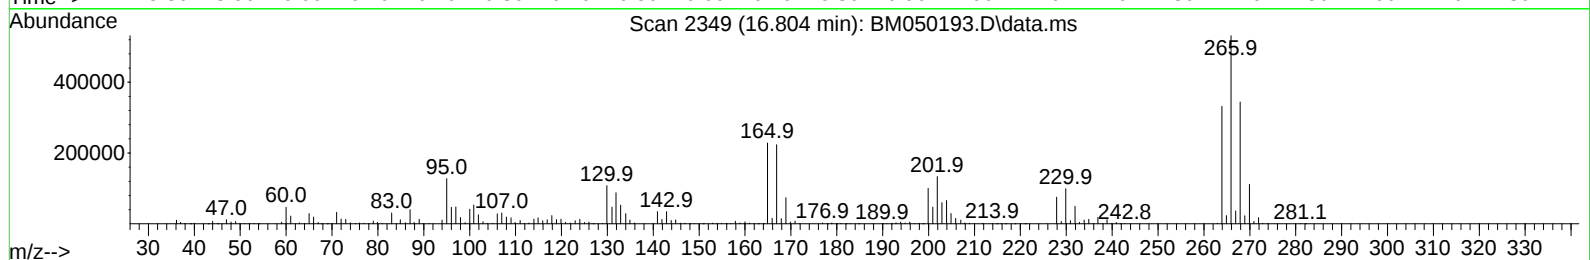


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050193.D
Acq On : 05 Jun 2025 08:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 16:27:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

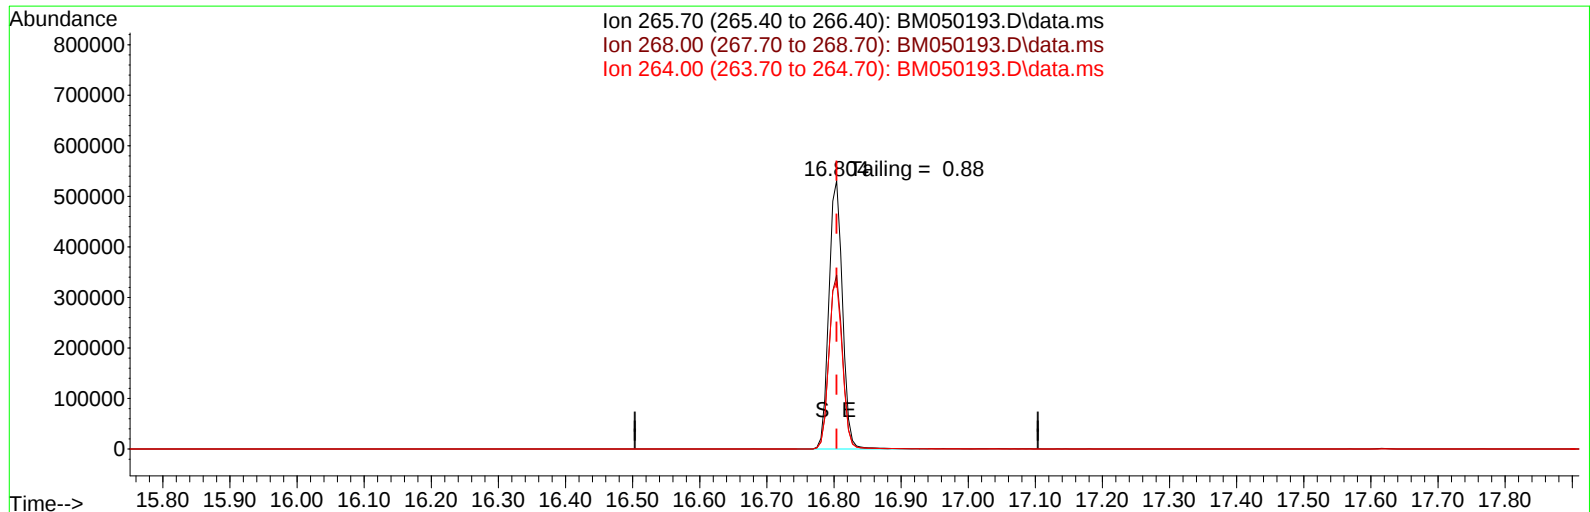

TIC: BM050193.D\data.ms

(70) Pentachlorophenol (C)




16.804min (+ 0.000) 1708888.69 ng

response 747502

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.80
264.00	63.50	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050193.D
Acq On : 05 Jun 2025 08:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 16:27:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

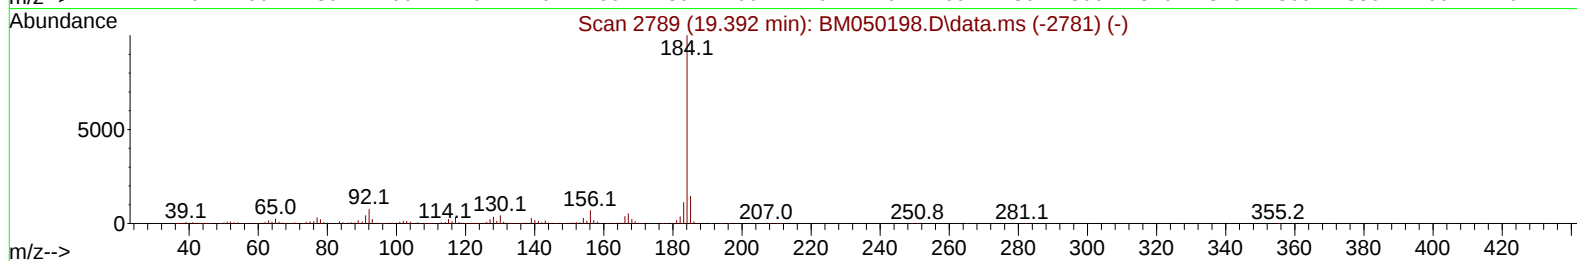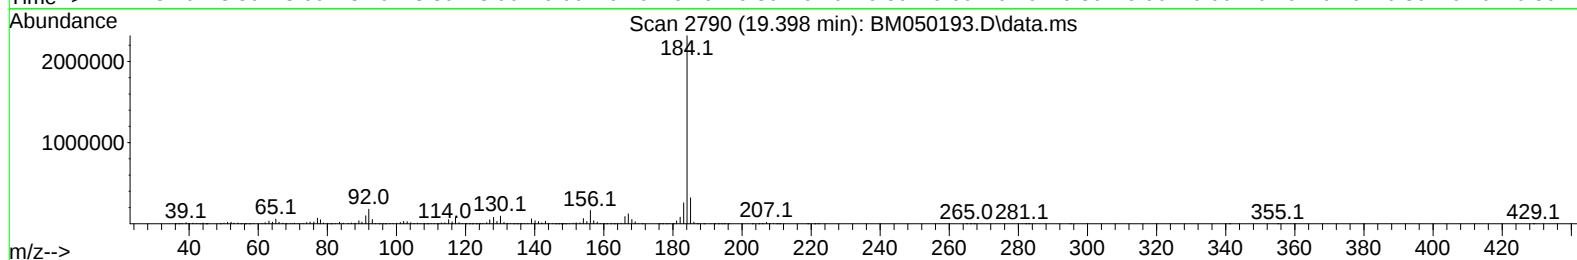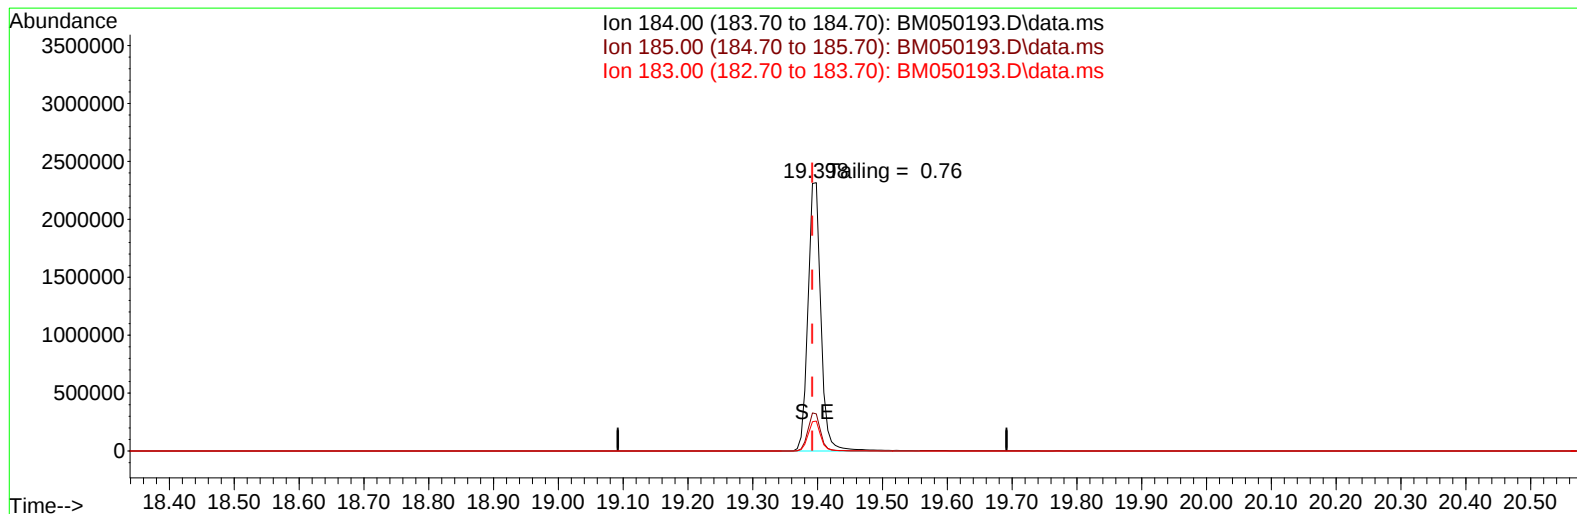

TIC: BM050193.D\data.ms

(77) Benzidine**19.398min (+ 0.006) 33233.28 ng****response 3215775**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.84
183.00	11.20	11.16
0.00	0.00	0.00