



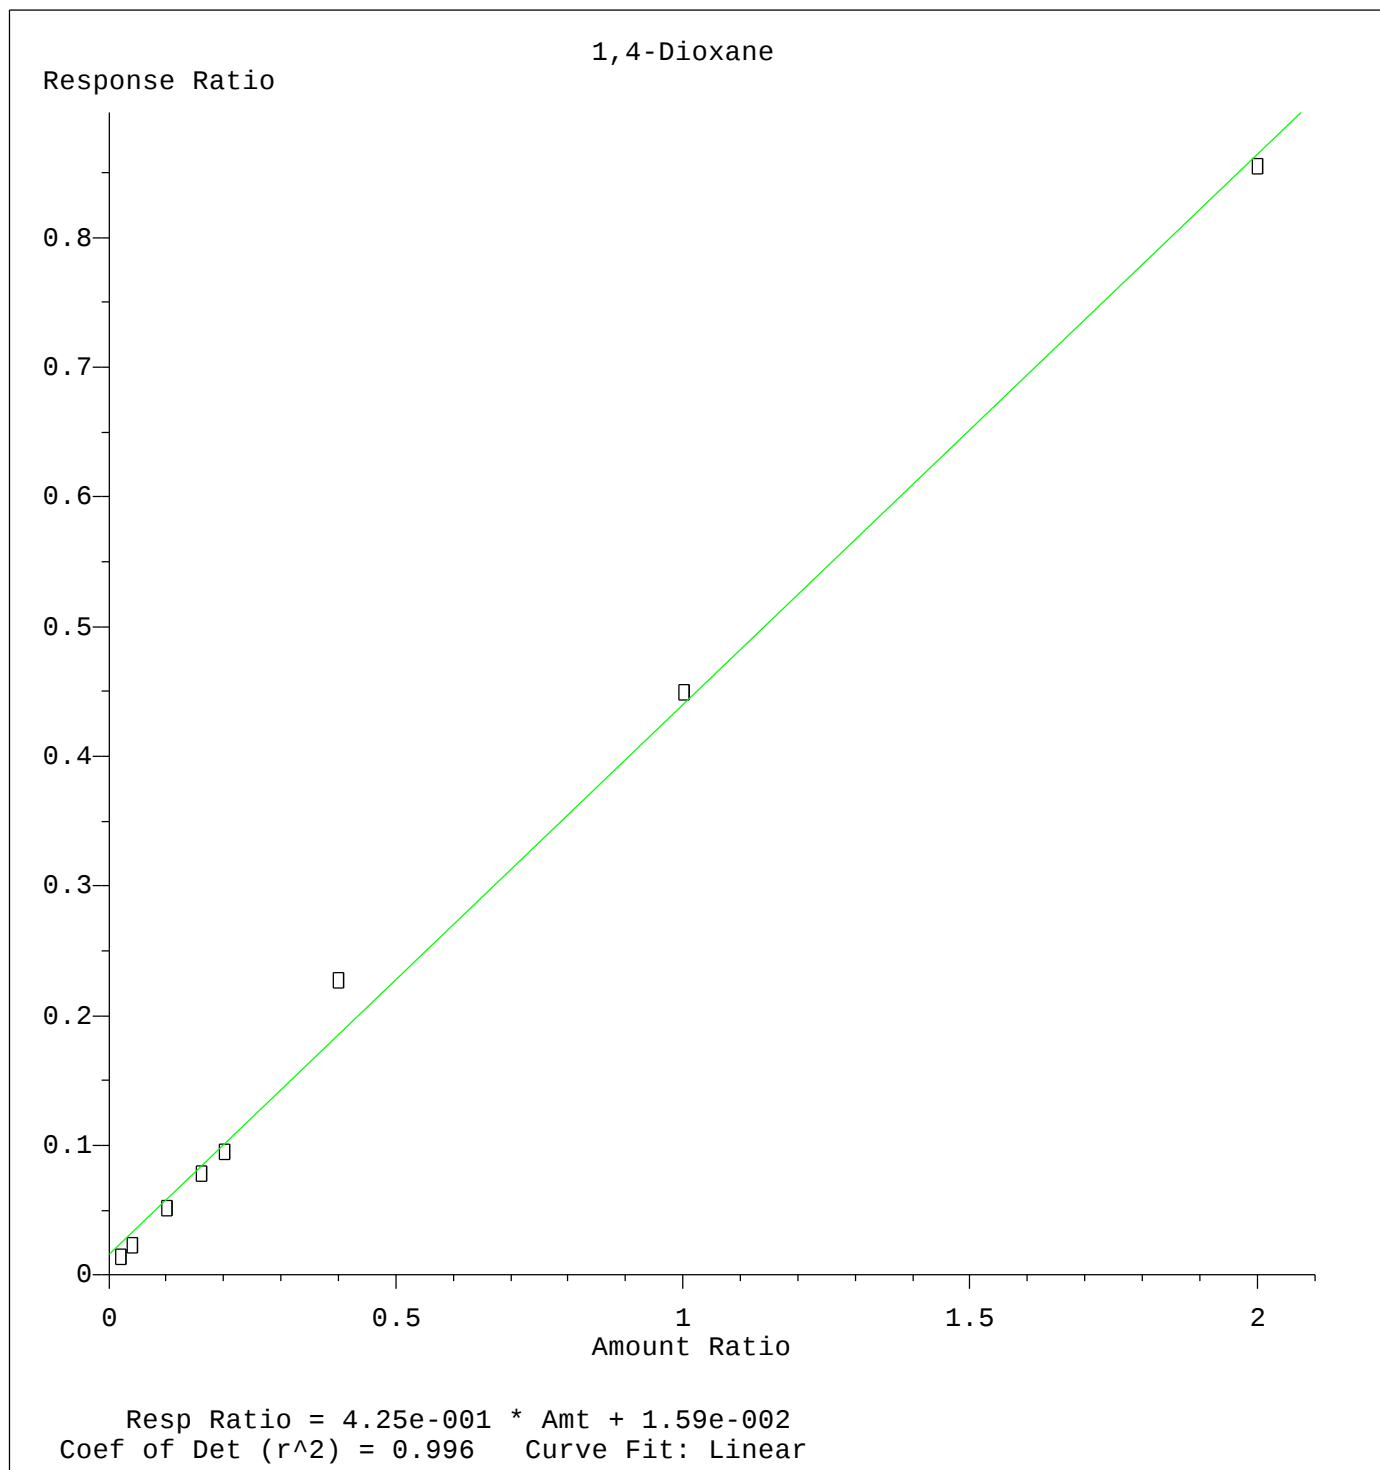


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
Calibration Table Last Updated: Mon Jun 08 05:27:25 2015

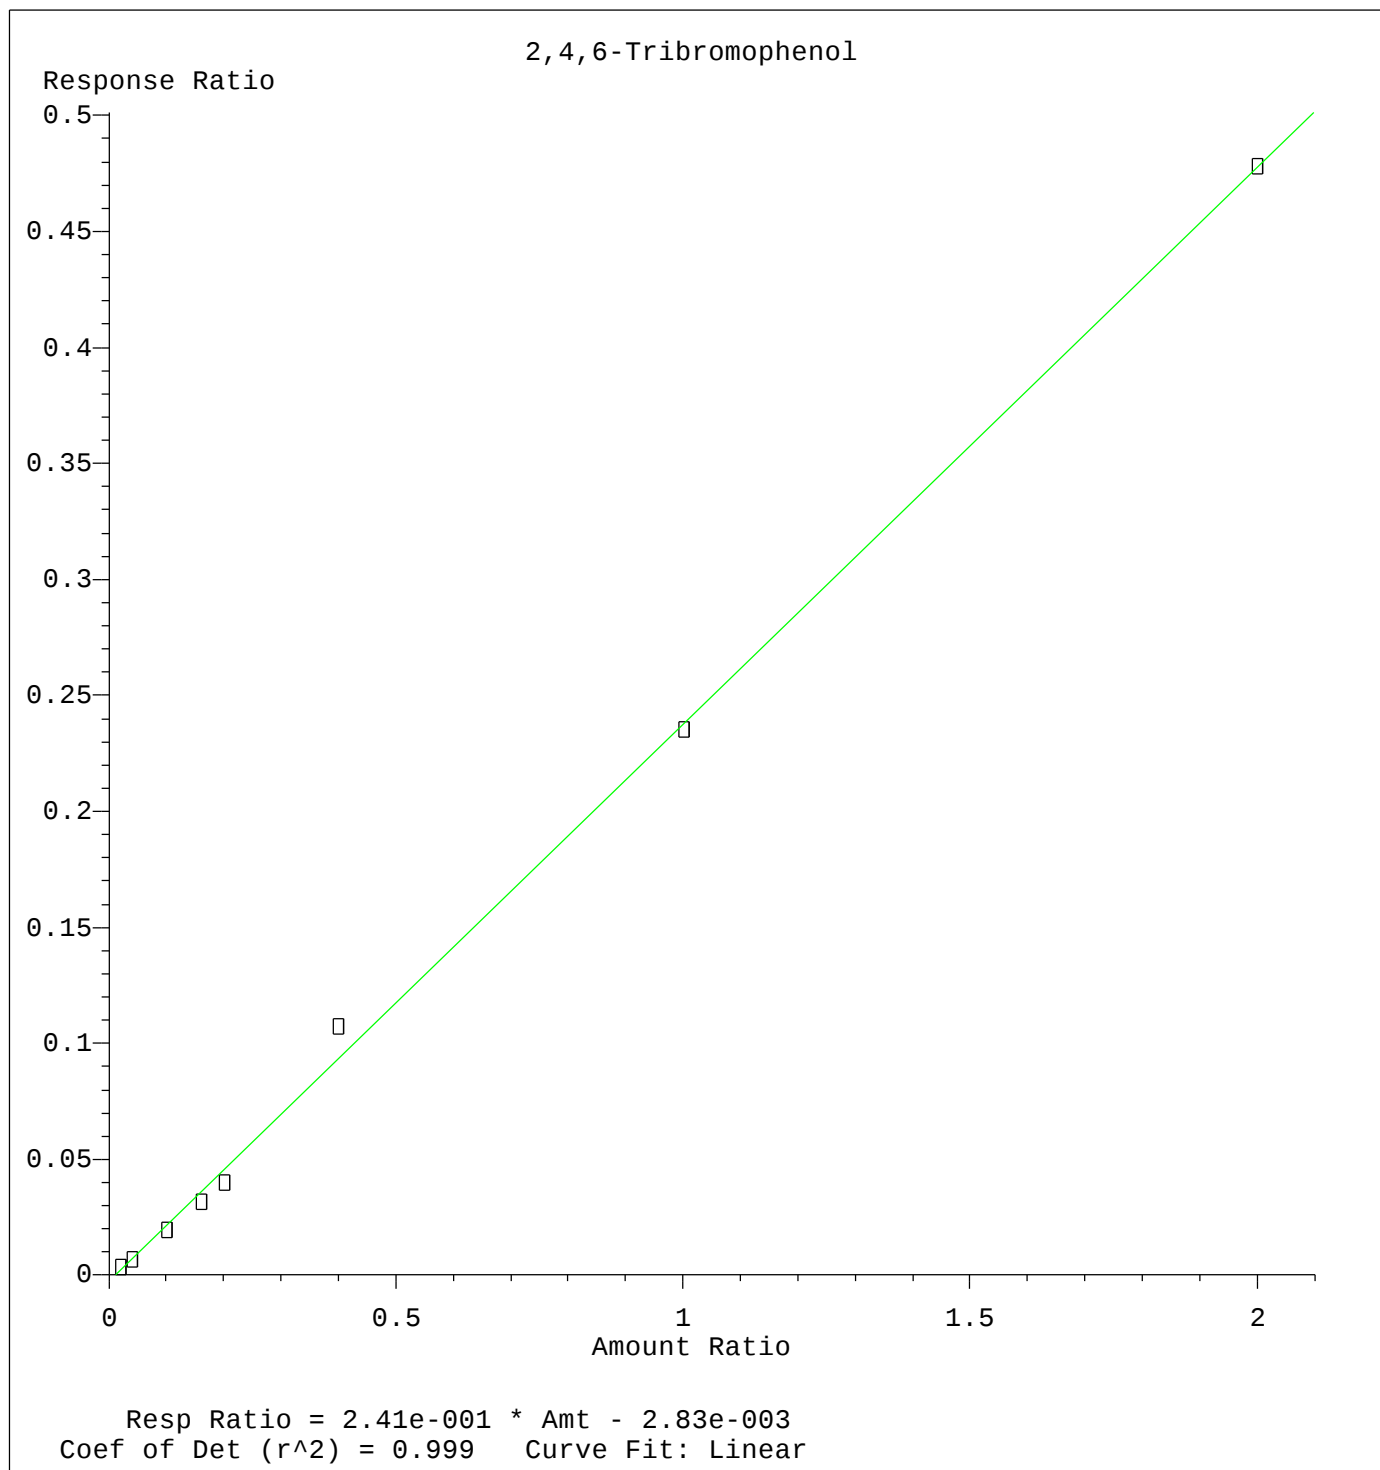


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
Calibration Table Last Updated: Mon Jun 08 05:27:25 2015

4-Bromophenyl-phenylether

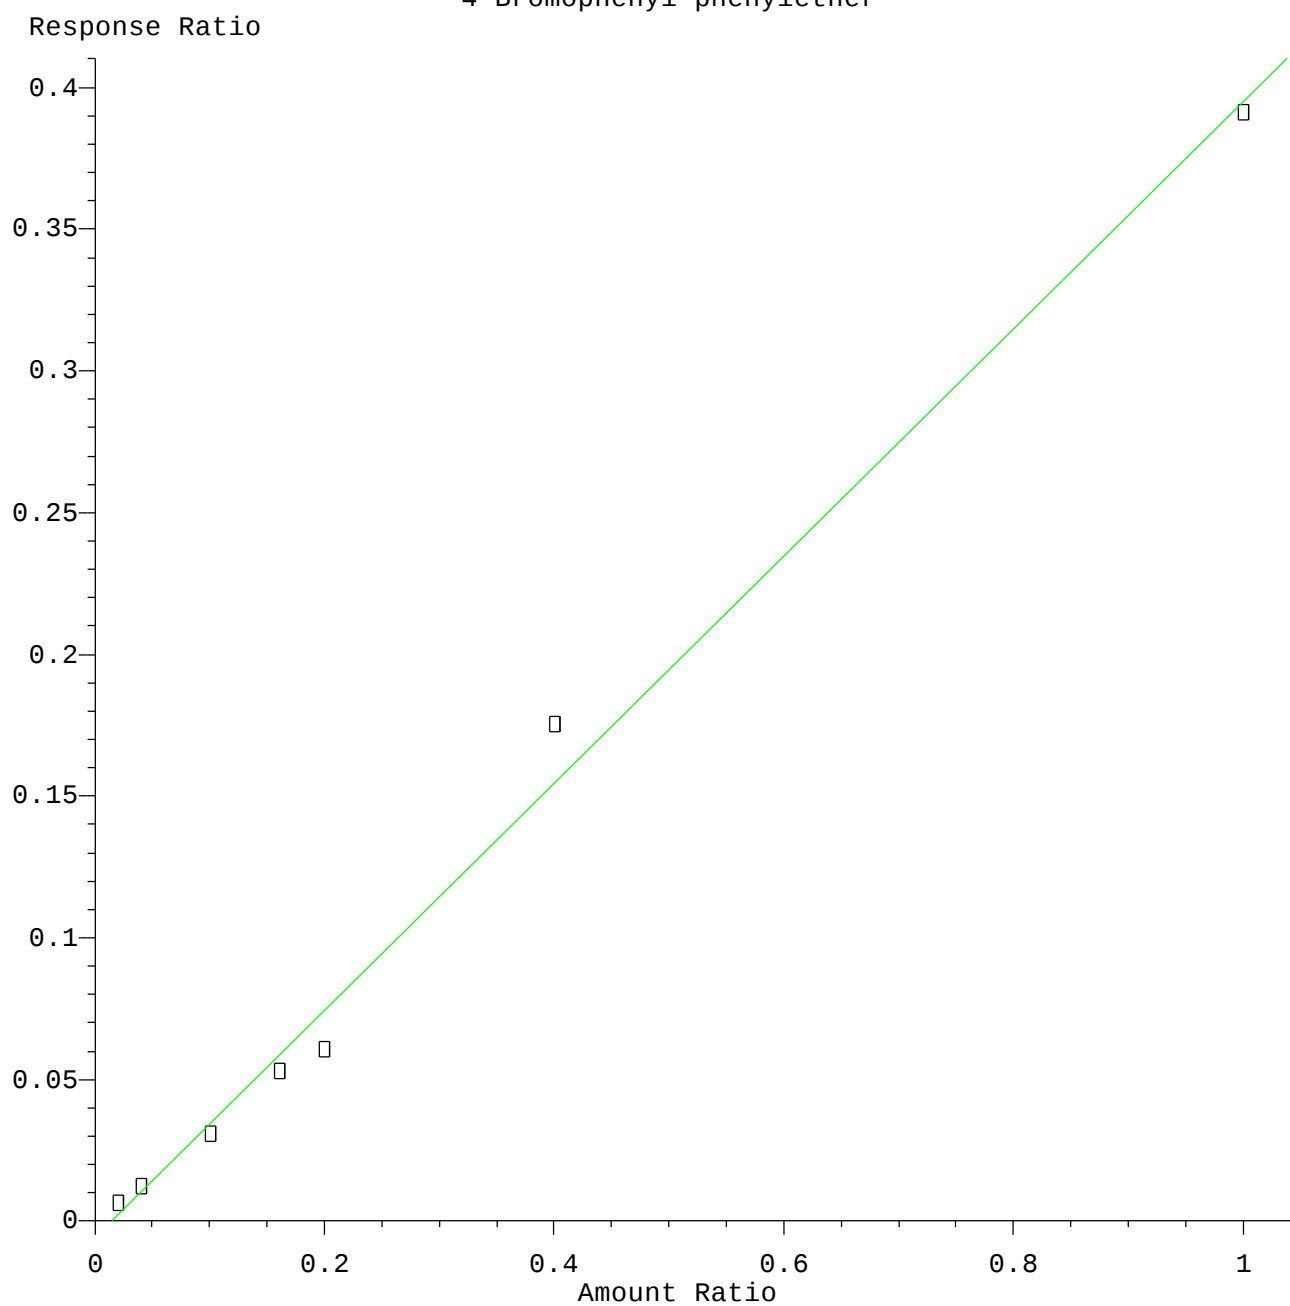

Resp Ratio = $4.02e-001 * \text{Amt} - 6.08e-003$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
Calibration Table Last Updated: Mon Jun 08 05:27:25 2015

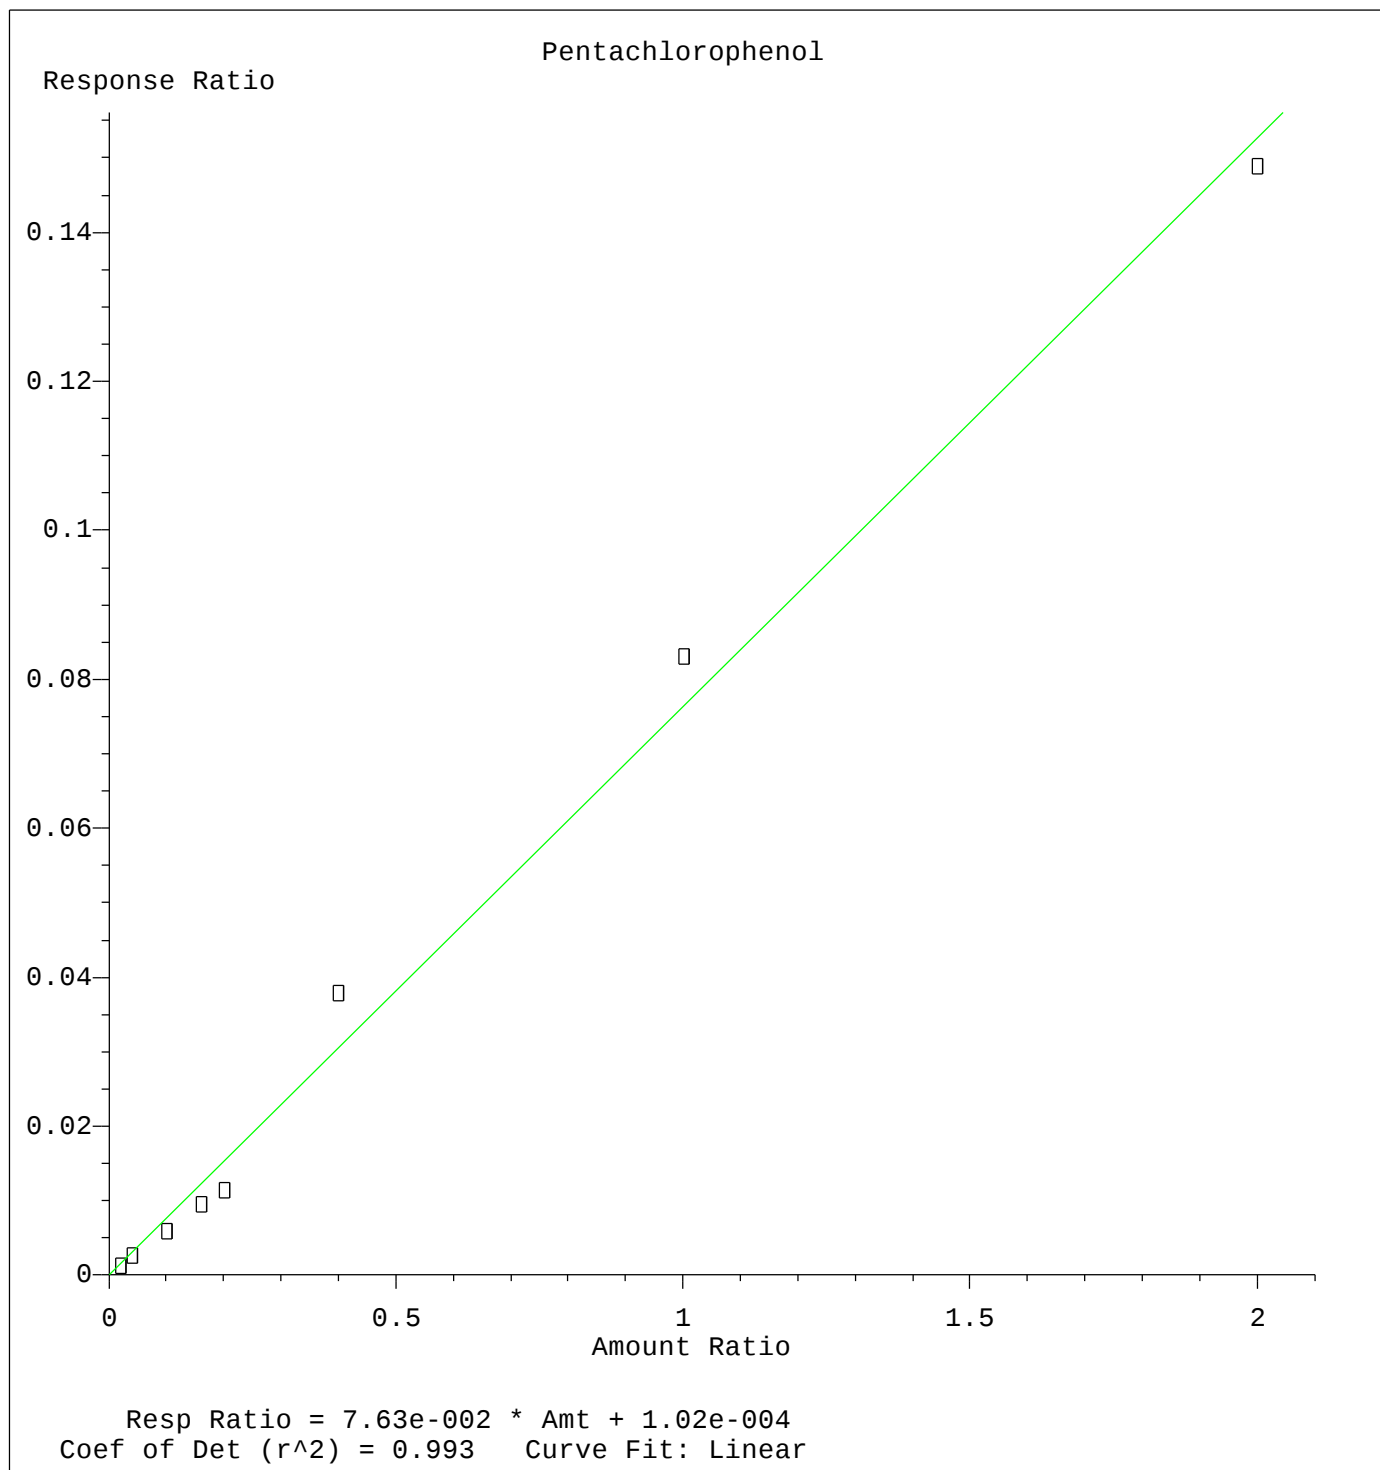

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
Calibration Table Last Updated: Mon Jun 08 05:27:25 2015

Bis(2-ethylhexyl)phthalate

Response Ratio

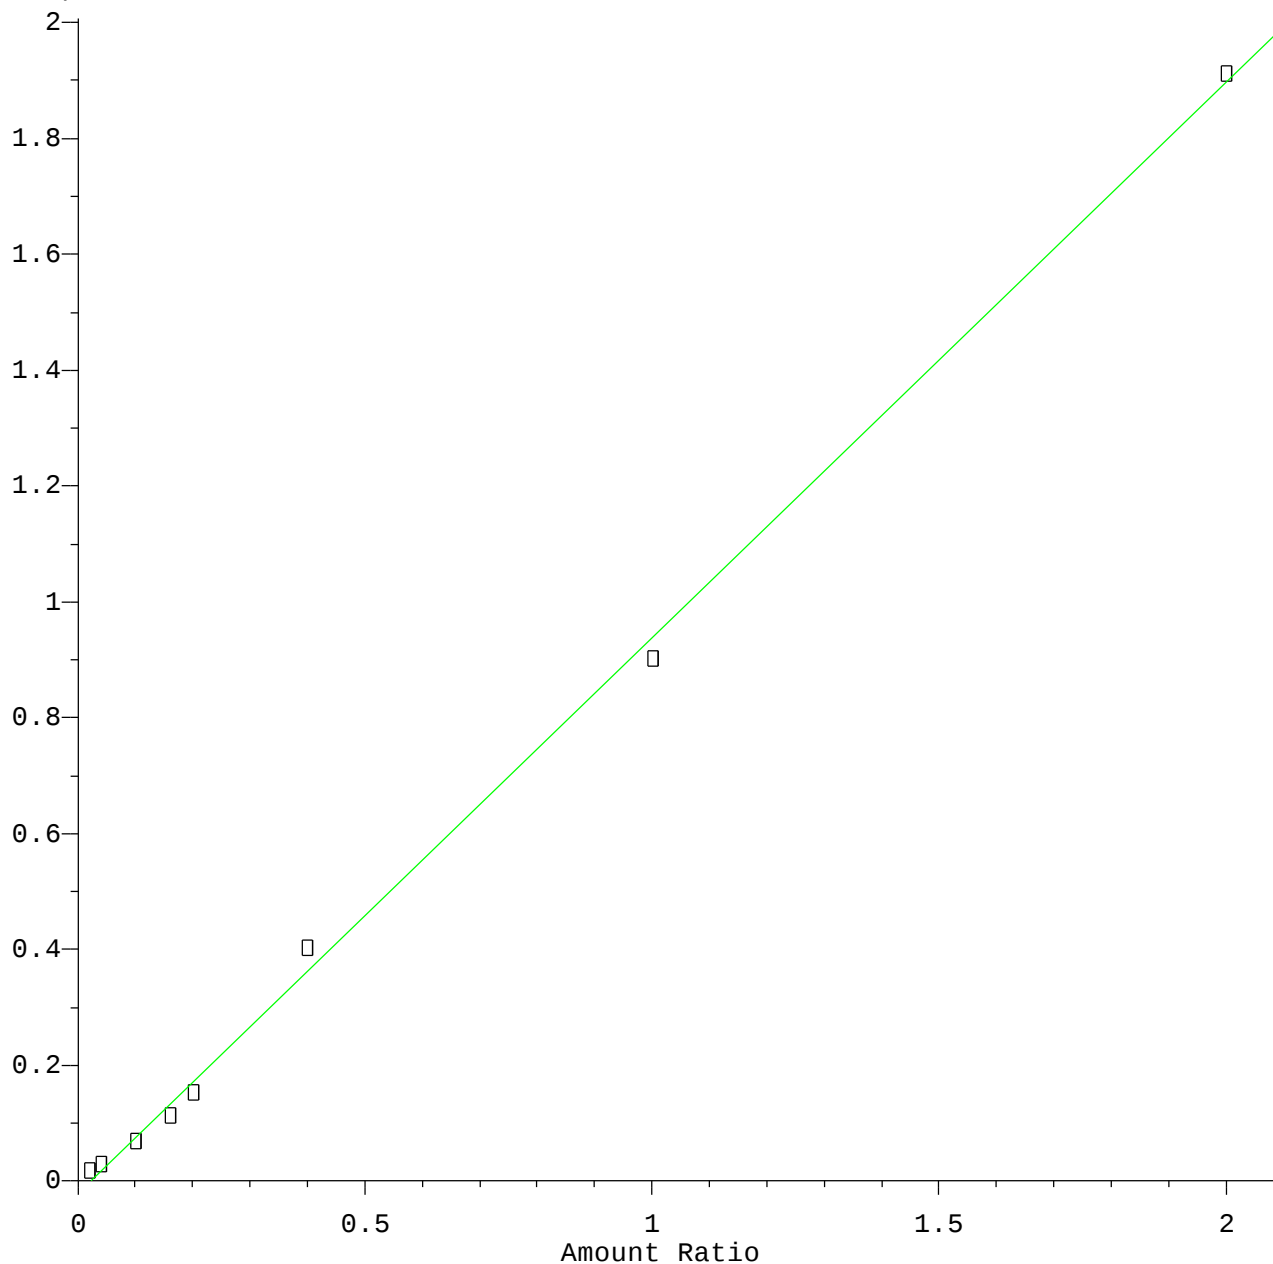

Resp Ratio = $9.59 \times 10^{-1} \times \text{Amt} - 2.07 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
Calibration Table Last Updated: Mon Jun 08 05:27:25 2015