


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060615\
 Data File : BM001567.D
 Acq On : 05 Jun 2015 15:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 05:27:25 2015

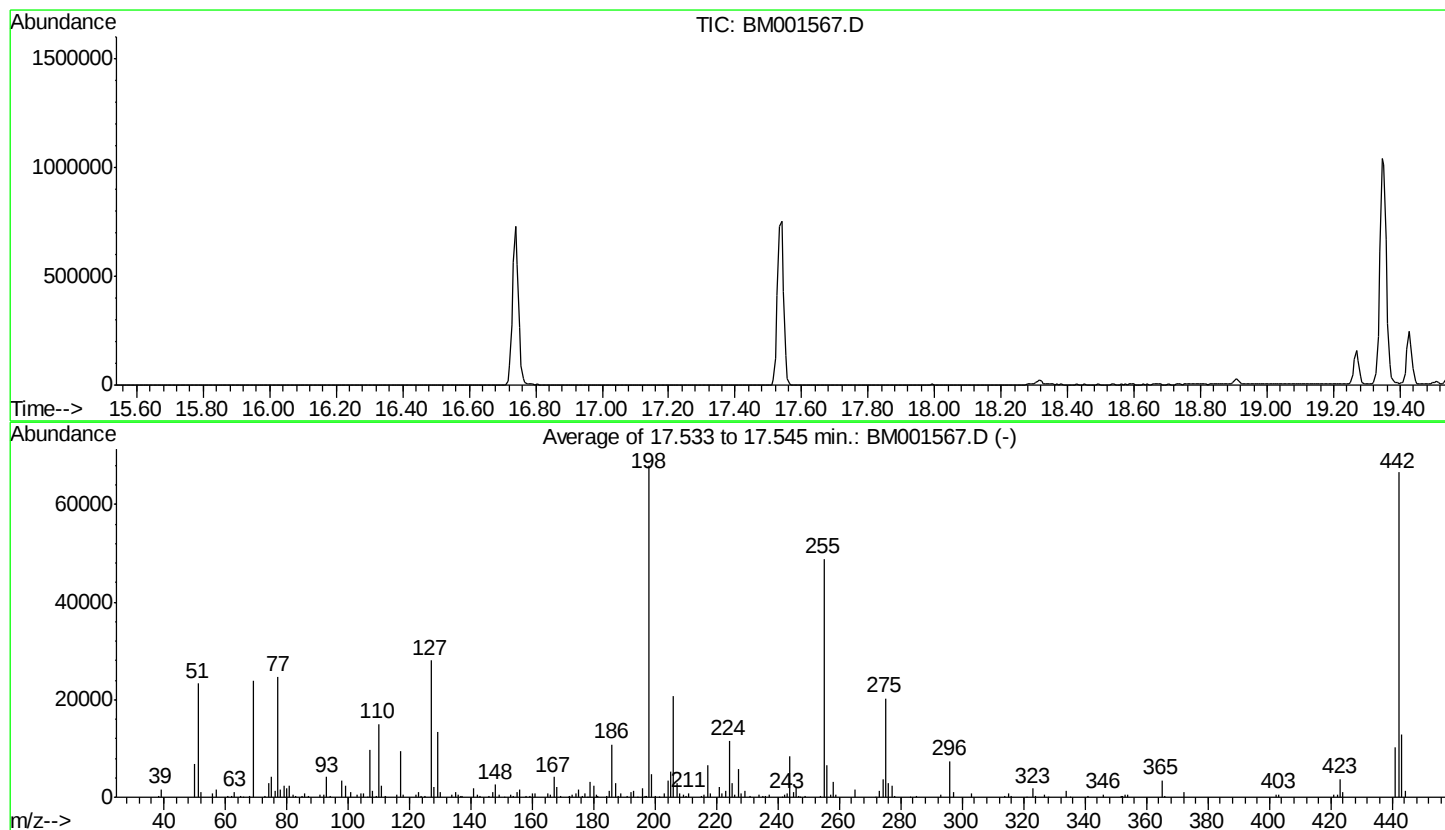

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	23342	PASS
68	69	0.00	2	1.7	403	PASS
69	198	0.00	100	35.2	23927	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	27970	PASS
197	198	0.00	2	0.5	357	PASS
198	198	100	100	100.0	67954	PASS
199	198	5	9	6.9	4685	PASS
275	198	10	60	29.9	20322	PASS
365	198	1	100	5.2	3533	PASS
441	442	0.01	24	15.5	10354	PASS
442	198	50	100	98.1	66693	PASS
443	442	15	24	19.2	12800	PASS