


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060615\
Data File : BM001577.D
Acq On : 06 Jun 2015 03:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 08 05:27:25 2015

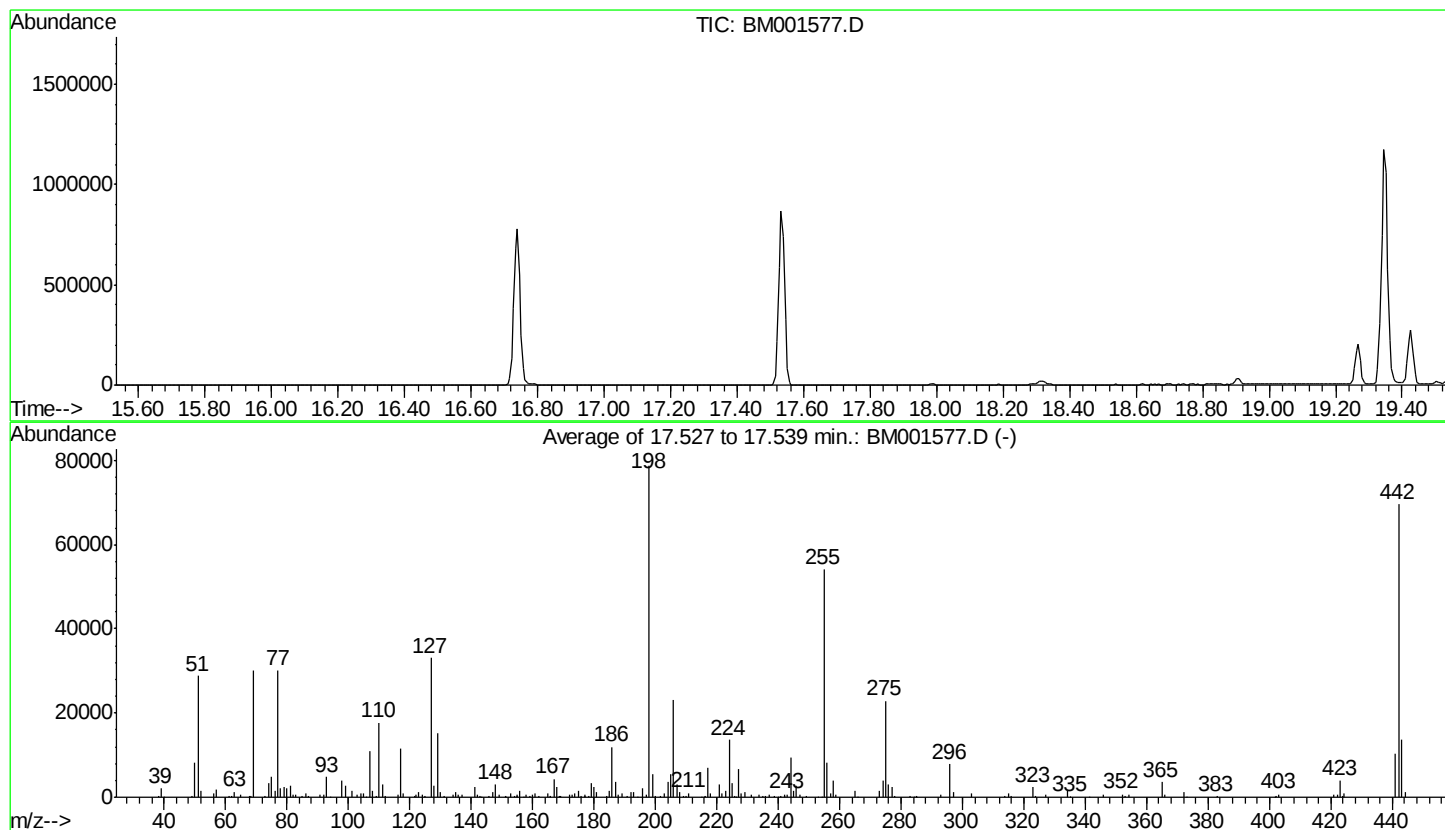

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	28866	PASS
68	69	0.00	2	1.3	397	PASS
69	198	0.00	100	38.2	30064	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	33010	PASS
197	198	0.00	2	0.7	519	PASS
198	198	100	100	100.0	78778	PASS
199	198	5	9	7.0	5480	PASS
275	198	10	60	29.0	22832	PASS
365	198	1	100	4.5	3529	PASS
441	442	0.01	24	14.9	10371	PASS
442	198	50	100	88.2	69504	PASS
443	442	15	24	19.7	13679	PASS