

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060616\
 Data File : BM005678.D
 Acq On : 06 Jun 2016 20:14
 Operator : UM/SJ
 Sample : H3412-05MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XS5MS

Manual Integrations
 APPROVED

sohil
 6/7/2016 7:13:51 PM

Quant Time: Jun 07 04:59:10 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM060216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 07 04:25:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	109887	20.00	ng/ul	0.00
7) Naphthalene-d8	10.55	136	446732	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.40	164	213376	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.14	188	421378	20.00	ng/ul	0.00
29) Chrysene-d12	21.33	240	432434	20.00	ng/ul	0.00
34) Perylene-d12	23.59	264	459592	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.22	96	4161	1.59	ng/uL	0.00
3) Phenol-d5	6.94	99	123669	12.80	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.09	67	96730	16.45	ng/ul	0.00
5) 2-Chlorophenol-d4	7.29	132	116932	14.67	ng/ul	0.00
6) 4-Methylphenol-d8	8.47	113	54516	7.13	ng/ul	0.00
8) Nitrobenzene-d5	8.92	128	57475	16.75	ng/ul	0.00
9) 2-Nitrophenol-d4	9.64	143	59166	16.12	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.18	165	91642	14.05	ng/ul	0.00
12) 4-Chloroaniline-d4	10.69	131	87389	11.27	ng/ul	0.00
16) Dimethylphthalate-d6	13.81	166	290865	17.73	ng/ul	0.00
17) Acenaphthylene-d8	14.09	160	372805	17.47	ng/ul	0.00
20) 4-Nitrophenol-d4	14.63	143	17420	7.42	ng/ul	0.00
21) Fluorene-d10	15.39	176	251141	17.83	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.53	200	16239	8.18	ng/ul	0.00
26) Anthracene-d10	17.24	188	349070	17.44	ng/ul	0.00
30) Pyrene-d10	19.54	212	380575	17.51	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.44	264	374457	17.70	ng/ul	0.00

Target Compounds

						Qvalue
18) Acenaphthylene	14.12	152	33420	1.51	ng/ul	100
19) Acenaphthene	14.46	153	233804	16.32	ng/ul	96
25) Phenanthrene	17.19	178	97932	4.21	ng/ul	99
27) Anthracene	17.28	178	31900	1.35	ng/ul	98
28) Fluoranthene	19.20	202	215500	9.06	ng/ul	99
31) Pyrene	19.57	202	632265	23.17	ng/ul	97
32) Benzo(a)anthracene	21.31	228	143620	5.66	ng/ul	96
33) Chrysene	21.36	228	152247	6.35	ng/ul	95
35) Benzo(b)fluoranthene	22.91	252	304969	11.00	ng/ul#	98
36) Benzo(k)fluoranthene	22.95	252	87505m	3.37	ng/ul	
38) Benzo(a)pyrene	23.49	252	172106	6.45	ng/ul	98
39) Indeno(1,2,3-cd)pyrene	25.87	276	147665	4.68	ng/ul	96
40) Dibenzo(a,h)anthracene	25.87	278	43388	1.64	ng/ul#	86
41) Benzo(g,h,i)perylene	26.57	276	144066	5.44	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060616\
Data File : BM005678.D
Acq On : 06 Jun 2016 20:14
Operator : UM/SJ
Sample : H3412-05MS
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9XS5MS

Manual Integrations
APPROVED

sohil
6/7/2016 7:13:51 PM

Quant Time: Jun 07 04:59:10 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM060216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 07 04:25:20 2016
Response via : Initial Calibration

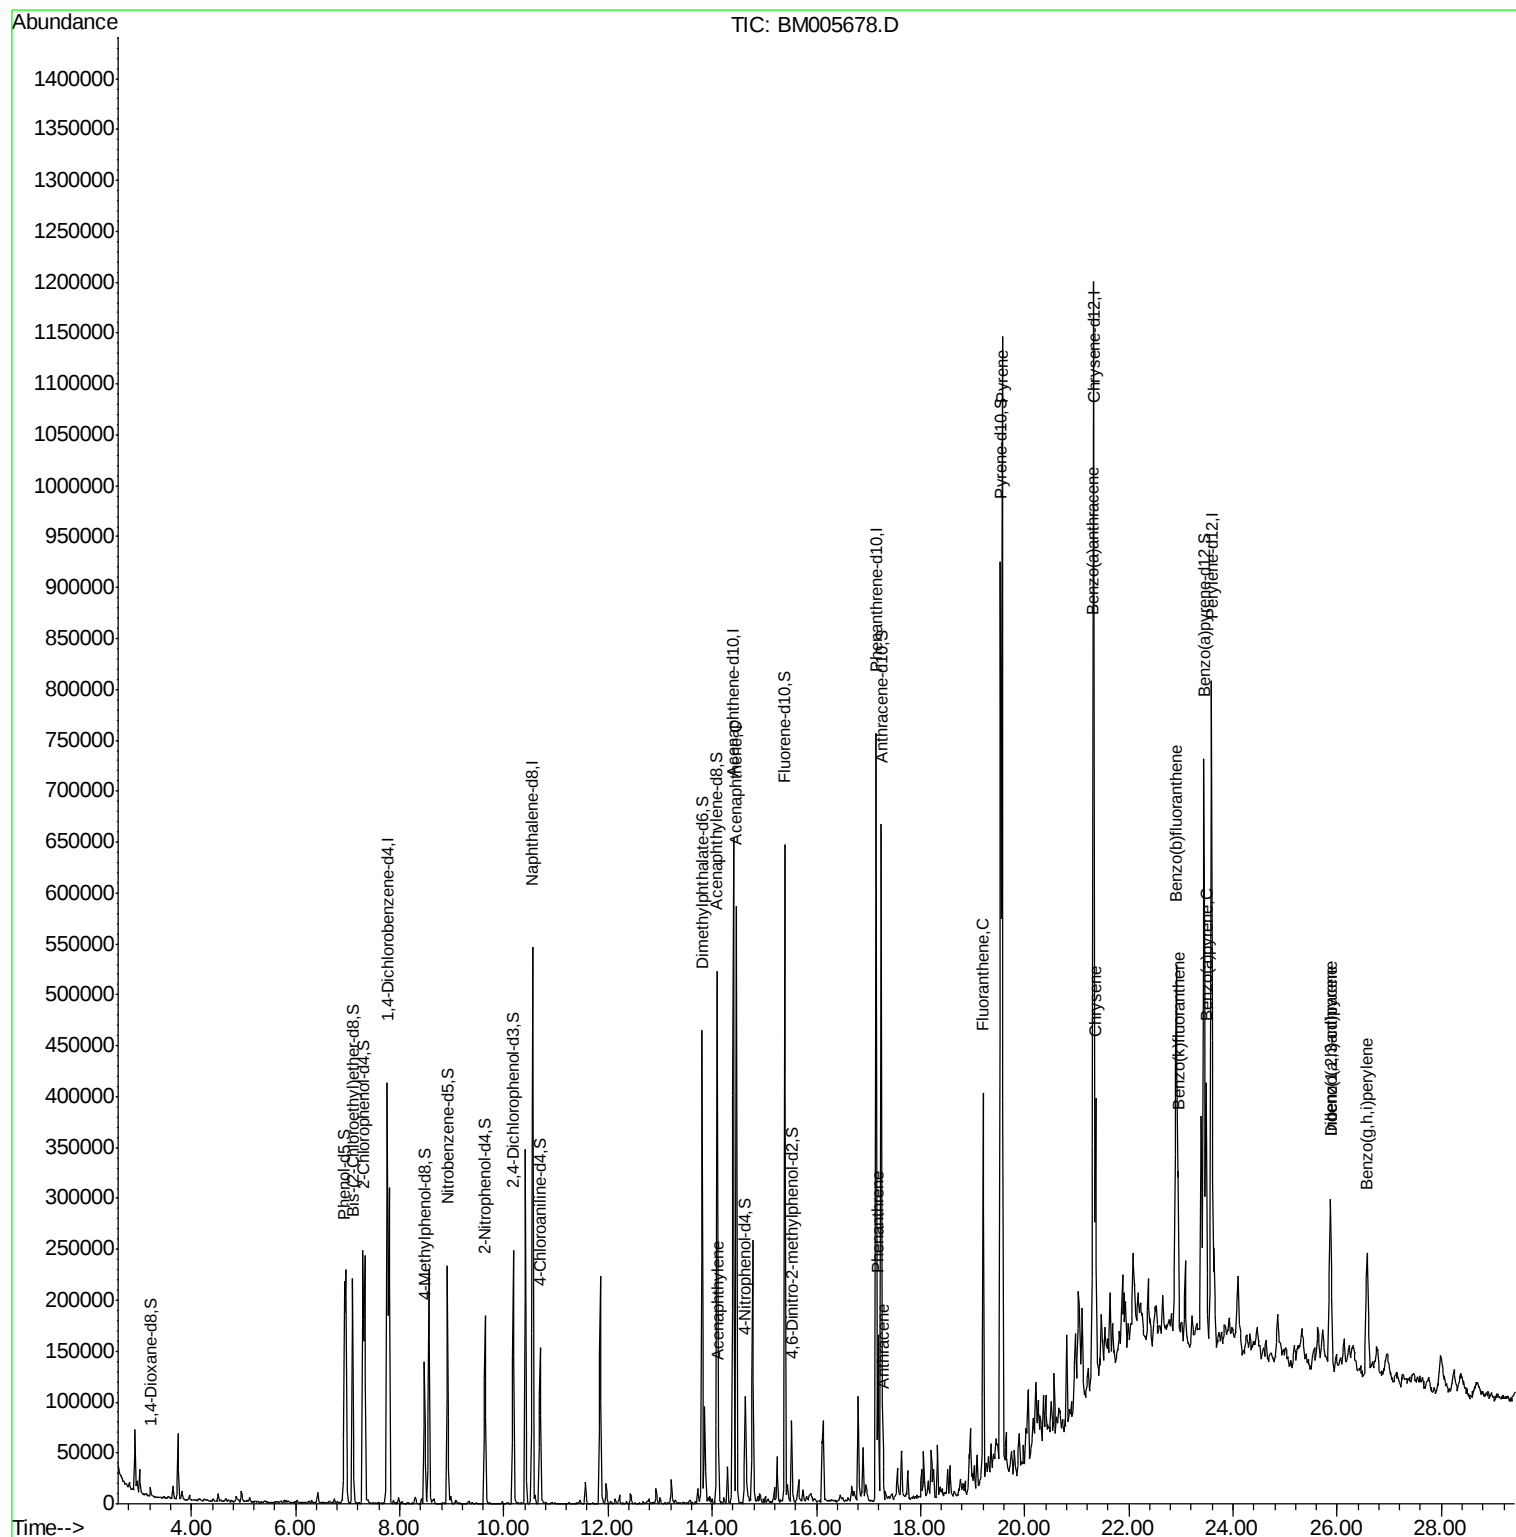







#18
Acenaphthylene
Concen: 1.51 ng/ul
RT: 14.12 min Scan# 1961
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Instrument :
BNA_M
ClientSampled :
D9XS5MS

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	33420		
151	21.6	17.3	25.9	
153	14.3	11.1	16.7	




Manual Integrations
APPROVED


sohil
6/7/2016 7:13:51 PM

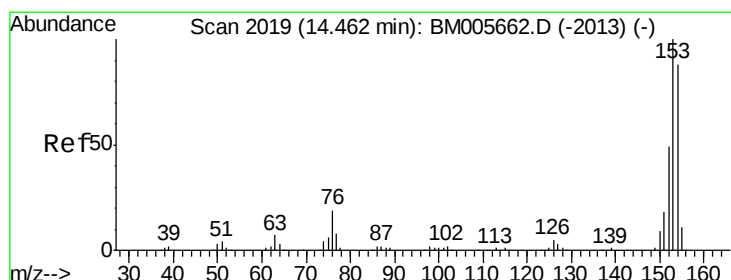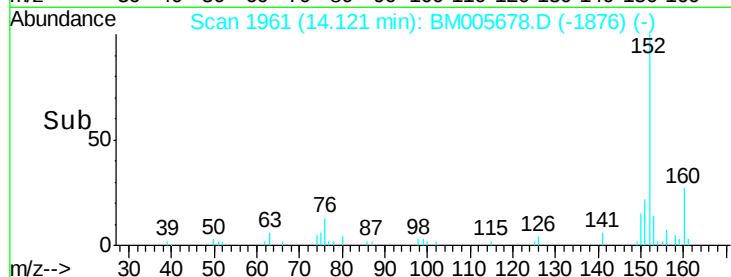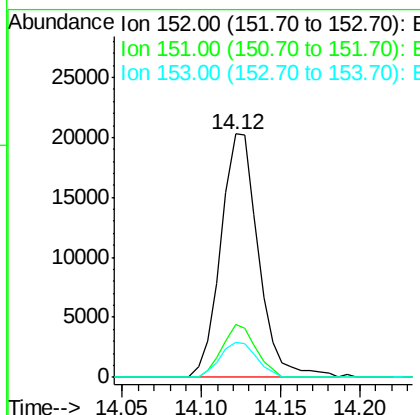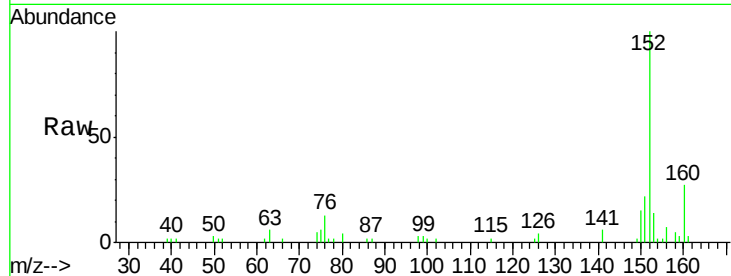

#19
Acenaphthene
Concen: 16.32 ng/ul
RT: 14.46 min Scan# 2019
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	233804		
152	48.1	36.5	54.7	
154	87.7	67.3	100.9	

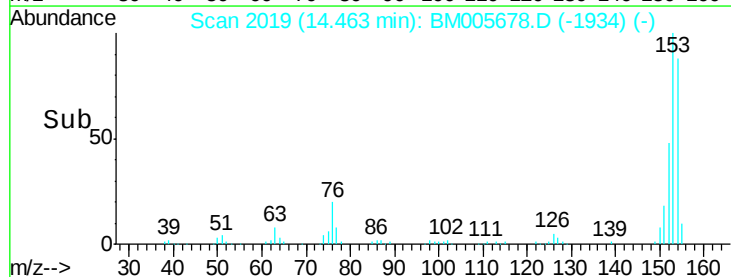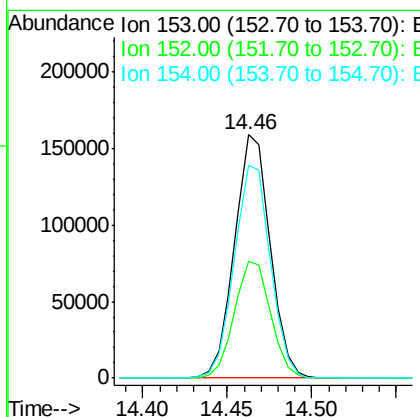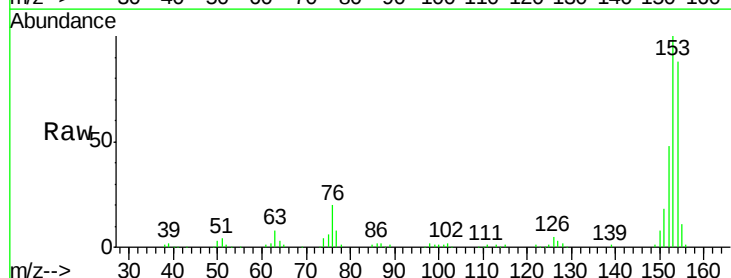







#25
Phenanthrene
Concen: 4.21 ng/ul
RT: 17.19 min Scan# 2482
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Instrument :
BNA_M
ClientSampleId :
D9XS5MS

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.2	11.8	17.8
176	18.9	14.8	22.2




Manual Integrations
APPROVED


sohil
6/7/2016 7:13:51 PM

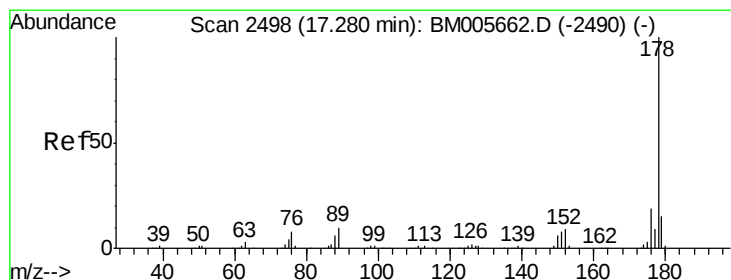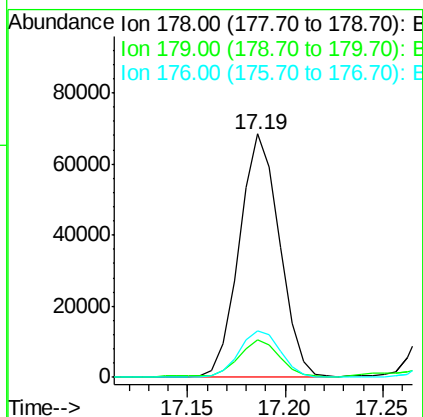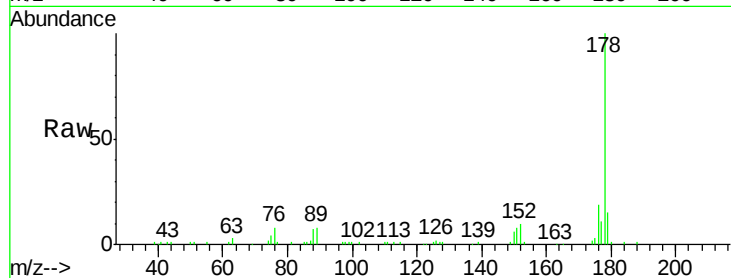

#27
Anthracene
Concen: 1.35 ng/ul
RT: 17.28 min Scan# 2498
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.7	12.9	19.3
176	18.6	15.6	23.4

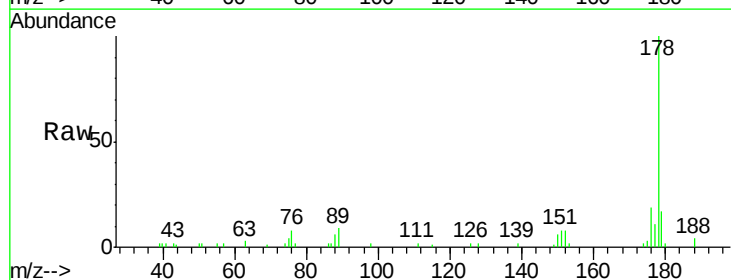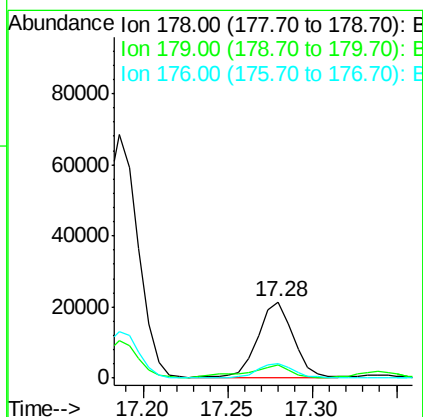



#28

Fluoranthene

Concen: 9.06 ng/ul

RT: 19.20 min Scan# 2825

Delta R.T. 0.00 min

Lab File: BM005678.D


Acq: 06 Jun 2016 20:14

Instrument :

BNA_M

ClientSampleId :




D9XS5MS

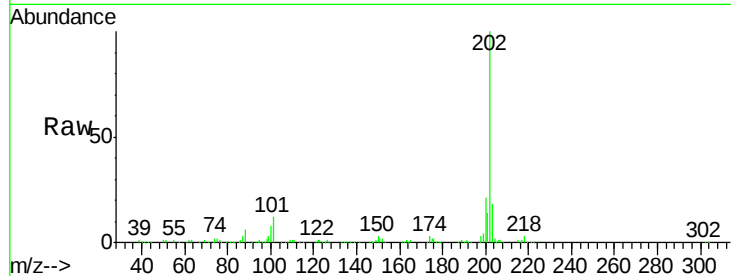

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	215500		
101	11.8	8.9	13.3	
100	8.4	7.0	10.4	

Manual Integrations
APPROVED

sohil
6/7/2016 7:13:51 PM

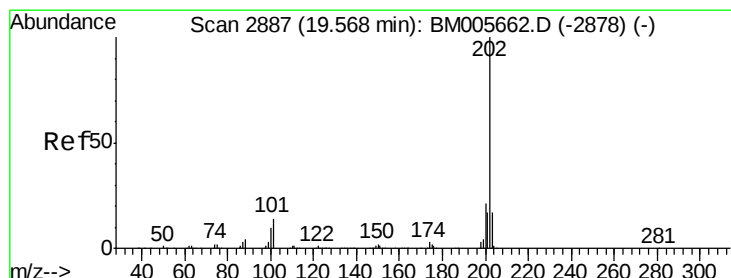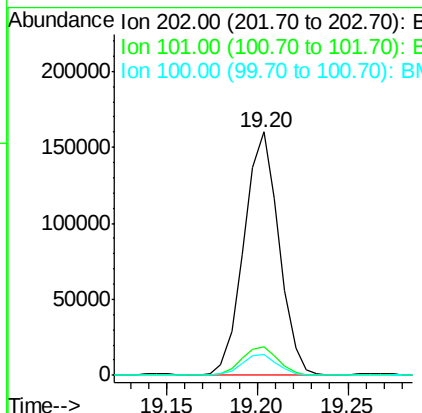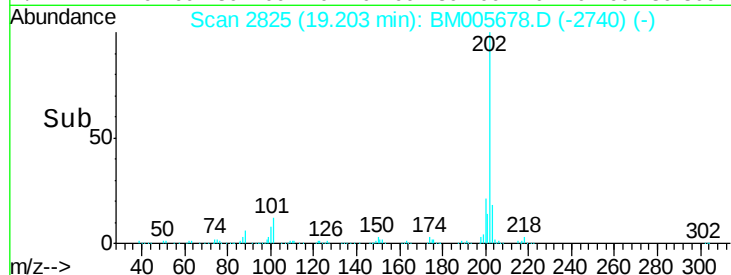

#31

Pyrene

Concen: 23.17 ng/ul




RT: 19.57 min Scan# 2887


Delta R.T. 0.00 min

Lab File: BM005678.D

Acq: 06 Jun 2016 20:14

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	632265		
101	13.8	9.8	14.8	
100	10.8	9.3	13.9	

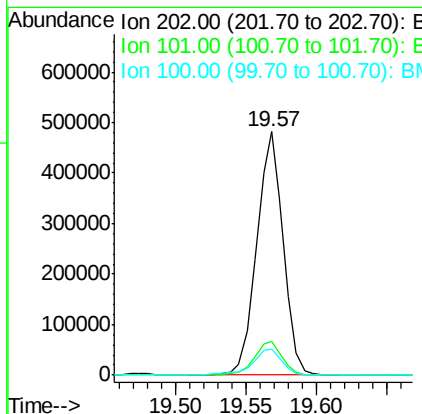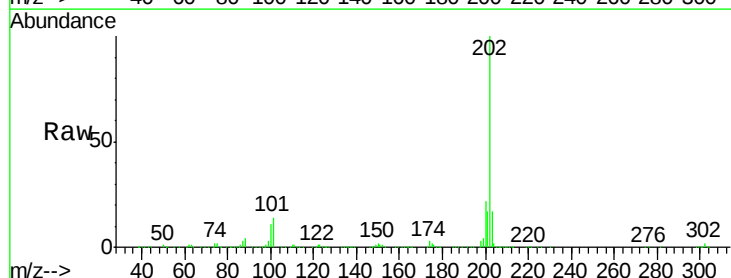



#32

Benzo(a)anthracene

Concen: 5.66 ng/ul

RT: 21.31 min Scan# 3183

Delta R.T. -0.01 min

Lab File: BM005678.D


Acq: 06 Jun 2016 20:14

Instrument :

BNA_M

ClientSampleId :




D9XS5MS

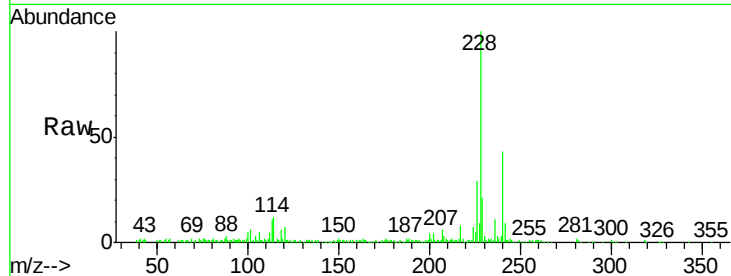

Tgt Ion:	228	Resp:	143620
Ion Ratio	Lower	Upper	
228	100		
229	21.2	16.6	25.0
226	29.4	21.0	31.4

Manual Integrations
APPROVED

sohil
6/7/2016 7:13:51 PM

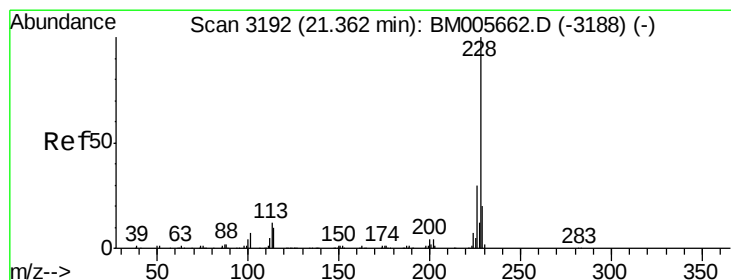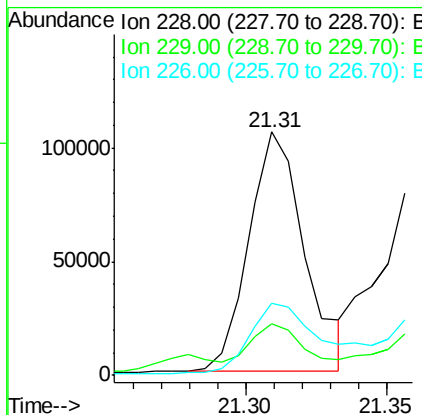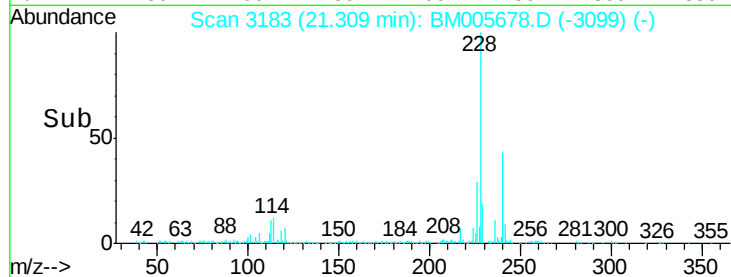

#33

Chrysene

Concen: 6.35 ng/ul




RT: 21.36 min Scan# 3192


Delta R.T. 0.00 min

Lab File: BM005678.D

Acq: 06 Jun 2016 20:14

Tgt Ion:	228	Resp:	152247
Ion Ratio	Lower	Upper	
228	100		
226	31.4	23.4	35.2
229	23.3	16.2	24.2

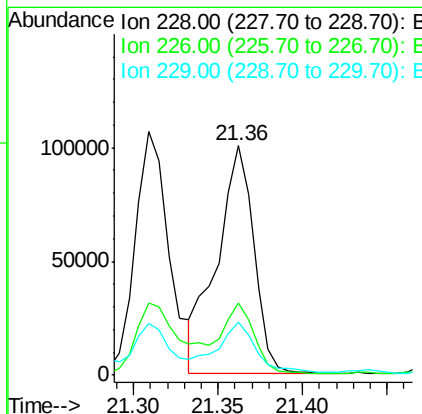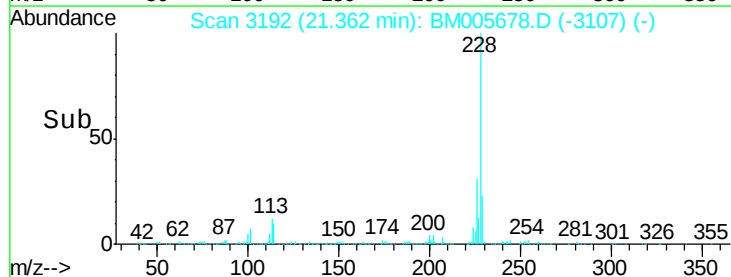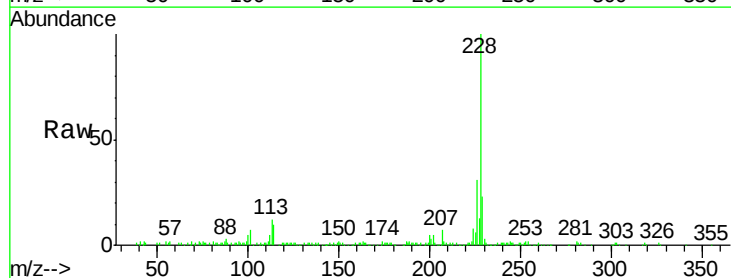







#35
Benzo(b)fluoranthene
Concen: 11.00 ng/ul
RT: 22.91 min Scan# 3455
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Instrument :
BNA_M
ClientSampleId :
D9XS5MS

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	304969		
253	22.5	18.1	27.1	
125	11.7	7.6	11.4	




Manual Integrations
APPROVED


sohil
6/7/2016 7:13:51 PM

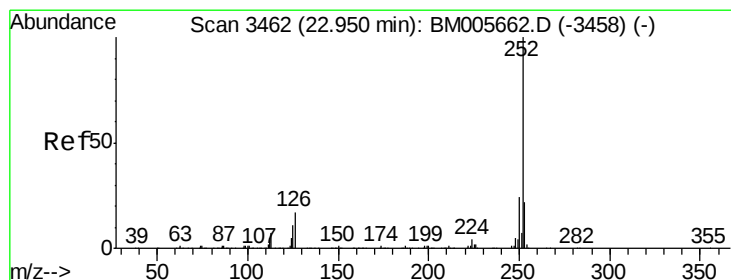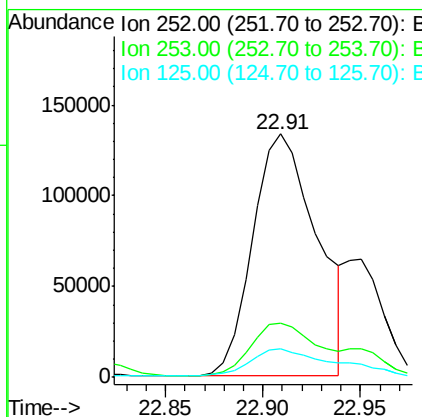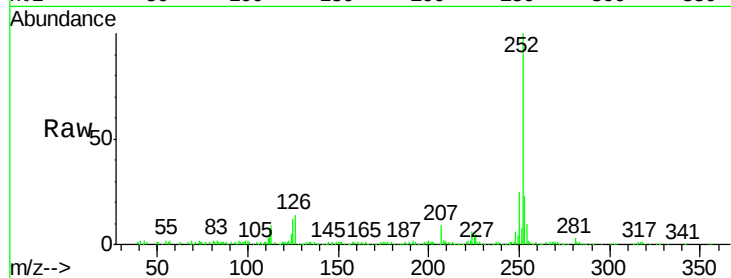

#36
Benzo(k)fluoranthene
Concen: 3.37 ng/ul m
RT: 22.95 min Scan# 3462
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	87505		
253	23.8	17.8	26.8	
125	11.4	7.7	11.5	

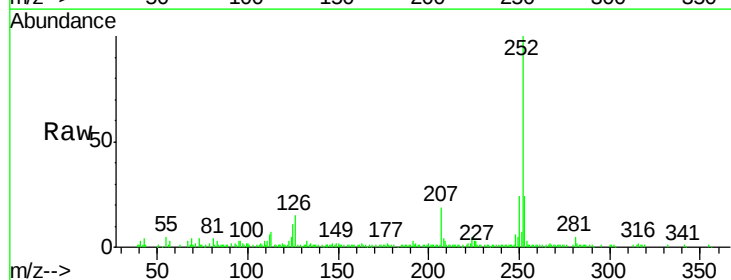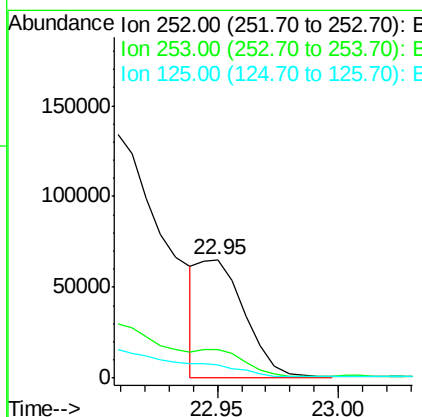

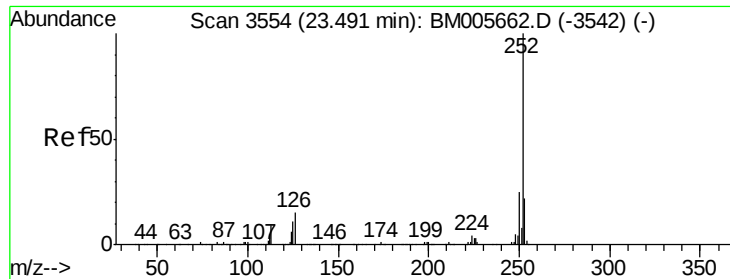

#38

Benzo(a)pyrene

Concen: 6.45 ng/ul

RT: 23.49 min Scan# 3554

Delta R.T. 0.00 min

Lab File: BM005678.D


Acq: 06 Jun 2016 20:14

Instrument :

BNA_M

ClientSampleId :




D9XS5MS

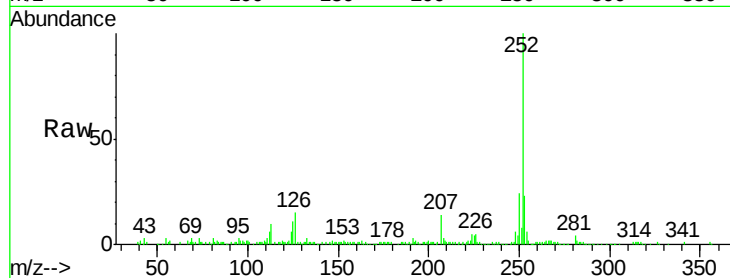

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.4	26.0
125	11.4	8.2	12.2

Manual Integrations
APPROVED

sohil
6/7/2016 7:13:51 PM

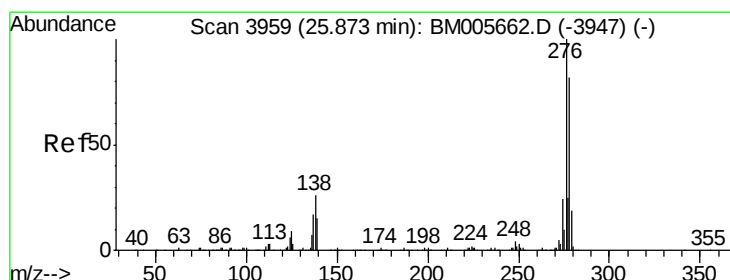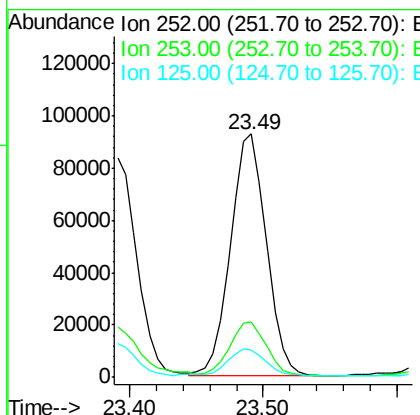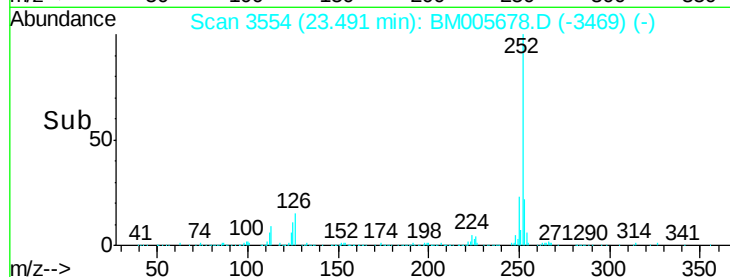

#39

Indeno(1,2,3-cd)pyrene

Concen: 4.68 ng/ul




RT: 25.87 min Scan# 3959


Delta R.T. 0.00 min

Lab File: BM005678.D

Acq: 06 Jun 2016 20:14

Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.5	15.8	23.6
277	25.4	19.0	28.6

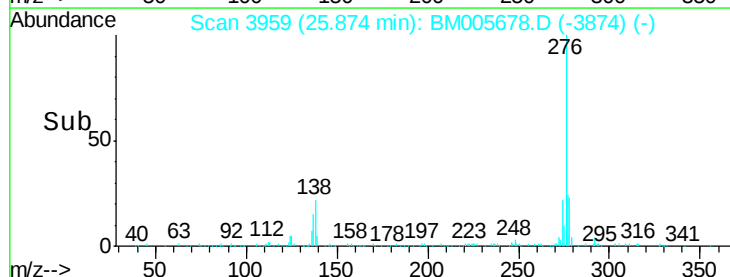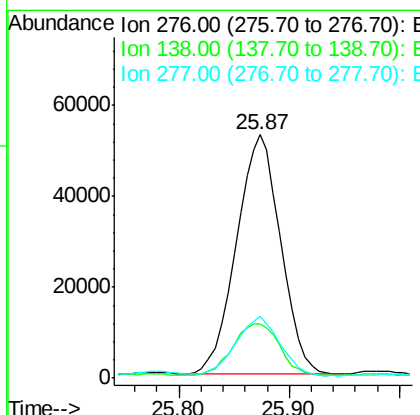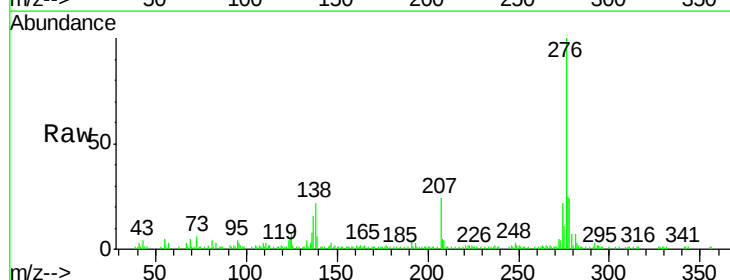




#40
Dibenzo(a,h)anthracene
Concen: 1.64 ng/ul
RT: 25.87 min Scan# 3959
Delta R.T. -0.01 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Instrument :
BNA_M
ClientSampleId :
D9XS5MS




Tgt Ion	Ratio	Lower	Upper
278	100		
139	24.7	12.1	18.1#
279	29.0	19.8	29.8

Manual Integrations
APPROVED

sohil
6/7/2016 7:13:51 PM

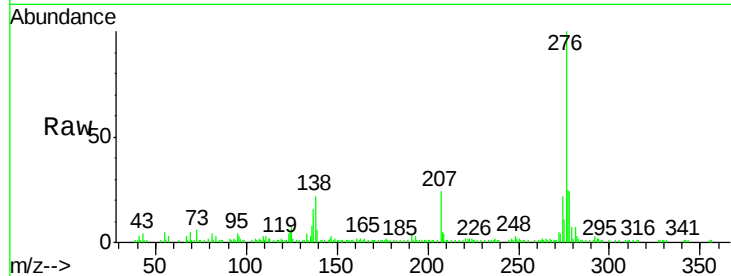

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

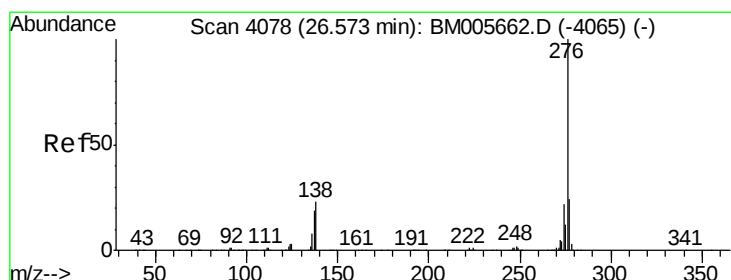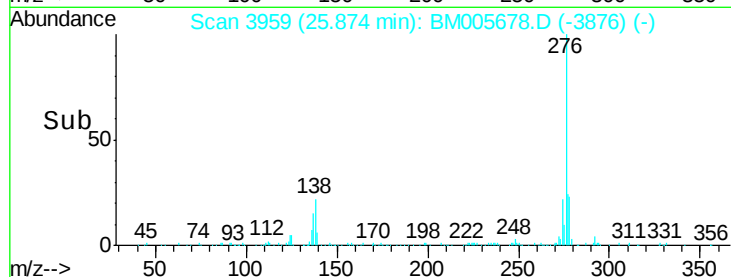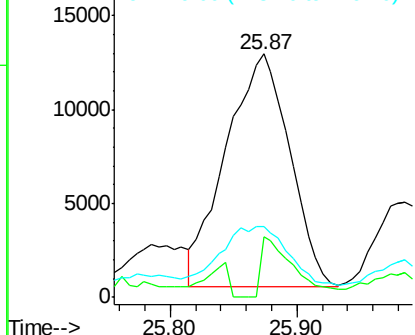

#41
Benzo(g,h,i)perylene
Concen: 5.44 ng/ul
RT: 26.57 min Scan# 4078
Delta R.T. 0.00 min
Lab File: BM005678.D
Acq: 06 Jun 2016 20:14

Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.1	13.9	20.9#
277	25.6	19.8	29.6

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

