


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060618\
 Data File : BM015484.D
 Acq On : 06 Jun 2018 11:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 06 14:01:06 2018

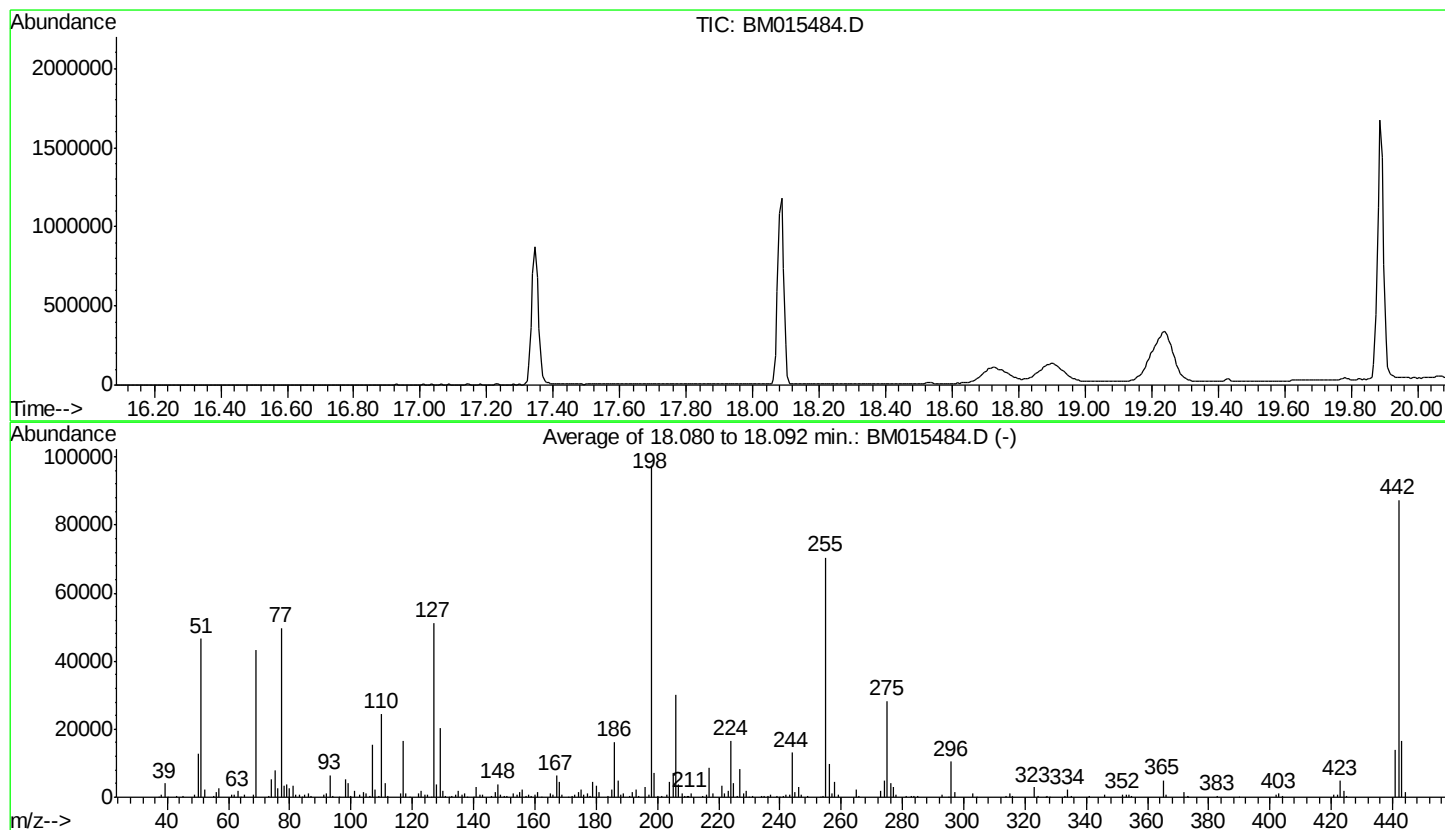

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	46557	PASS
68	69	0.00	2	1.9	820	PASS
69	198	0.00	100	44.5	43384	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	51317	PASS
197	198	0.00	2	0.6	631	PASS
198	198	100	100	100.0	97445	PASS
199	198	5	9	7.3	7135	PASS
275	198	10	60	29.0	28245	PASS
365	198	1	100	5.2	5058	PASS
441	443	0.01	100	83.3	13787	PASS
442	198	50	100	89.7	87373	PASS
443	442	15	24	19.0	16559	PASS