


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060618\  
 Data File : BM015504.D  
 Acq On : 07 Jun 2018 00:53  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM052518.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jun 06 14:01:06 2018

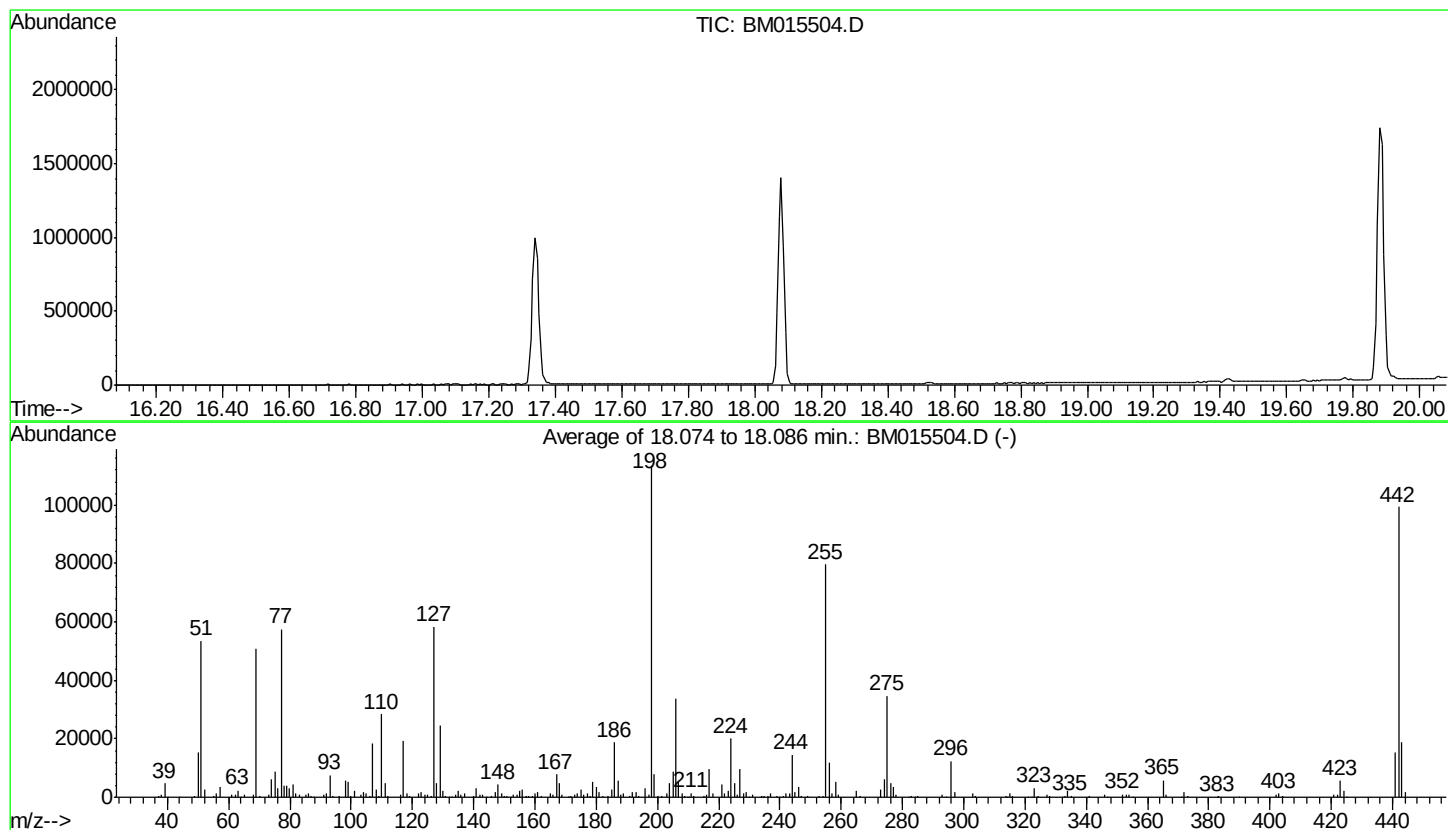

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 47.2      | 53546   | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 1020    | PASS             |
| 69          | 198          | 0.00         | 100          | 44.9      | 50933   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 277     | PASS             |
| 127         | 198          | 10           | 80           | 51.4      | 58352   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 715     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 113490  | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 8012    | PASS             |
| 275         | 198          | 10           | 60           | 30.6      | 34725   | PASS             |
| 365         | 198          | 1            | 100          | 5.1       | 5738    | PASS             |
| 441         | 443          | 0.01         | 100          | 81.0      | 15374   | PASS             |
| 442         | 198          | 50           | 100          | 87.6      | 99405   | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 18980   | PASS             |