

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060716\
 Data File : BM005700.D
 Acq On : 07 Jun 2016 19:49
 Operator : UM/SJ
 Sample : H3411-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XR7

Manual Integrations
 APPROVED

sohil
 6/8/2016 7:16:50 PM

Quant Time: Jun 08 01:51:19 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM060216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 08 01:24:32 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	117591	20.00	ng/ul	0.00
7) Naphthalene-d8	10.55	136	567952	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.40	164	322948	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.14	188	708161	20.00	ng/ul	0.00
29) Chrysene-d12	21.33	240	634699	20.00	ng/ul	0.00
34) Perylene-d12	23.59	264	514623	20.00	ng/ul	-0.01

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.20	96	3772	1.35	ng/uL	0.00
3) Phenol-d5	6.93	99	146015	14.12	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.09	67	112504	17.88	ng/ul	0.00
5) 2-Chlorophenol-d4	7.29	132	134518	15.77	ng/ul	0.00
6) 4-Methylphenol-d8	8.47	113	88081	10.77	ng/ul	0.00
8) Nitrobenzene-d5	8.92	128	76263	17.49	ng/ul	0.00
9) 2-Nitrophenol-d4	9.63	143	84883	18.19	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.17	165	133105	16.05	ng/ul	0.00
12) 4-Chloroaniline-d4	10.69	131	144184	14.63	ng/ul	0.00
16) Dimethylphthalate-d6	13.80	166	455535	18.35	ng/ul	0.00
17) Acenaphthylene-d8	14.09	160	590888	18.30	ng/ul	0.00
20) 4-Nitrophenol-d4	14.63	143	31199	8.78	ng/ul	0.00
21) Fluorene-d10	15.39	176	409387	19.20	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.53	200	35808	10.74	ng/ul	0.00
26) Anthracene-d10	17.24	188	626381	18.63	ng/ul	0.00
30) Pyrene-d10	19.54	212	661403	20.73	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.44	264	435399	18.38	ng/ul	0.00

Target Compounds

						Ovalue
18) Acenaphthylene	14.12	152	35062	1.05	ng/ul	98
25) Phenanthrene	17.19	178	190731	4.88	ng/ul	98
27) Anthracene	17.27	178	41091	1.03	ng/ul	99
28) Fluoranthene	19.20	202	430437	10.77	ng/ul	99
31) Pyrene	19.57	202	385648	9.63	ng/ul	97
32) Benzo(a)anthracene	21.31	228	215730	5.80	ng/ul	97
33) Chrysene	21.36	228	224654	6.39	ng/ul	97
35) Benzo(b)fluoranthene	22.91	252	323177	10.41	ng/ul#	98
36) Benzo(k)fluoranthene	22.95	252	94583m	3.25	ng/ul	
38) Benzo(a)pyrene	23.49	252	183408	6.14	ng/ul#	95
39) Indeno(1,2,3-cd)pyrene	25.87	276	134940	3.82	ng/ul	95
40) Dibenzo(a,h)anthracene	25.87	278	37707	1.27	ng/ul#	79
41) Benzo(g,h,i)perylene	26.58	276	134329	4.53	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM060716\
Data File : BM005700.D
Acq On : 07 Jun 2016 19:49
Operator : UM/SJ
Sample : H3411-19
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9XR7

Manual Integrations
APPROVED

sohil
6/8/2016 7:16:50 PM

Quant Time: Jun 08 01:51:19 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM060216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 08 01:24:32 2016
Response via : Initial Calibration

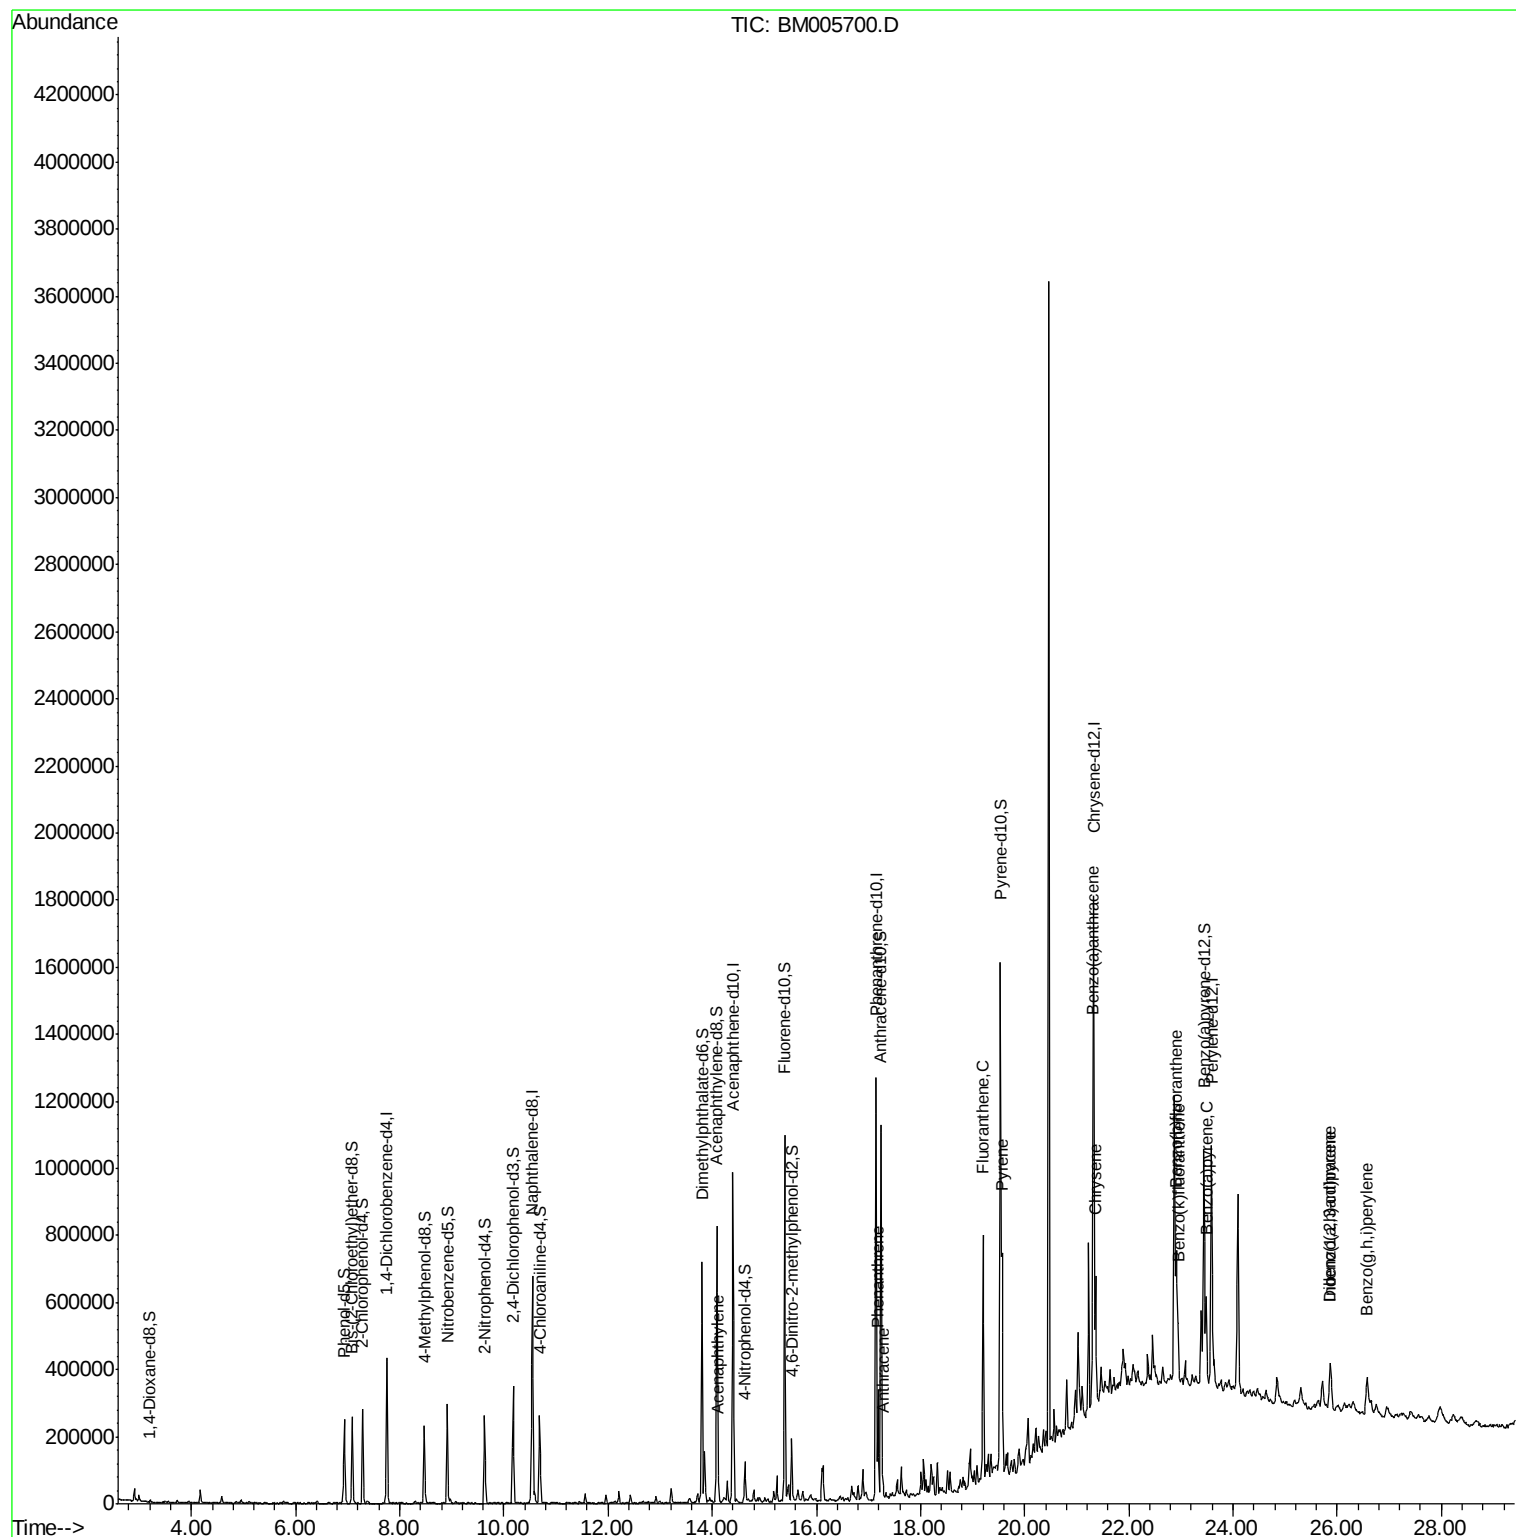

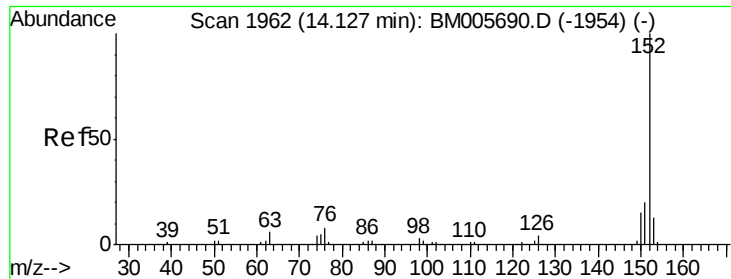

#18

Acenaphthylene

Concen: 1.05 ng/ul

RT: 14.12 min Scan# 1961

Delta R.T. -0.01 min

Lab File: BM005700.D

Acq: 07 Jun 2016 19:49

Instrument :

BNA_M


ClientSampleId :

D9XR7




Tot Ion:	152	Resp:	35062
Ion Ratio	Lower	Upper	
152	100		
151	20.1	17.3	25.9
153	14.3	11.1	16.7

Manual Integrations
APPROVED

sohil
6/8/2016 7:16:50 PM

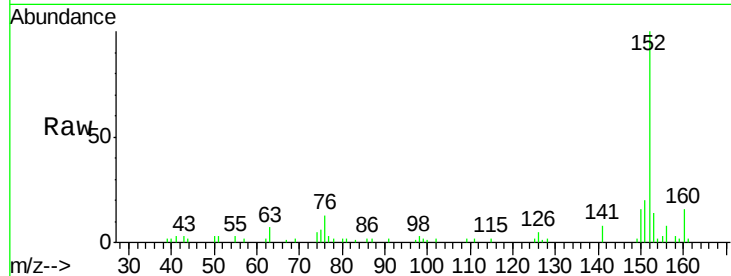

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

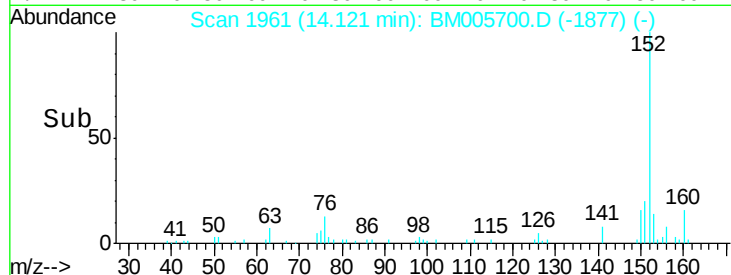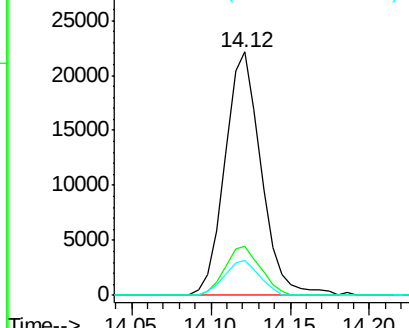

#25

Phenanthrene

Concen: 4.88 ng/ul


RT: 17.19 min Scan# 2482

Delta R.T. -0.01 min



Lab File: BM005700.D


Acq: 07 Jun 2016 19:49

Tgt Ion:	178	Resp:	190731
Ion Ratio	Lower	Upper	
178	100		
179	15.3	11.8	17.8
176	19.9	14.8	22.2



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

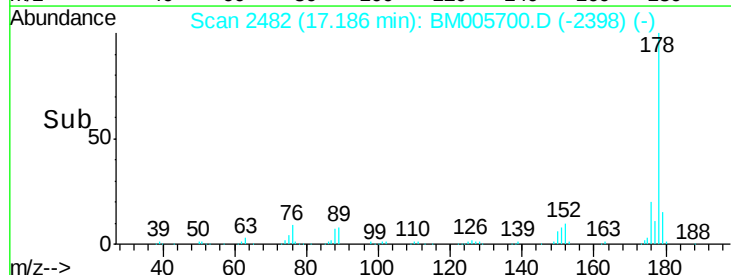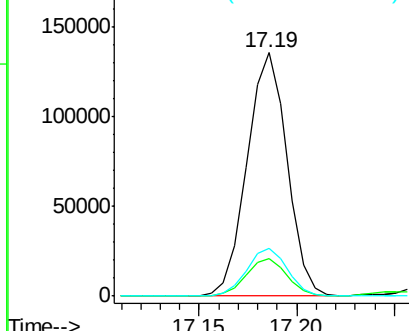

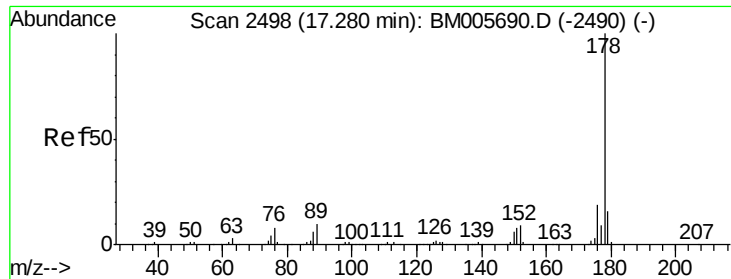





#27
 Anthracene
 Concen: 1.03 ng/ul
 RT: 17.27 min Scan# 2497
 Delta R.T. -0.01 min
 Lab File: BM005700.D
 Acq: 07 Jun 2016 19:49

Instrument :
 BNA_M
 ClientSampled :
 D9XR7

Tot Ion	Ratio	Lower	Upper
178	100		
179	16.3	12.9	19.3
176	20.0	15.6	23.4




Manual Integrations
 APPROVED


sohil
 6/8/2016 7:16:50 PM

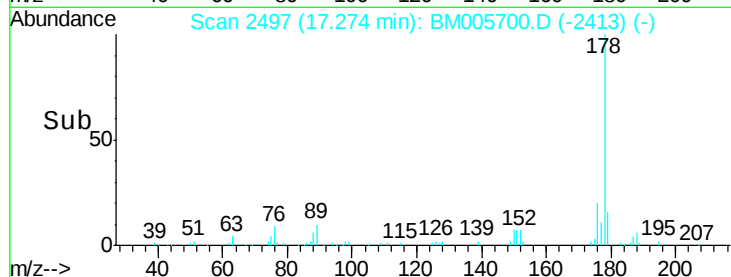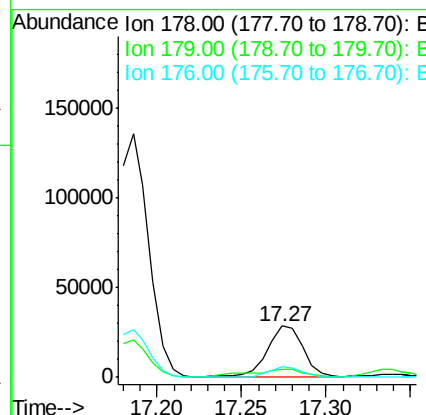

#28
 Fluoranthene
 Concen: 10.77 ng/ul
 RT: 19.20 min Scan# 2825
 Delta R.T. -0.00 min
 Lab File: BM005700.D
 Acq: 07 Jun 2016 19:49

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.6	8.9	13.3
100	8.5	7.0	10.4

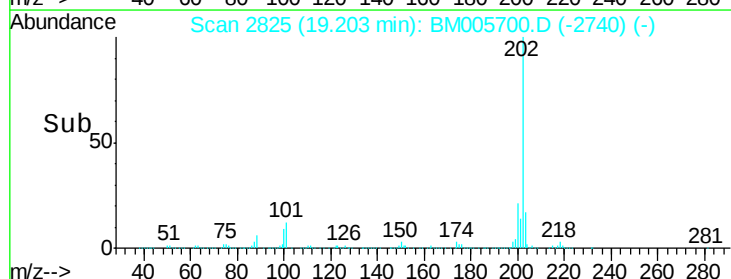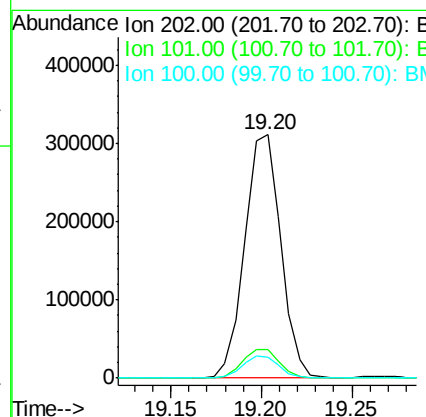

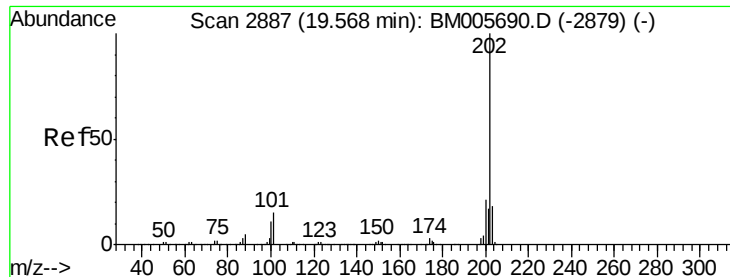





#31
Pvrene
Concen: 9.63 ng/ul
RT: 19.57 min Scan# 2887
Delta R.T. -0.00 min
Lab File: BM005700.D
Acq: 07 Jun 2016 19:49

Instrument :
BNA_M
ClientSampleId :
D9XR7

Tot Ion	Ratio	Resp	Lower	Upper
202	100	385648		
101	13.5	9.8	14.8	
100	10.9	9.3	13.9	




Manual Integrations
APPROVED


sohil
6/8/2016 7:16:50 PM

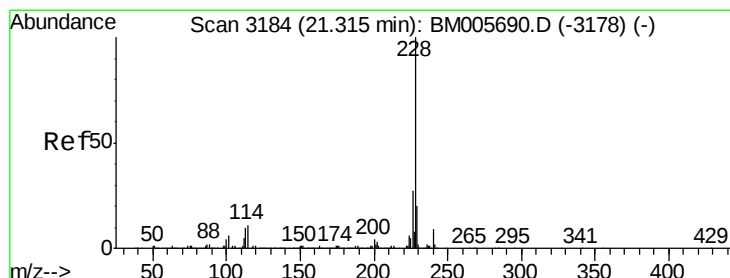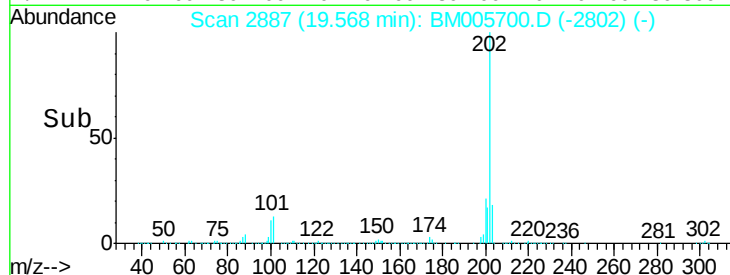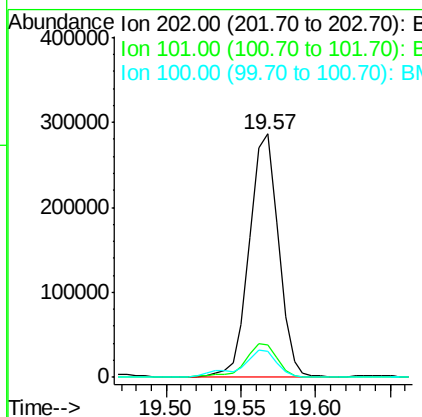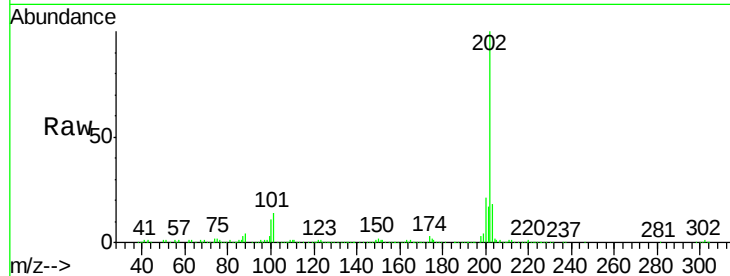

#32
Benzo(a)anthracene
Concen: 5.80 ng/ul
RT: 21.31 min Scan# 3183
Delta R.T. -0.01 min
Lab File: BM005700.D
Acq: 07 Jun 2016 19:49

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	215730		
229	21.5	16.6	25.0	
226	28.1	21.0	31.4	

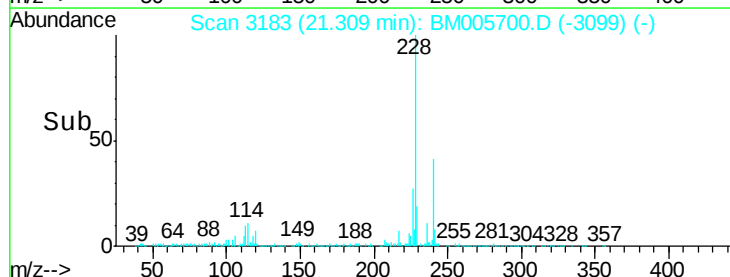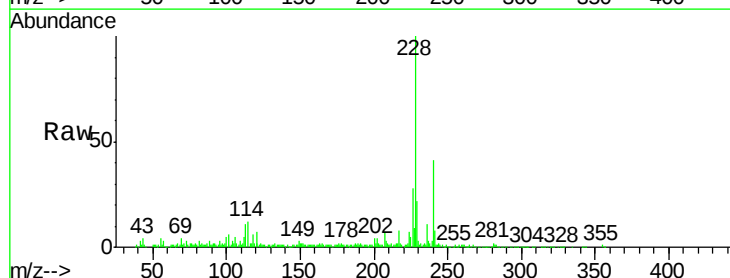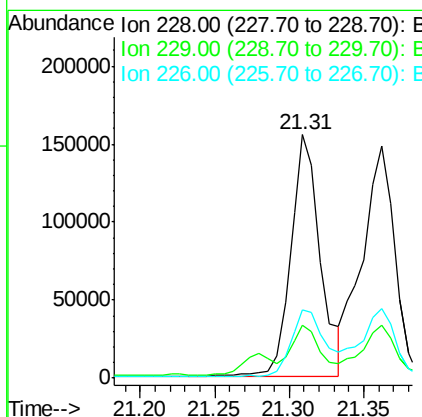

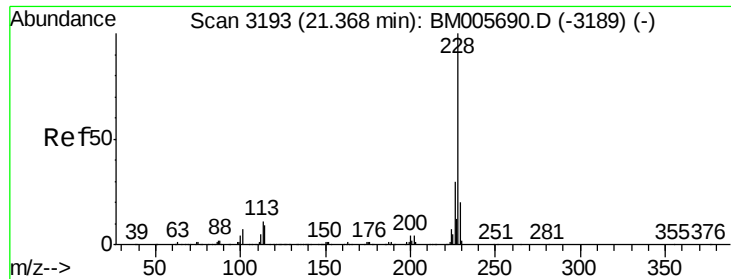





#33
Chrysene
Concen: 6.39 ng/ul
RT: 21.36 min Scan# 3192
Delta R.T. -0.01 min
Lab File: BM005700.D
Acq: 07 Jun 2016 19:49

Instrument :
BNA_M
ClientSampleId :
D9XR7

Tot Ion	Ratio	Resp	Lower	Upper
228	100	224654		
226	30.2		23.4	35.2
229	23.0		16.2	24.2




Manual Integrations
APPROVED


sohil
6/8/2016 7:16:50 PM

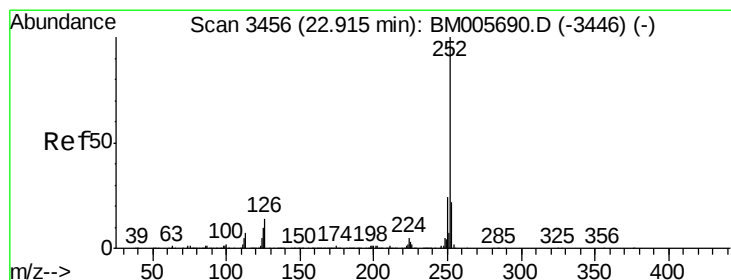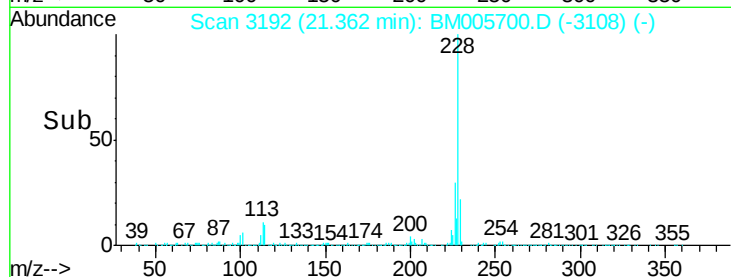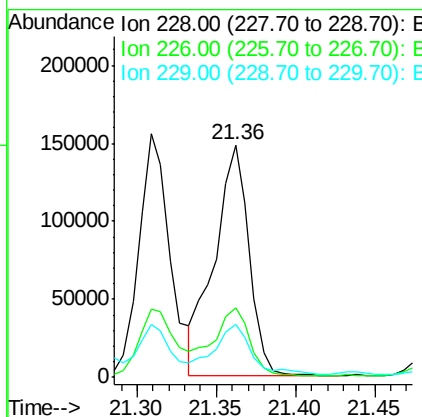

#35
Benzo(b)fluoranthene
Concen: 10.41 ng/ul
RT: 22.91 min Scan# 3455
Delta R.T. -0.01 min
Lab File: BM005700.D
Acq: 07 Jun 2016 19:49

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	323177		
253	22.8		18.1	27.1
125	12.1		7.6	11.4#

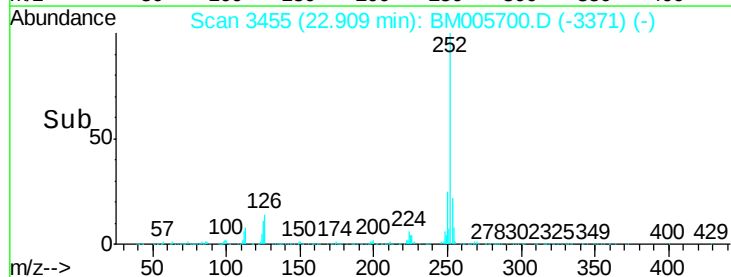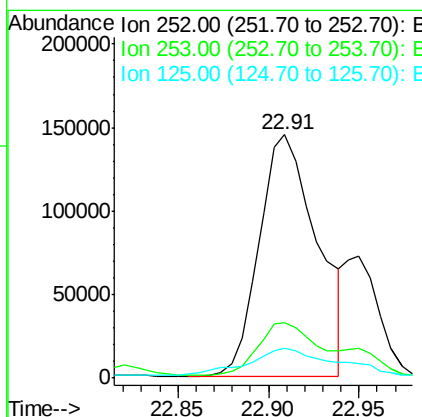

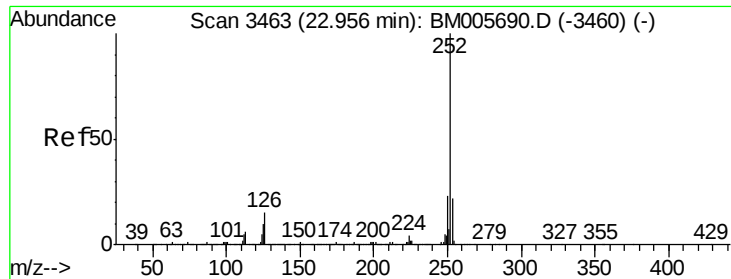

#36

Benzo(k)fluoranthene

Concen: 3.25 ng/ul m

RT: 22.95 min Scan# 3462

Delta R.T. -0.01 min

Lab File: BM005700.D

Acq: 07 Jun 2016 19:49

Instrument :

BNA_M





ClientSampleId :

D9XR7

Tot Ion:	252	Resp:	94583
Ion Ratio	Lower	Upper	
252	100		
253	24.3	17.8	26.8
125	12.1	7.7	11.5#

Manual Integrations
APPROVED

sohil
6/8/2016 7:16:50 PM

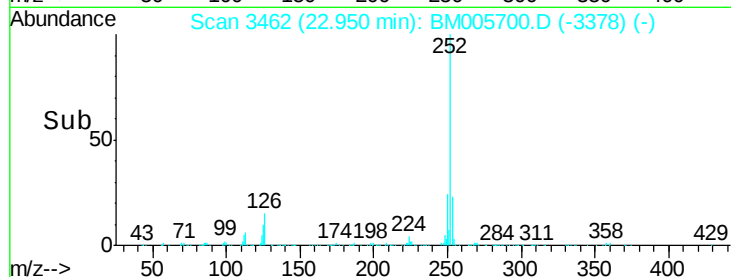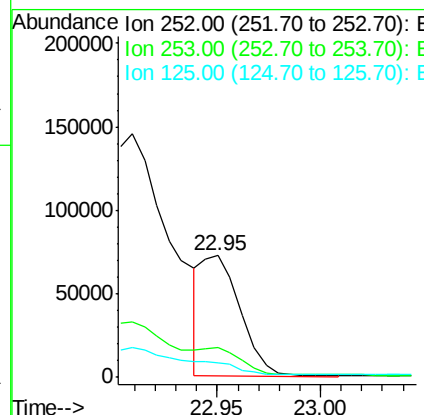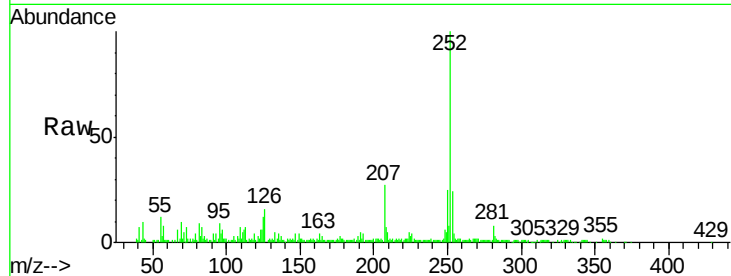

#38

Benzo(a)pyrene

Concen: 6.14 ng/ul




RT: 23.49 min Scan# 3554


Delta R.T. -0.01 min

Lab File: BM005700.D

Acq: 07 Jun 2016 19:49

Tgt Ion:	252	Resp:	183408
Ion Ratio	Lower	Upper	
252	100		
253	23.7	17.4	26.0
125	12.3	8.2	12.2#

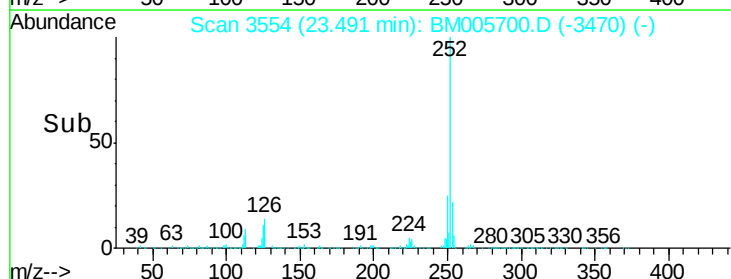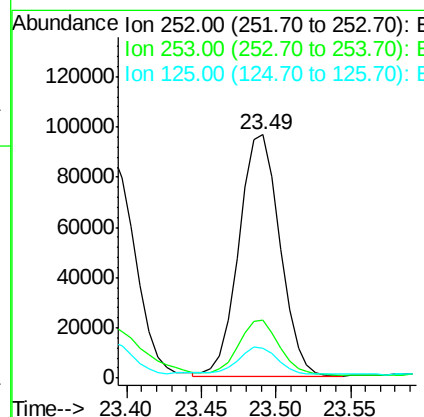

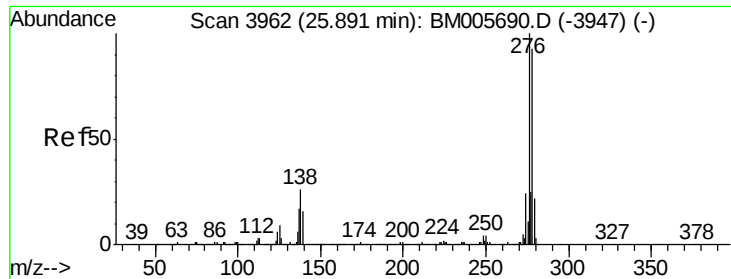





#39
Indeno(1,2,3-cd)pyrene
Concen: 3.82 ng/ul
RT: 25.87 min Scan# 3959
Delta R.T. -0.02 min
Lab File: BM005700.D
Acq: 07 Jun 2016 19:49

Instrument :
BNA_M
ClientSampleId :
D9XR7

Tot Ion	Ratio	Lower	Upper
276	100		
138	23.0	15.8	23.6
277	25.3	19.0	28.6




Manual Integrations
APPROVED




sohil
6/8/2016 7:16:50 PM

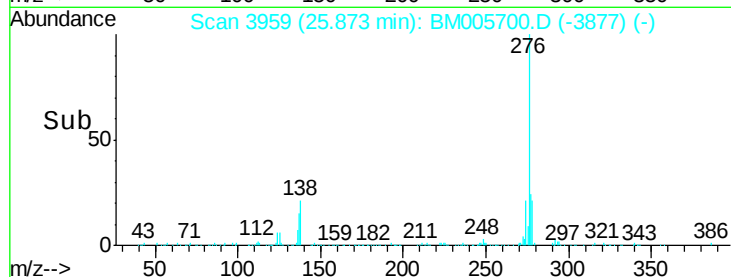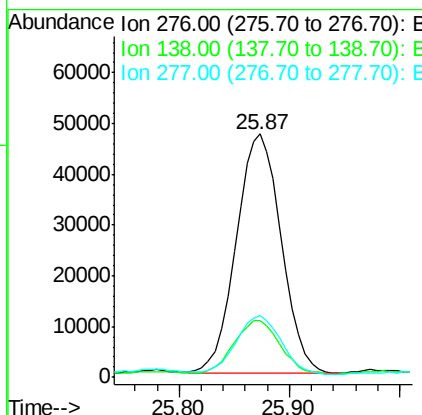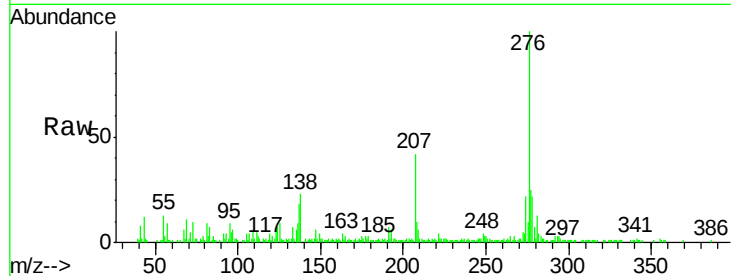

#40
Dibenzo(a,h)anthracene
Concen: 1.27 ng/ul
RT: 25.87 min Scan# 3958
Delta R.T. -0.02 min
Lab File: BM005700.D
Acq: 07 Jun 2016 19:49

Tgt Ion	Ratio	Lower	Upper
278	100		
139	27.4	12.1	18.1#
279	32.3	19.8	29.8#

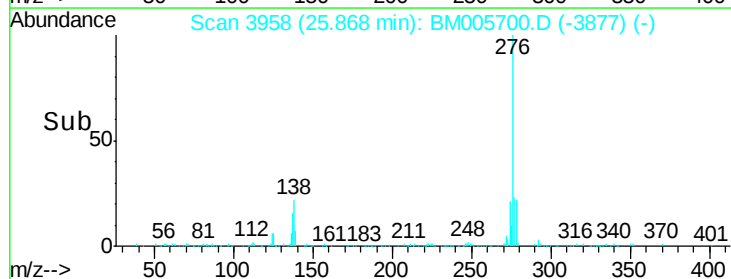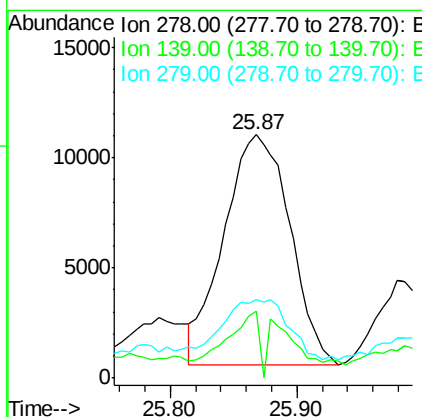

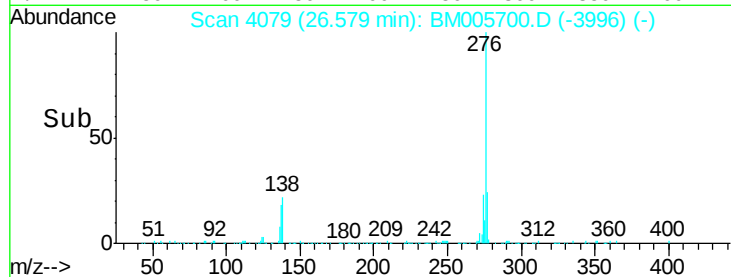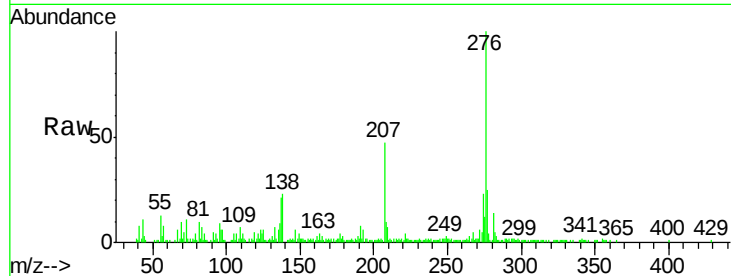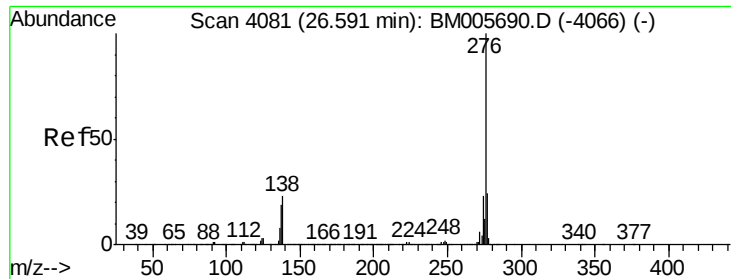

#41

Benzo(a,h,i)perylene

Concen: 4.53 ng/ul

RT: 26.58 min Scan# 4079

Delta R.T. -0.01 min

Lab File: BM005700.D

Acq: 07 Jun 2016 19:49

Instrument :

BNA_M

ClientSampleId :

D9XR7

Tot Ion	Ratio	Lower	Upper
276	100		
138	23.4	13.9	20.9#
277	24.8	19.8	29.6

Manual Integrations
APPROVED

sohil
6/8/2016 7:16:50 PM

