

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060717\
 Data File : BM010434.D
 Acq On : 07 Jun 2017 15:19
 Operator : SJ/MA
 Sample : I3446-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC50

Quant Time: Jun 08 01:24:22 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 08 01:22:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	224538	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	776763	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.55	164	494484	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	1144210	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	1642768	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1799624	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.38	96	18326	3.35	ng/uL	0.00
5) Phenol-d5	7.09	99	285578	16.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	174162	18.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	268193	19.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	242265	17.65	ng/ul	-0.01
19) Nitrobenzene-d5	9.09	128	123149	21.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.81	143	141538	21.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.34	165	286009	21.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.88	131	297136	22.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	904034	22.00	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	996205	20.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.79	143	51170	8.32	ng/ul	0.00
57) Fluorene-d10	15.53	176	756673	20.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	93592	11.55	ng/ul	0.00
70) Anthracene-d10	17.39	188	1222352	21.95	ng/ul	0.00
76) Pyrene-d10	19.68	212	1501481	22.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.65	264	1797416	21.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.00	163	288773	7.147	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060717\
Data File : BM010434.D
Acq On : 07 Jun 2017 15:19
Operator : SJ/MA
Sample : I3446-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC50

Quant Time: Jun 08 01:24:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 08 01:22:27 2017
Response via : Initial Calibration

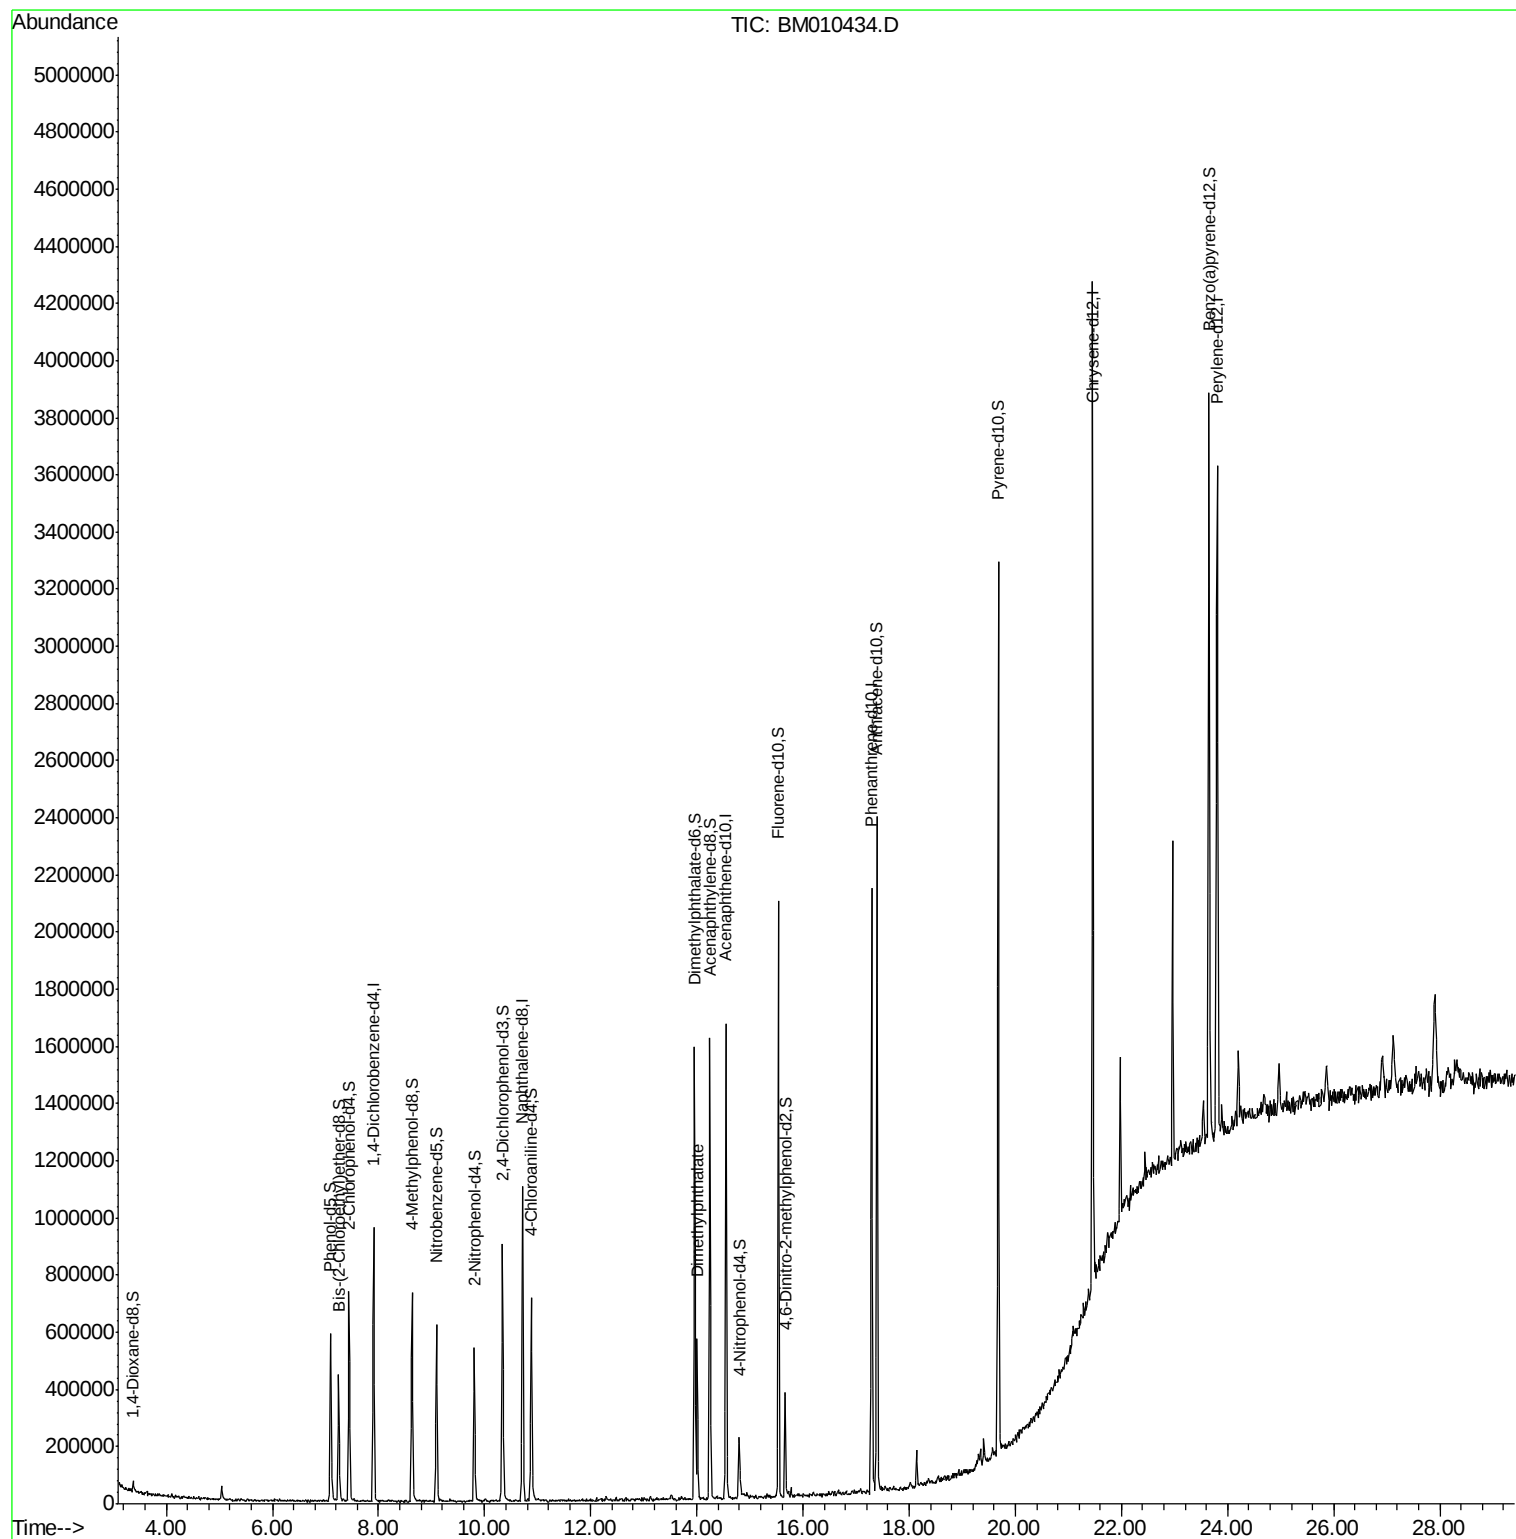

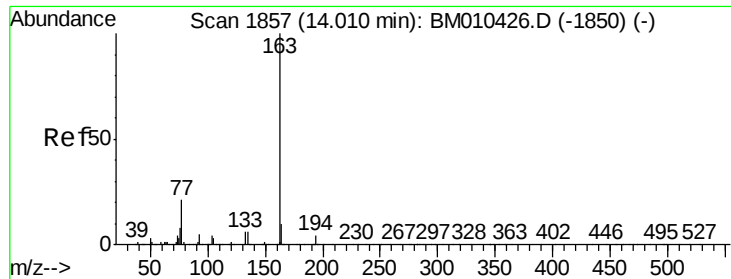

#44

Dimethylphthalate

Concen: 7.147 ng/ul

RT: 14.00 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM010434.D

Acq: 07 Jun 2017 15:19

Instrument :

BNA_M

ClientSampleId :

BDC50


Tgt Ion:163 Resp: 288773

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 11.9 8.2 12.4

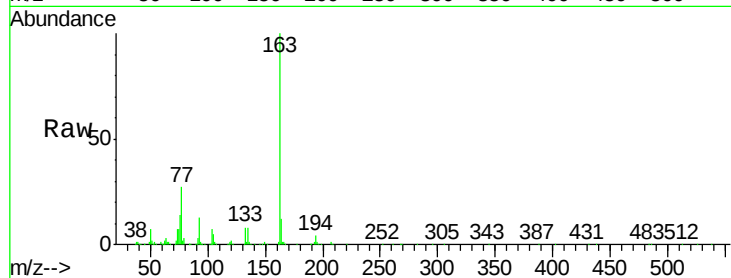

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

