

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060717\
 Data File : BM010435.D
 Acq On : 07 Jun 2017 15:55
 Operator : SJ/MA
 Sample : I3446-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	46	49	54	rBV	45615	62749	1.04%	0.107%
2	7.093	675	681	693	rBV	793847	1353206	22.33%	2.312%
3	7.251	702	708	716	rBV	554791	876207	14.46%	1.497%
4	7.445	734	741	754	rVB	910500	1524775	25.16%	2.605%
5	7.910	813	820	828	rBV	983777	1551176	25.59%	2.650%
6	8.634	935	943	960	rBV	1015231	1676050	27.65%	2.863%
7	9.098	1015	1022	1031	rBV	751531	1282098	21.15%	2.190%
8	9.804	1134	1142	1149	rBV	721557	1192477	19.67%	2.037%
9	10.339	1227	1233	1245	rBV	1189066	1964538	32.41%	3.356%
10	10.716	1289	1297	1305	rBV	1126351	1925442	31.77%	3.289%
11	10.881	1318	1325	1337	rBV	806964	1468255	24.22%	2.508%
12	13.957	1841	1848	1853	rBV	2112840	2884026	47.58%	4.927%
13	14.004	1853	1856	1862	rVB	701288	931109	15.36%	1.591%
14	14.245	1890	1897	1905	rBV	2117454	3055862	50.42%	5.221%
15	14.545	1941	1948	1955	rBV2	1662305	2496016	41.18%	4.264%
16	14.792	1982	1990	2004	rBV	413853	847479	13.98%	1.448%
17	15.533	2108	2116	2124	rBV	2671964	3904878	64.43%	6.671%
18	15.663	2132	2138	2145	rBV	638772	905410	14.94%	1.547%
19	17.292	2408	2415	2420	rBV	2091289	3073465	50.71%	5.251%
20	17.333	2420	2422	2426	rVV	73100	87579	1.44%	0.150%
21	17.392	2426	2432	2440	rVV	3136935	4252305	70.16%	7.264%
22	18.133	2553	2558	2567	rBV3	170023	279815	4.62%	0.478%
23	19.309	2753	2758	2760	rBV5	49264	80052	1.32%	0.137%
24	19.345	2760	2764	2770	rVB	201668	282688	4.66%	0.483%
25	19.409	2771	2775	2780	rBV7	92517	134775	2.22%	0.230%
26	19.574	2798	2803	2806	rBV5	47850	89130	1.47%	0.152%
27	19.680	2815	2821	2830	rBV	3832165	5515746	91.00%	9.423%
28	21.456	3118	3123	3128	rBV	3611338	4375383	72.19%	7.475%
29	23.650	3490	3496	3503	rBV2	3446244	6061094	100.00%	10.355%
30	23.803	3516	3522	3530	rVB2	2267290	4401753	72.62%	7.520%


Sum of corrected areas: 58535538

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060717\
Data File : BM010435.D
Acq On : 07 Jun 2017 15:55
Operator : SJ/MA
Sample : I3446-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC51

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

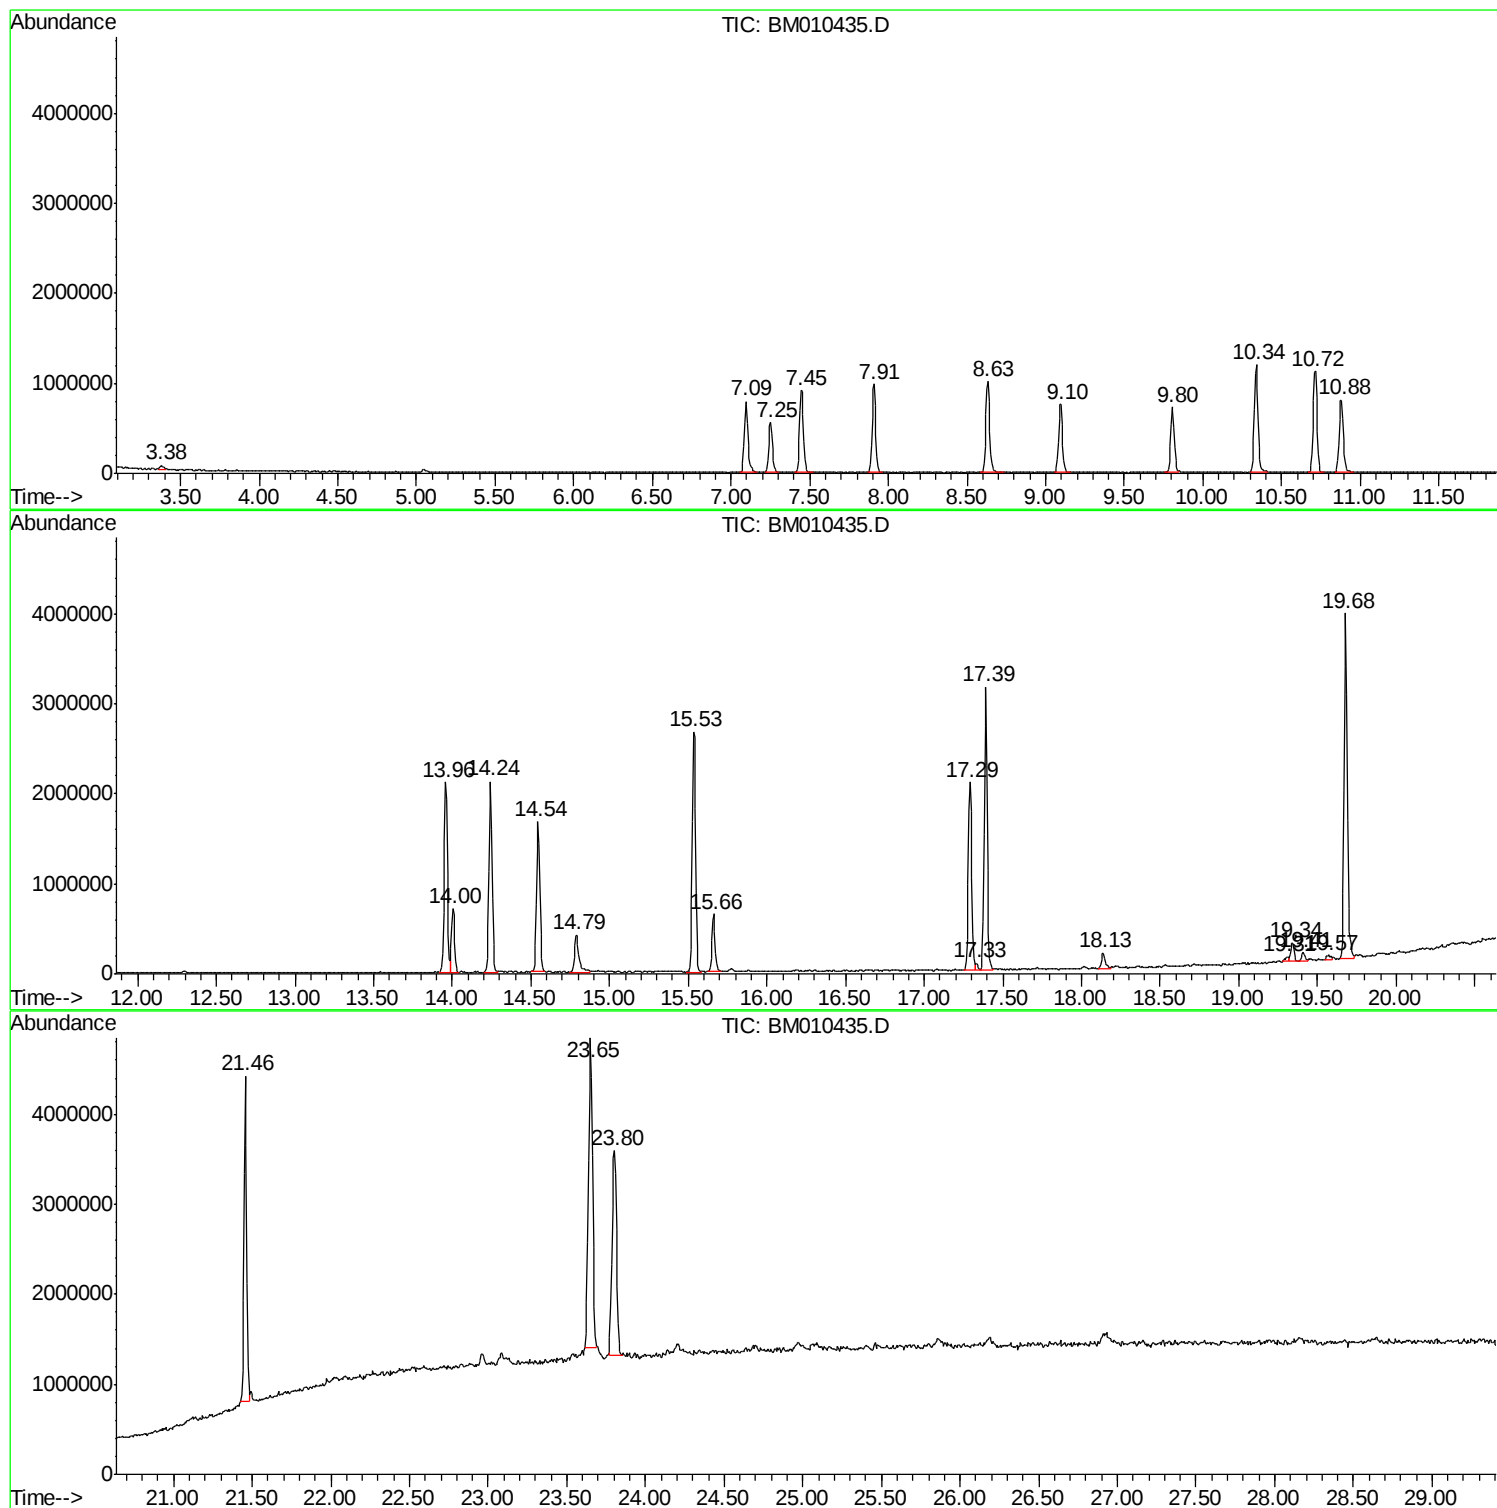

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060717\
Data File : BM010435.D
Acq On : 07 Jun 2017 15:55
Operator : SJ/MA
Sample : I3446-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC51

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060717\
Data File : BM010435.D
Acq On : 07 Jun 2017 15:55
Operator : SJ/MA
Sample : I3446-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC51

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc