

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
 Data File : BM030306.D
 Acq On : 07 Jun 2021 10:34
 Operator : CG/JU
 Sample : PB136695BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK695

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030306.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	35	39	49	rVB	63939	93572	1.48%	0.167%
2	3.728	106	109	130	rBV	568529	1079424	17.10%	1.921%
3	4.057	162	165	169	rVB2	10576	13888	0.22%	0.025%
4	4.275	198	202	210	rVB9	4091	7351	0.12%	0.013%
5	7.004	660	666	678	rBV	843731	1335406	21.16%	2.377%
6	7.181	689	696	709	rBV	690698	1106606	17.53%	1.970%
7	7.381	723	730	742	rVB	881406	1398324	22.15%	2.489%
8	7.851	800	810	820	rVB	698103	1122063	17.78%	1.997%
9	8.545	921	928	940	rBV	1038109	1646742	26.09%	2.931%
10	9.004	998	1006	1014	rBV	806038	1299376	20.59%	2.313%
11	9.728	1121	1129	1139	rBV	573381	968179	15.34%	1.723%
12	10.257	1210	1219	1230	rBV	1033355	1680419	26.62%	2.991%
13	10.639	1276	1284	1293	rBV	962307	1651326	26.16%	2.939%
14	10.775	1299	1307	1324	rBV	1005343	1760384	27.89%	3.134%
15	12.228	1548	1554	1560	rBV2	16391	27383	0.43%	0.049%
16	13.880	1828	1835	1845	rBV	1975702	2700662	42.79%	4.807%
17	14.169	1877	1884	1893	rBV	2174934	3164450	50.14%	5.633%
18	14.474	1929	1936	1946	rBV	1583434	2325936	36.85%	4.140%
19	14.651	1960	1966	1986	rBV	847675	1265654	20.05%	2.253%
20	15.463	2098	2104	2112	rBV	2946850	4174320	66.14%	7.431%
21	15.574	2117	2123	2131	rBV	787763	1082862	17.16%	1.928%
22	15.704	2140	2145	2150	rVB2	32211	47753	0.76%	0.085%
23	16.245	2232	2237	2242	rVB2	10400	15435	0.24%	0.027%
24	16.998	2361	2365	2369	rBV2	6793	9725	0.15%	0.017%
25	17.210	2394	2401	2410	rBV	1986846	2780779	44.06%	4.950%
26	17.310	2411	2418	2436	rVV	3218314	4580130	72.57%	8.153%
27	19.227	2740	2744	2748	rVV	32661	46457	0.74%	0.083%
28	19.480	2783	2787	2792	rBV	28144	36626	0.58%	0.065%
29	19.592	2800	2806	2815	rBV	4121883	5584372	88.48%	9.940%
30	21.368	3103	3108	3115	rBV	2568501	3269618	51.80%	5.820%
31	23.509	3465	3472	3483	rBV2	3375020	6311748	100.00%	11.235%
32	23.656	3490	3497	3509	rVB2	1865351	3591207	56.90%	6.393%




Sum of corrected areas: 56178177

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
Data File : BM030306.D
Acq On : 07 Jun 2021 10:34
Operator : CG/JU
Sample : PB136695BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK695

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

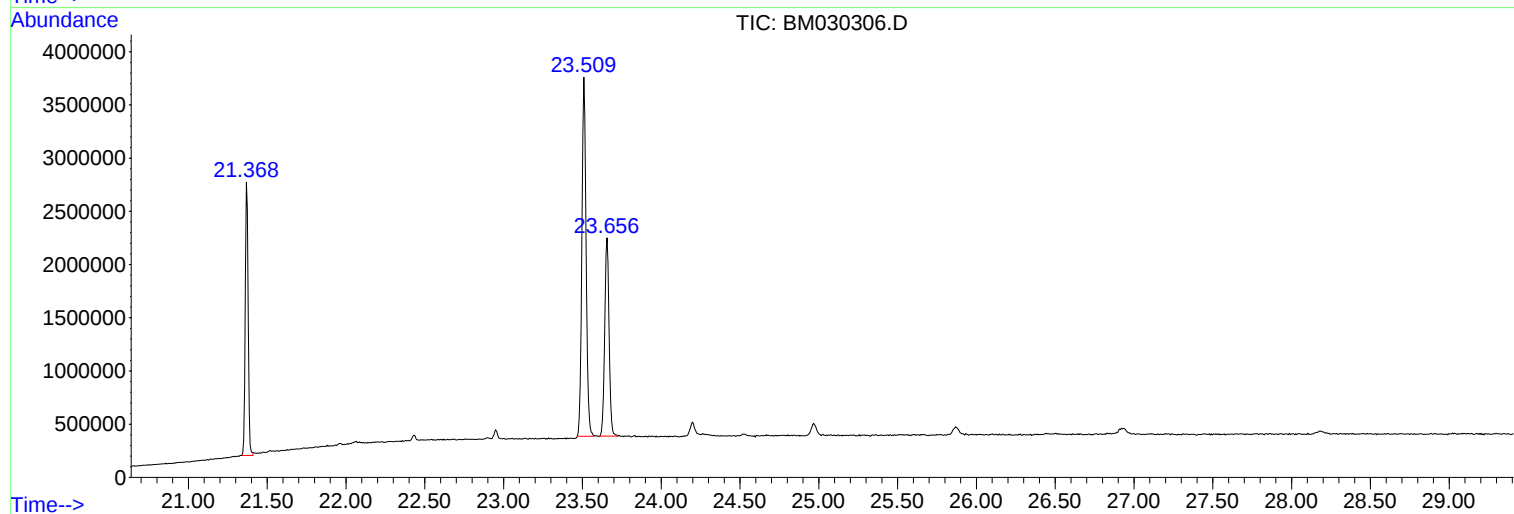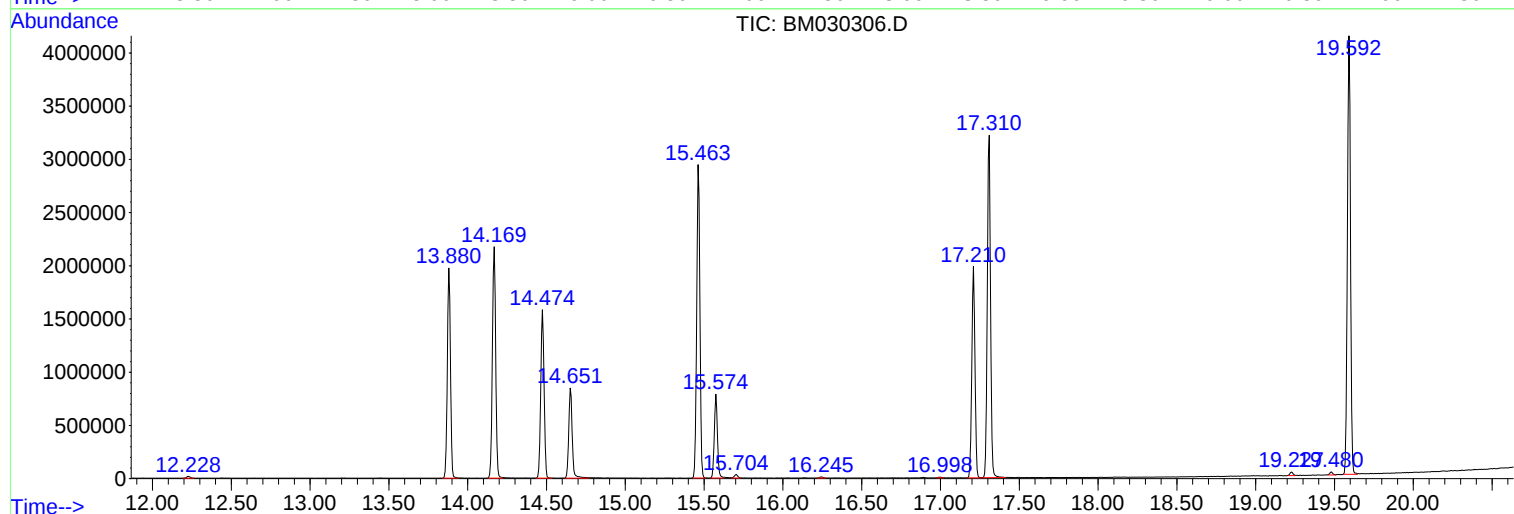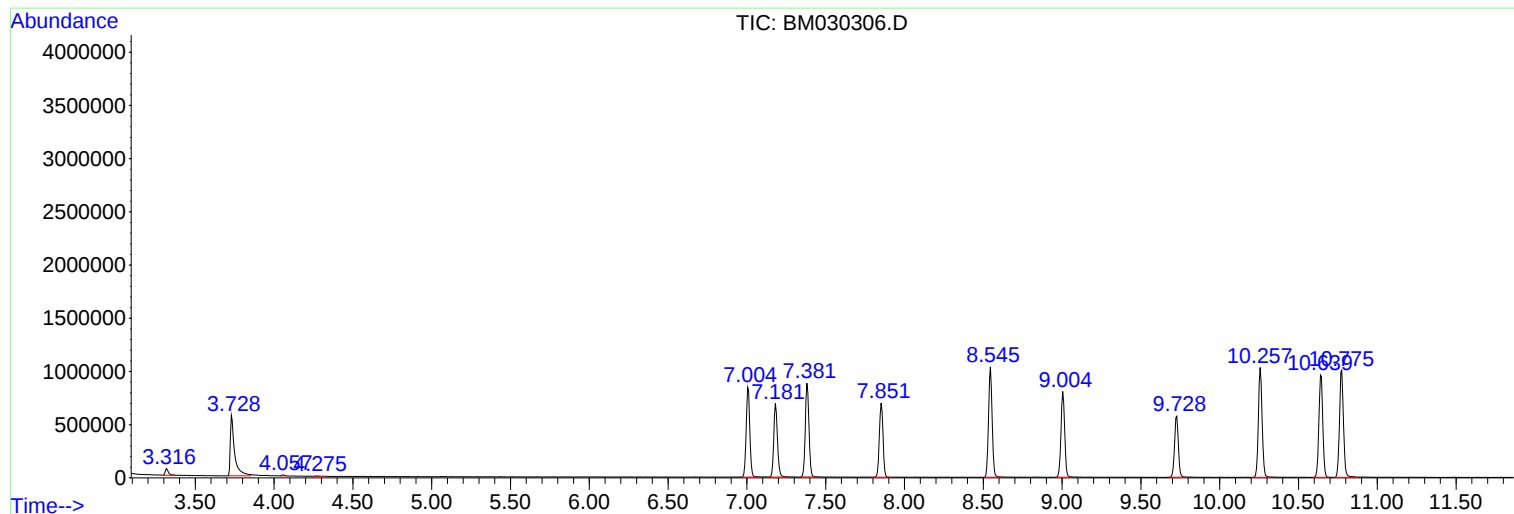

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
Data File : BM030306.D
Acq On : 07 Jun 2021 10:34
Operator : CG/JU
Sample : PB136695BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK695

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
Data File : BM030306.D
Acq On : 07 Jun 2021 10:34
Operator : CG/JU
Sample : PB136695BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK695

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------