

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
 Data File : BM030308.D
 Acq On : 07 Jun 2021 14:39
 Operator : CG/JU
 Sample : PB136692BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030308.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	36	39	57	rVB	70278	113437	2.62%	0.240%
2	3.728	106	109	135	rBV	608601	1115076	25.71%	2.360%
3	4.057	162	165	168	rVB	9814	11125	0.26%	0.024%
4	4.687	268	272	275	rVB5	4864	5773	0.13%	0.012%
5	7.004	660	666	676	rBV	841610	1339511	30.88%	2.834%
6	7.181	690	696	713	rBV	669194	1095218	25.25%	2.317%
7	7.381	723	730	743	rBV	869940	1405682	32.40%	2.974%
8	7.851	803	810	819	rBV	701760	1118417	25.78%	2.367%
9	8.545	920	928	945	rBV	1002725	1601371	36.92%	3.389%
10	9.004	999	1006	1022	rBV	768127	1267239	29.21%	2.681%
11	9.728	1120	1129	1139	rBV	541763	927941	21.39%	1.964%
12	10.257	1212	1219	1231	rBV	966130	1612721	37.18%	3.413%
13	10.639	1275	1284	1293	rBV	932246	1588348	36.62%	3.361%
14	10.775	1299	1307	1320	rBV	939436	1649646	38.03%	3.491%
15	12.228	1547	1554	1560	rBV2	16287	28161	0.65%	0.060%
16	13.880	1828	1835	1845	rBV	1672526	2306058	53.16%	4.880%
17	14.169	1877	1884	1894	rBV	1985888	2835319	65.36%	6.000%
18	14.474	1929	1936	1944	rBV	1408074	2064841	47.60%	4.369%
19	14.651	1958	1966	1986	rBV	726362	1062637	24.50%	2.249%
20	15.463	2097	2104	2115	rVB	2535445	3635205	83.80%	7.692%
21	15.574	2117	2123	2130	rBV	642642	855319	19.72%	1.810%
22	15.704	2140	2145	2152	rVB2	29266	41710	0.96%	0.088%
23	16.245	2234	2237	2242	rVB5	8466	12205	0.28%	0.026%
24	16.992	2361	2364	2371	rVB3	5250	7782	0.18%	0.016%
25	17.210	2394	2401	2411	rBV	1690446	2291505	52.83%	4.849%
26	17.310	2411	2418	2433	rBV	2569676	3738858	86.19%	7.911%
27	18.957	2695	2698	2699	rBV3	3991	4453	0.10%	0.009%
28	19.227	2739	2744	2748	rBV	30601	39825	0.92%	0.084%
29	19.480	2784	2787	2792	rVB	18885	22905	0.53%	0.048%
30	19.592	2800	2806	2817	rBV	3387407	4302915	99.19%	9.105%
31	21.368	3103	3108	3116	rBV	1870262	2362121	54.45%	4.998%
32	23.509	3466	3472	3483	rVB2	2339211	4337863	100.00%	9.179%
33	23.656	3490	3497	3511	rVB	1272392	2457734	56.66%	5.201%




Sum of corrected areas: 47258921

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
Data File : BM030308.D
Acq On : 07 Jun 2021 14:39
Operator : CG/JU
Sample : PB136692BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK592

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

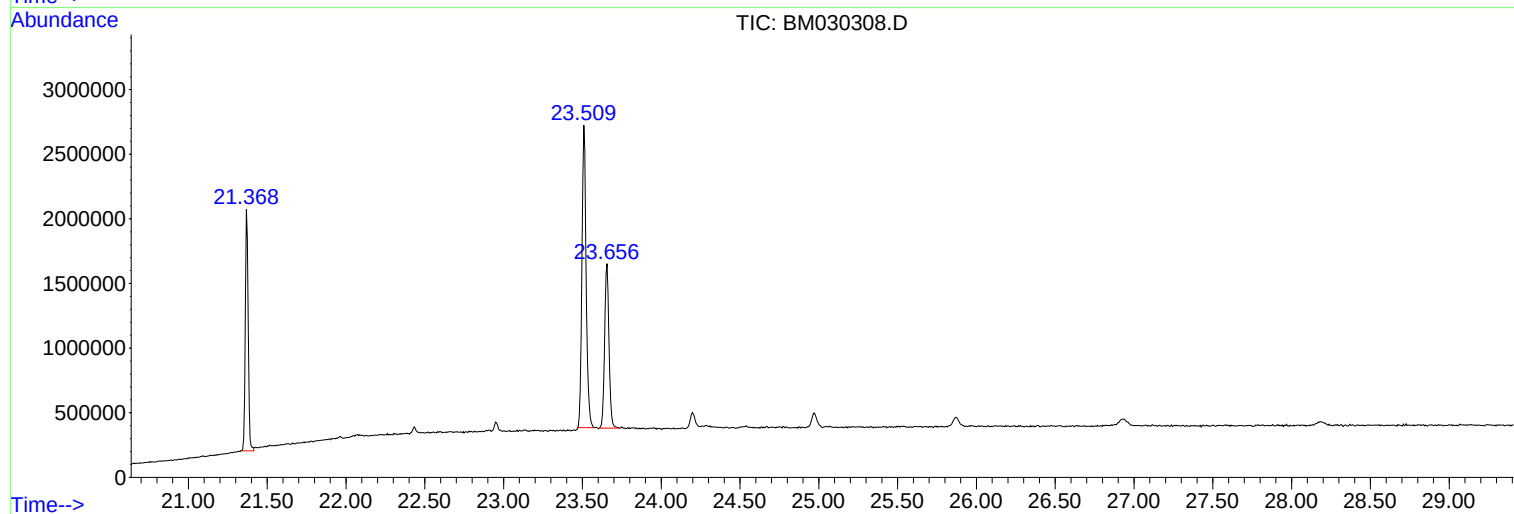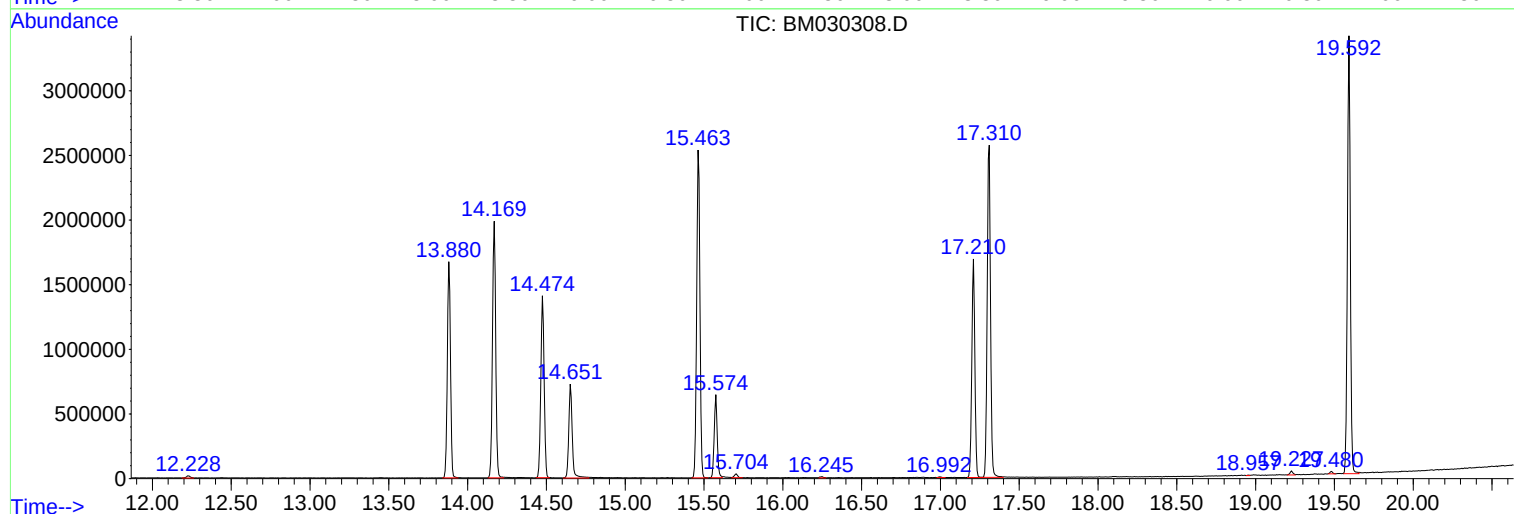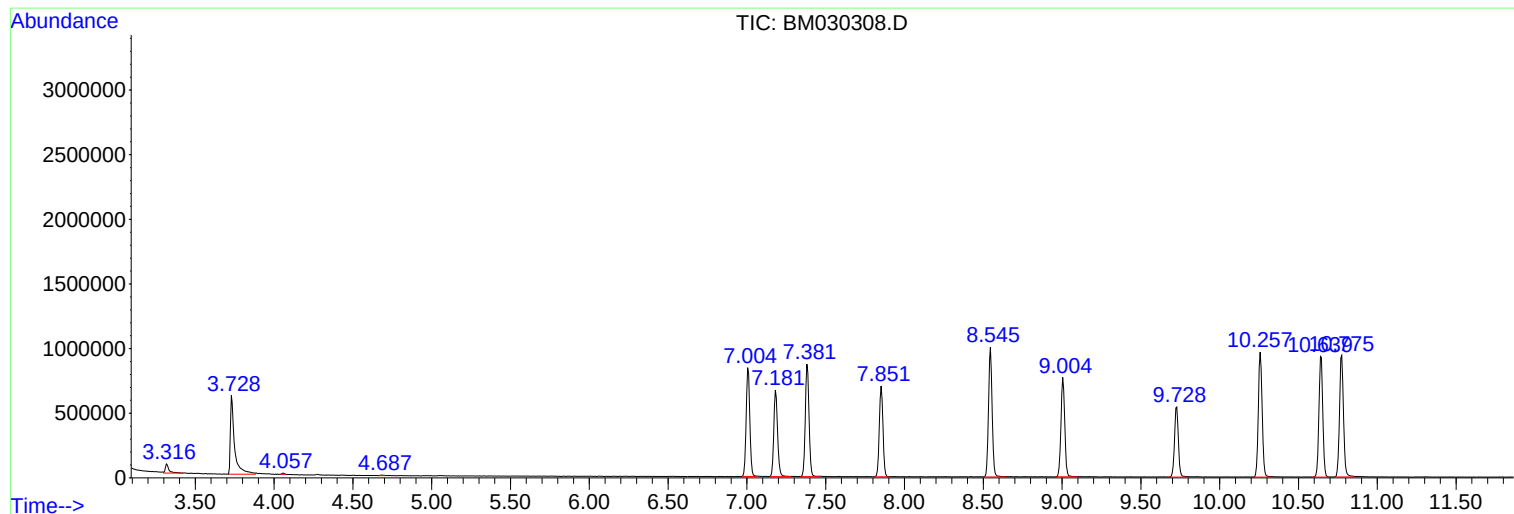

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
Data File : BM030308.D
Acq On : 07 Jun 2021 14:39
Operator : CG/JU
Sample : PB136692BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK592

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060721\
Data File : BM030308.D
Acq On : 07 Jun 2021 14:39
Operator : CG/JU
Sample : PB136692BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK592

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
