

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045887.D
 Acq On : 07 Jun 2024 19:17
 Operator : MA/JU
 Sample : PB161361BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK361

Quant Time: Jun 07 23:01:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.468	152	6540	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.237	136	22858	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.117	164	12016	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.954	188	1335754	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.05
23) Perylene-d12	23.162	264	22189	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.058	96	33518	4.500	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.848	152	8650	0.263	ng/ul	0.00
18) Fluoranthene-d10	18.889	212	15132	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
26) Benzo(a)pyrene	23.028	252	4602	0.063	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045887.D
Acq On : 07 Jun 2024 19:17
Operator : MA/JU
Sample : PB161361BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK361


Quant Time: Jun 07 23:01:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration

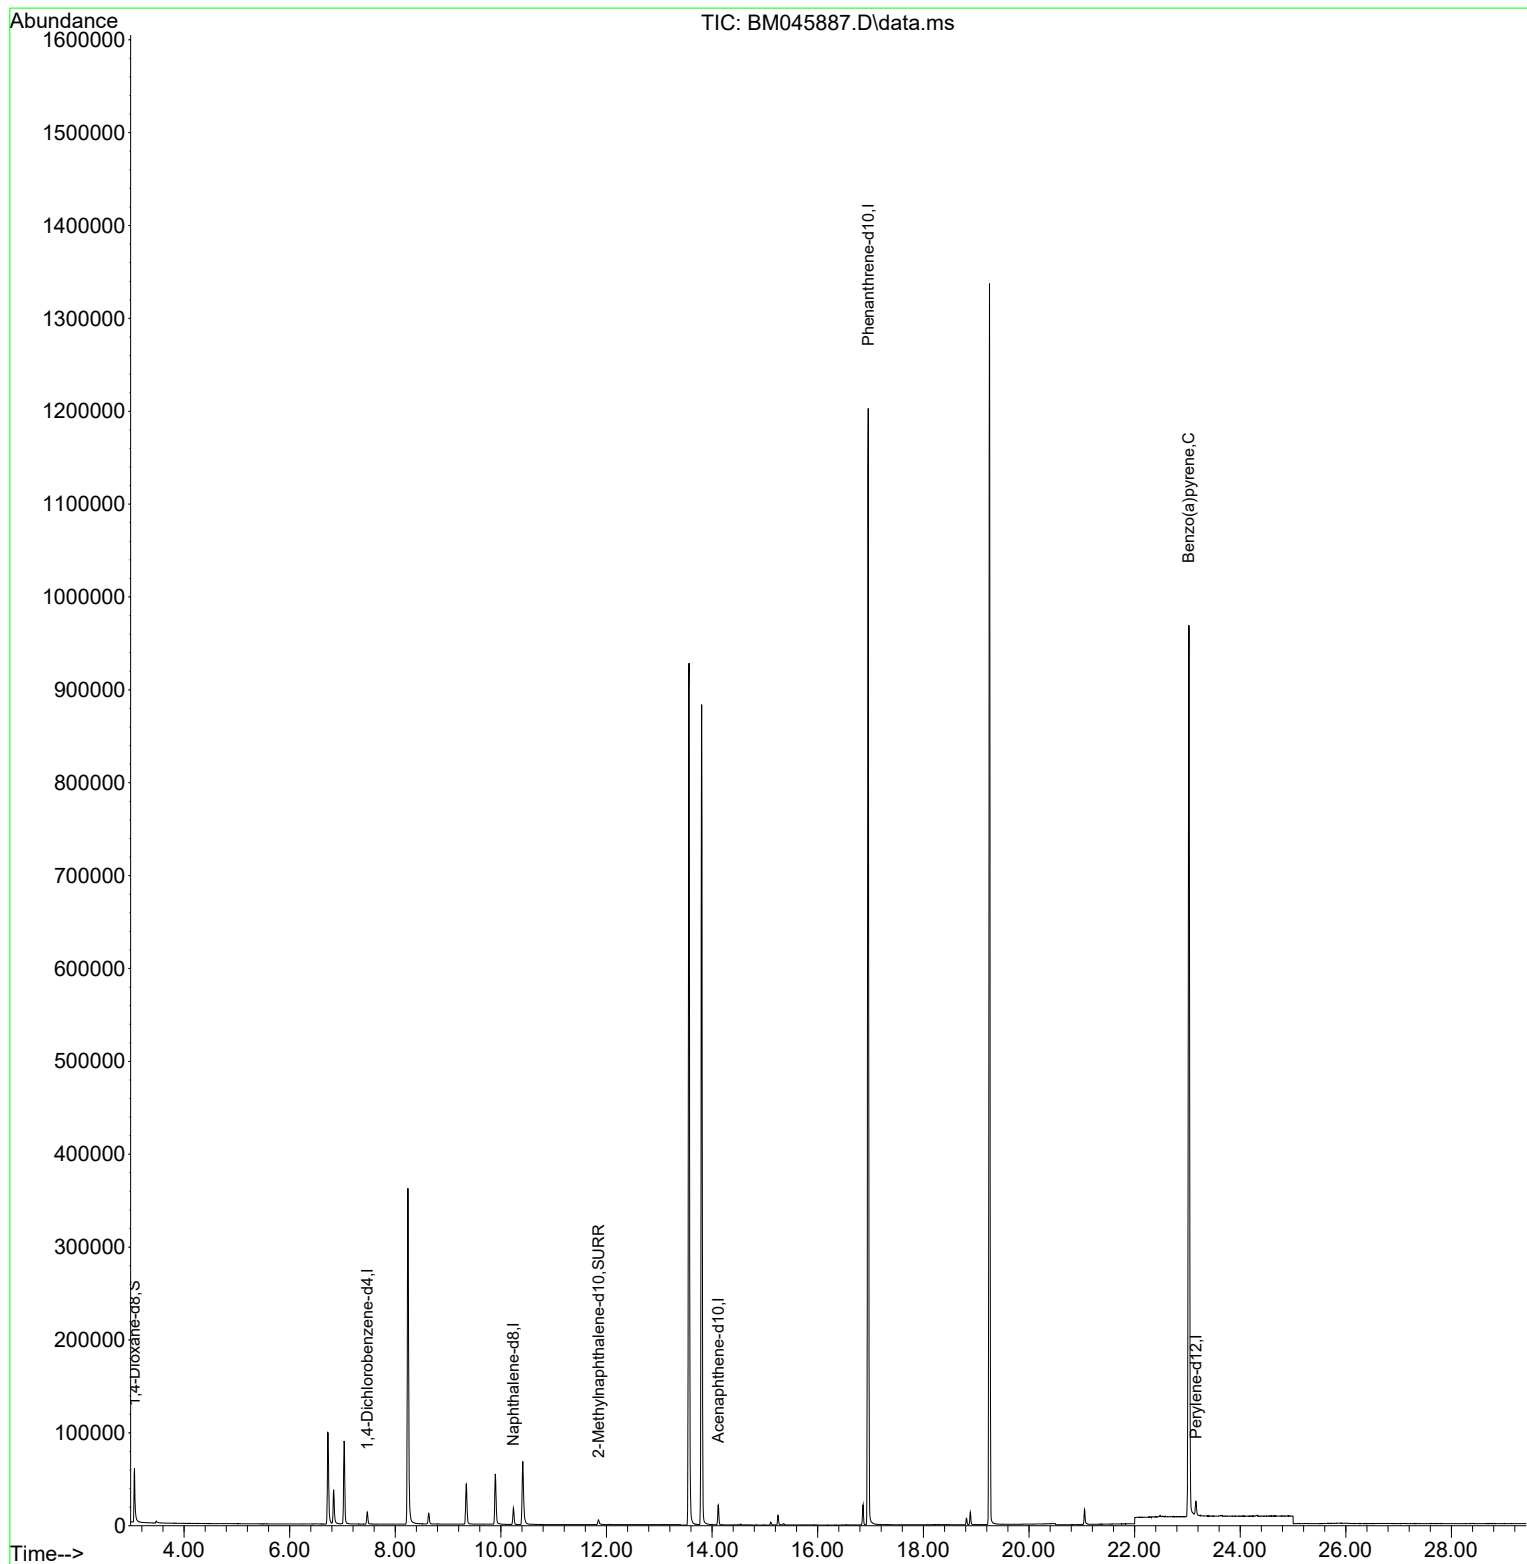

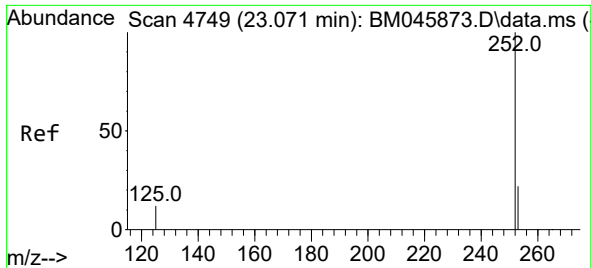

#26
Benzo(a)pyrene
Concen: 0.063 ng/ul
RT: 23.028 min Scan# 41
Delta R.T. -0.044 min
Lab File: BM045887.D
Acq: 07 Jun 2024 19:17

Instrument :
BNA_M
ClientSampleId :
SBLK361

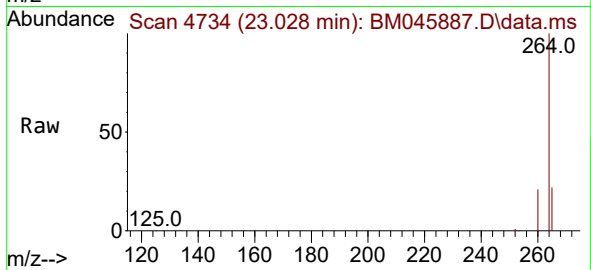

Tgt Ion:252 Resp: 4602
Ion Ratio Lower Upper
252 100
253 72.8 28.8 43.2#
125 57.0 17.3 25.9#

