

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045888.D
 Acq On : 07 Jun 2024 19:54
 Operator : MA/JU
 Sample : P2695-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D61

Quant Time: Jun 07 23:01:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.468	152	5683	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.238	136	19109	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.109	164	10653	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.951	188	1539211	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.05
23) Perylene-d12	23.162	264	20598	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.058	96	23391	3.614	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.833	152	8694	0.316	ng/ul	-0.02
18) Fluoranthene-d10	18.890	212	18252	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.282	128	1860	0.037	ng/ul#	84
26) Benzo(a)pyrene	23.028	252	5422	0.080	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045888.D
Acq On : 07 Jun 2024 19:54
Operator : MA/JU
Sample : P2695-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4D61

Quant Time: Jun 07 23:01:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration

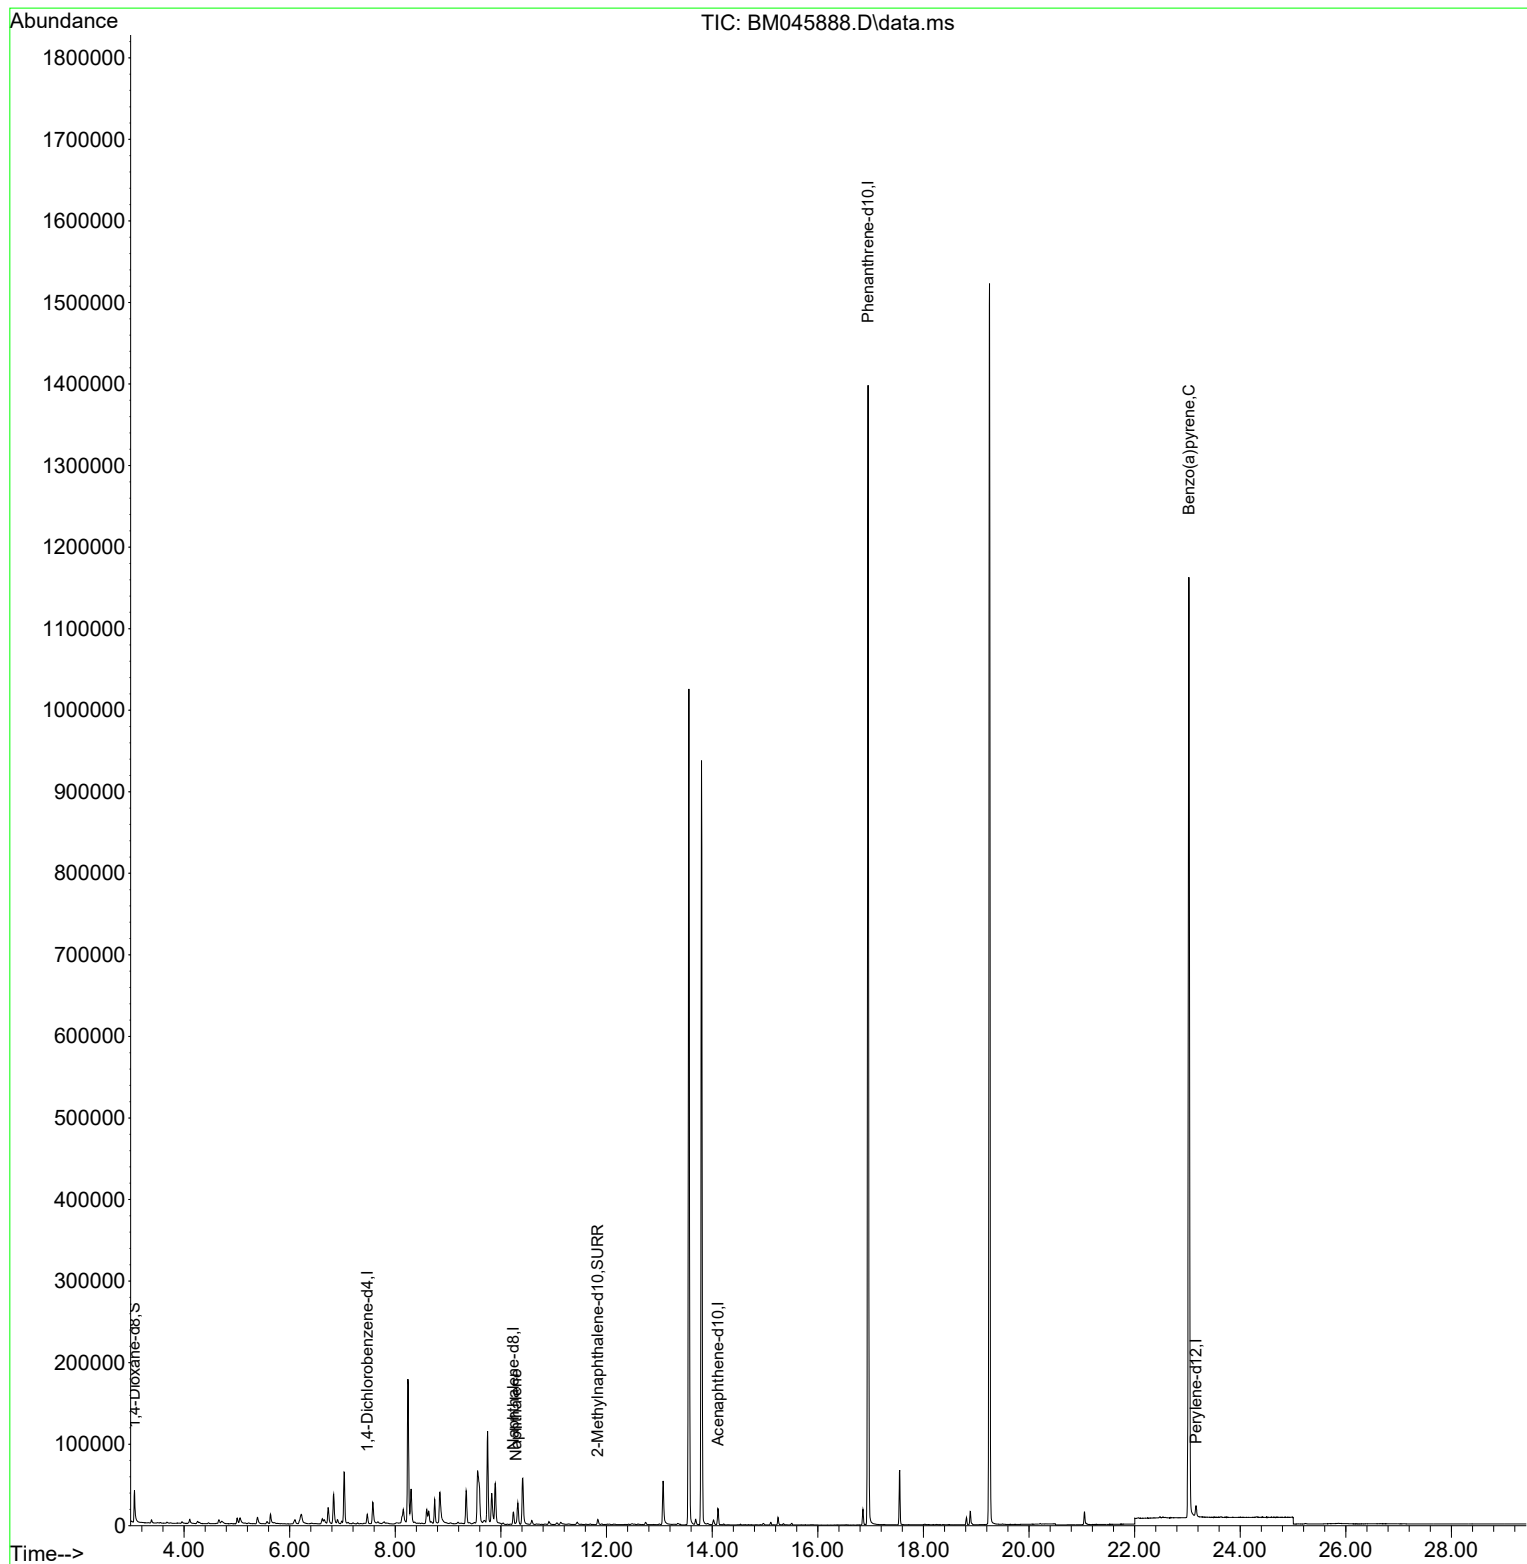

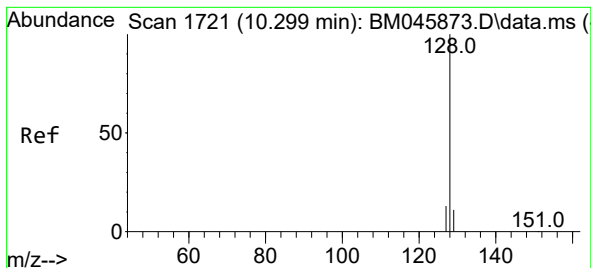

#5

Naphthalene

Concen: 0.037 ng/ul

RT: 10.282 min Scan# 1

Delta R.T. -0.021 min

Lab File: BM045888.D

Acq: 07 Jun 2024 19:54

Instrument :

BNA_M

ClientSampleId :

A4D61





Tgt Ion:128 Resp: 1860

Ion Ratio Lower Upper

128 100

129 18.2 9.4 14.0#

127 19.5 10.6 15.8#

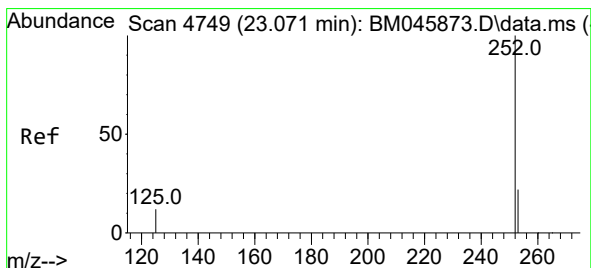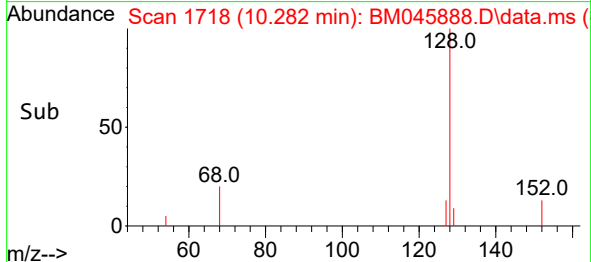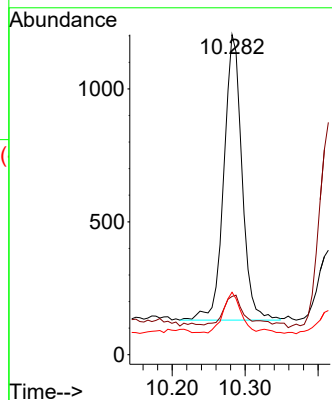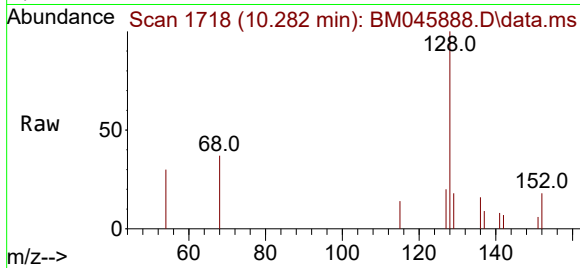

#26

Benzo(a)pyrene

Concen: 0.080 ng/ul

RT: 23.028 min Scan# 4734

Delta R.T. -0.044 min

Lab File: BM045888.D

Acq: 07 Jun 2024 19:54

Tgt Ion:252 Resp: 5422

Ion Ratio Lower Upper

252 100

253 67.1 28.8 43.2#

125 51.7 17.3 25.9#

