

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045912.D
 Acq On : 08 Jun 2024 12:38
 Operator : MA/JU
 Sample : PB161397BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK397

Quant Time: Jun 10 01:27:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.464	152	5628	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.233	136	18902	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.114	164	10247	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.947	188	1226152	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.05
23) Perylene-d12	23.156	264	26062	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.059	96	32039	4.998	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.844	152	6903	0.254	ng/ul	0.00
18) Fluoranthene-d10	18.886	212	15235	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.108	166	2279	0.060	ng/ul#	15
26) Benzo(a)pyrene	23.022	252	4969	0.058	ng/ul#	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045912.D
Acq On : 08 Jun 2024 12:38
Operator : MA/JU
Sample : PB161397BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK397

Quant Time: Jun 10 01:27:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration

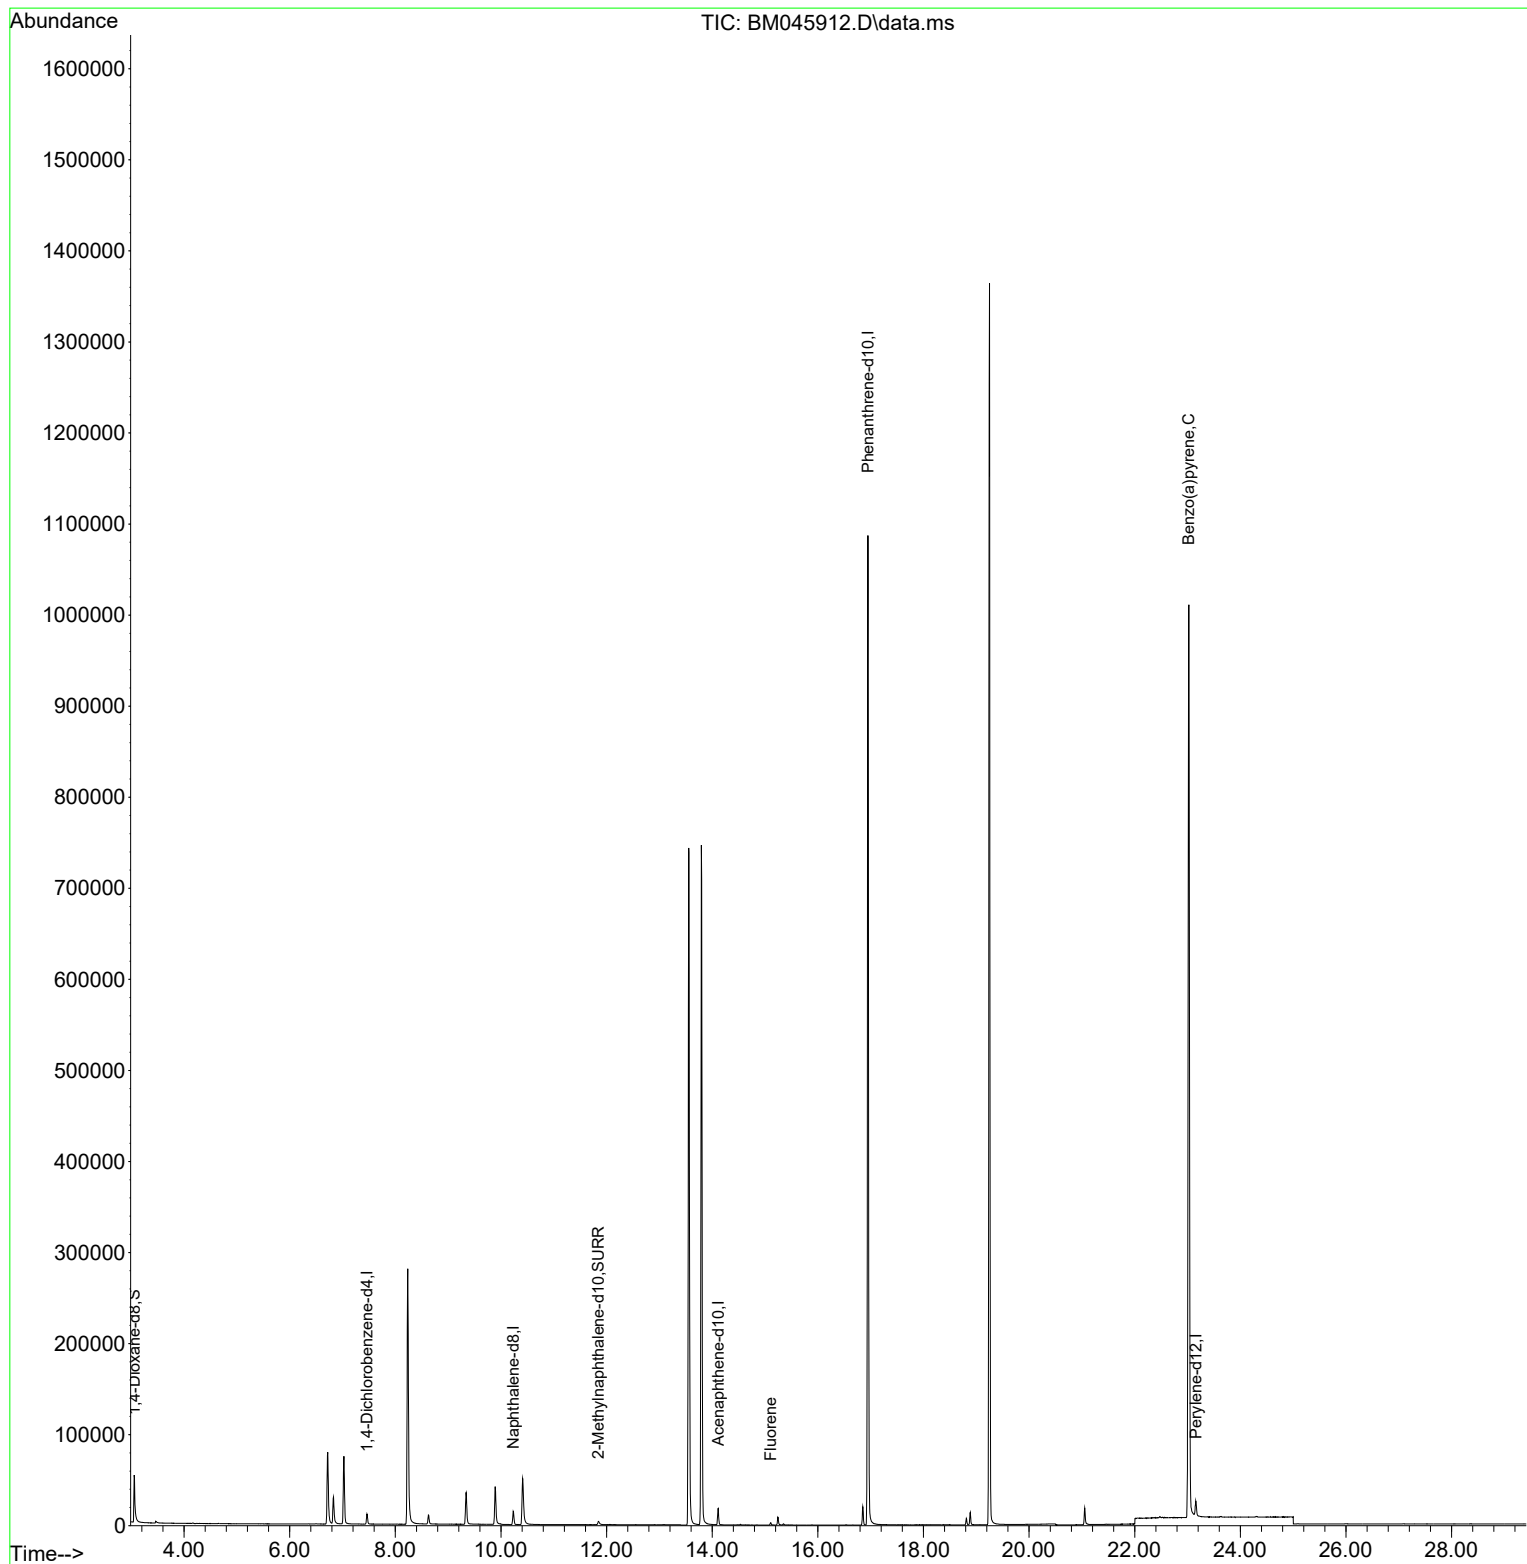

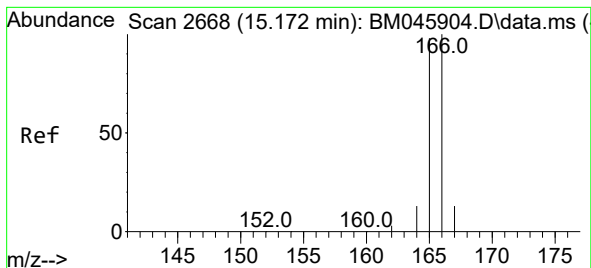

#12

Fluorene

Concen: 0.060 ng/ul

RT: 15.108 min Scan# 2

Delta R.T. -0.068 min

Lab File: BM045912.D

Acq: 08 Jun 2024 12:38

Instrument :

BNA_M

ClientSampleId :

SBLK397





Tgt Ion:166 Resp: 2279

Ion Ratio Lower Upper

166 100

165 9.7 79.7 119.5#

167 35.3 11.3 16.9#

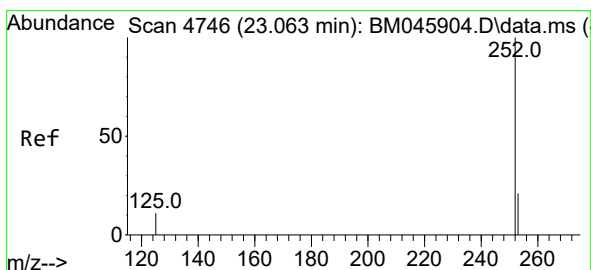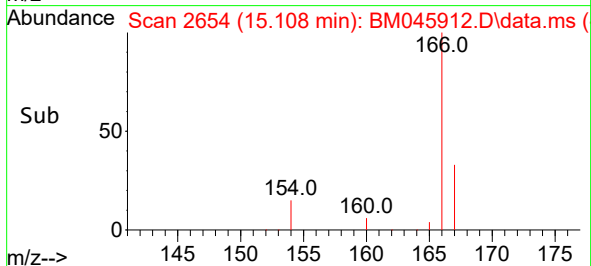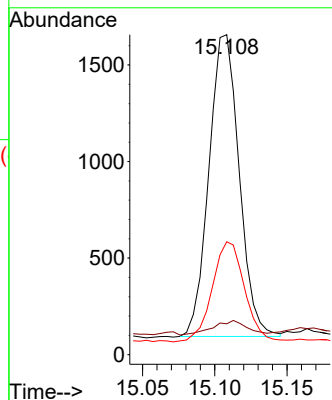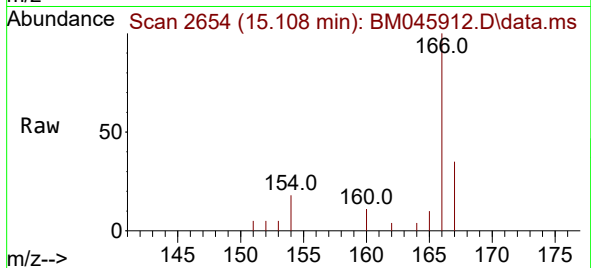

#26

Benzo(a)pyrene

Concen: 0.058 ng/ul

RT: 23.022 min Scan# 4732

Delta R.T. -0.050 min

Lab File: BM045912.D

Acq: 08 Jun 2024 12:38

Tgt Ion:252 Resp: 4969

Ion Ratio Lower Upper

252 100

253 66.2 28.8 43.2#

125 54.4 17.3 25.9#

