

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045925.D
 Acq On : 08 Jun 2024 20:30
 Operator : MA/JU
 Sample : P2640-13
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D66

Quant Time: Jun 10 01:29:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.463	152	5452	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.231	136	17102	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.107	164	8497	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.946	188	1204692	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.05
23) Perylene-d12	23.154	264	22032	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.058	96	23455	3.777	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.837	152	6417	0.261	ng/ul	-0.01
18) Fluoranthene-d10	18.885	212	14853	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.281	128	1284	0.029	ng/ul#	81
26) Benzo(a)pyrene	23.019	252	5204	0.072	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045925.D
Acq On : 08 Jun 2024 20:30
Operator : MA/JU
Sample : P2640-13
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4D66

Quant Time: Jun 10 01:29:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration




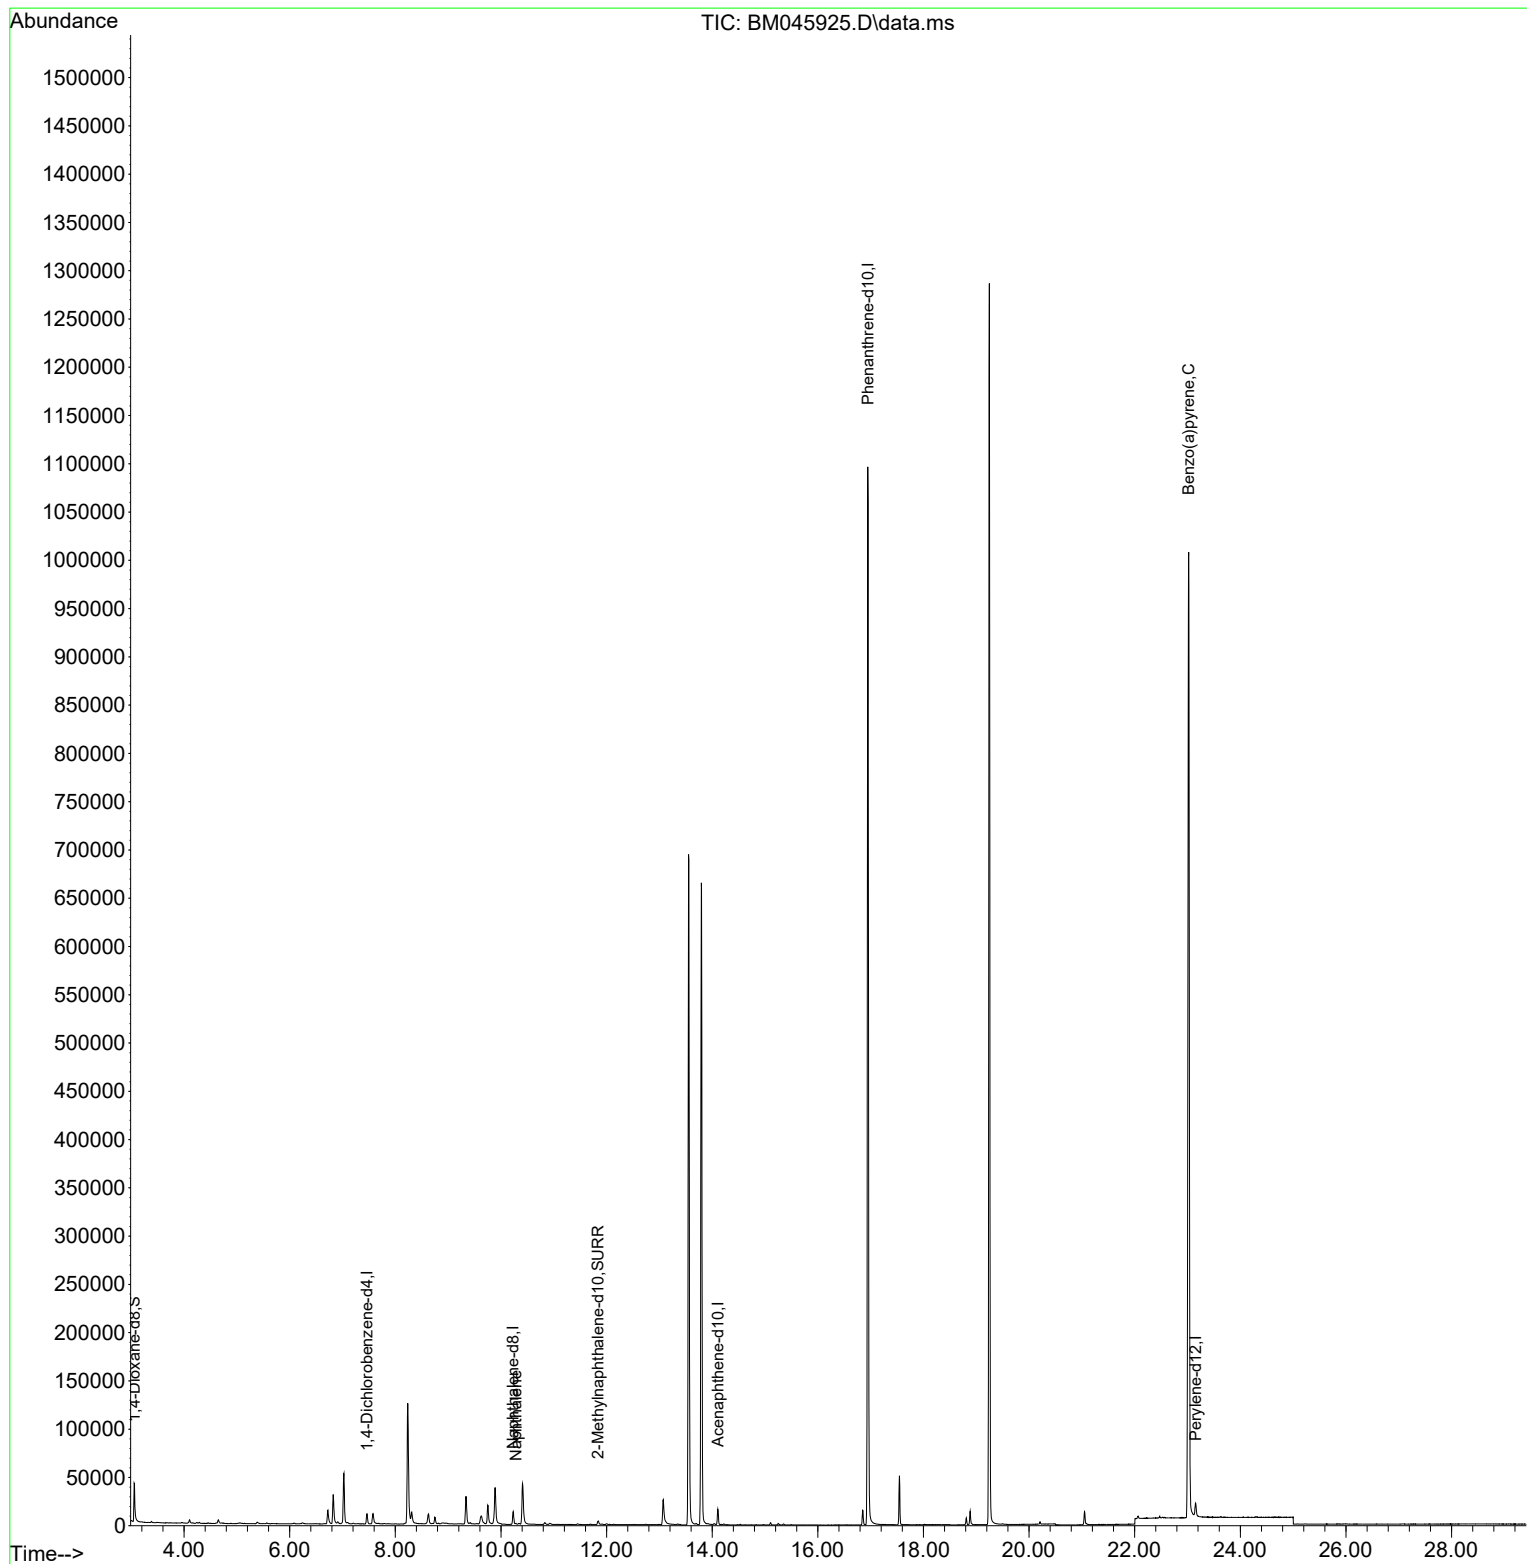


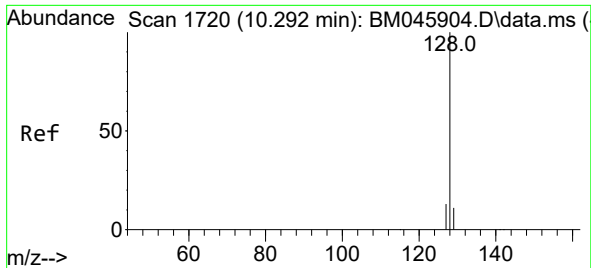

#5
Naphthalene
Concen: 0.029 ng/ul
RT: 10.281 min Scan# 11
Delta R.T. -0.022 min
Lab File: BM045925.D
Acq: 08 Jun 2024 20:30

Instrument :
BNA_M
ClientSampleId :
A4D66

Tgt Ion:128 Resp: 1284
Ion Ratio Lower Upper
128 100
129 21.6 9.4 14.0#
127 18.8 10.6 15.8#

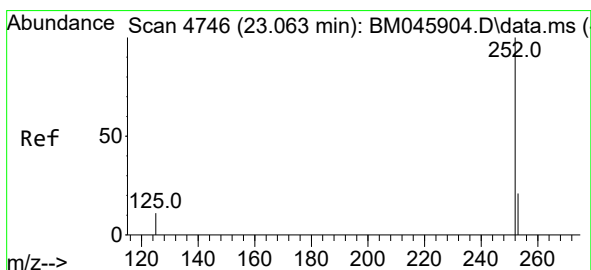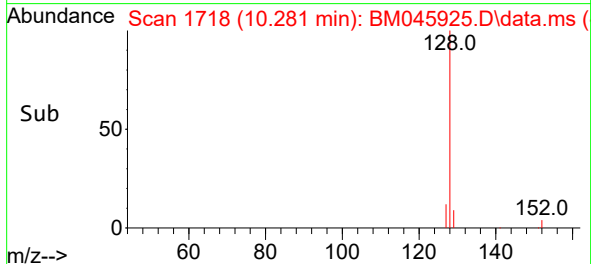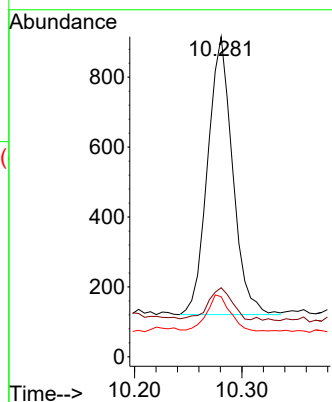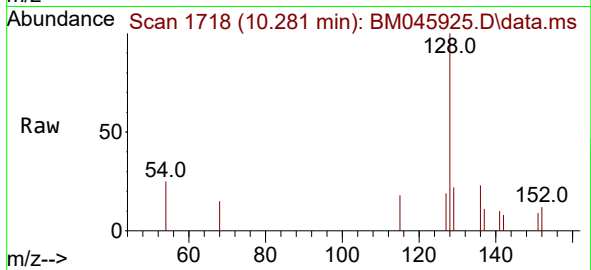

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.019 min Scan# 4731
Delta R.T. -0.053 min
Lab File: BM045925.D
Acq: 08 Jun 2024 20:30

Tgt Ion:252 Resp: 5204
Ion Ratio Lower Upper
252 100
253 63.5 28.8 43.2#
125 51.0 17.3 25.9#

