

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045929.D
 Acq On : 08 Jun 2024 23:31
 Operator : MA/JU
 Sample : PB161252BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK252

Quant Time: Jun 10 01:30:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	5672	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.233	136	18126	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.109	164	9286	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.947	188	1117110	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.05
23) Perylene-d12	23.151	264	23221	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.054	96	35523	5.499	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.849	152	6570	0.252	ng/ul	0.00
18) Fluoranthene-d10	18.881	212	12815	0.000	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.104	166	2167	0.062	ng/ul#	15
26) Benzo(a)pyrene	23.016	252	4637	0.061	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045929.D
Acq On : 08 Jun 2024 23:31
Operator : MA/JU
Sample : PB161252BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK252

Quant Time: Jun 10 01:30:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration




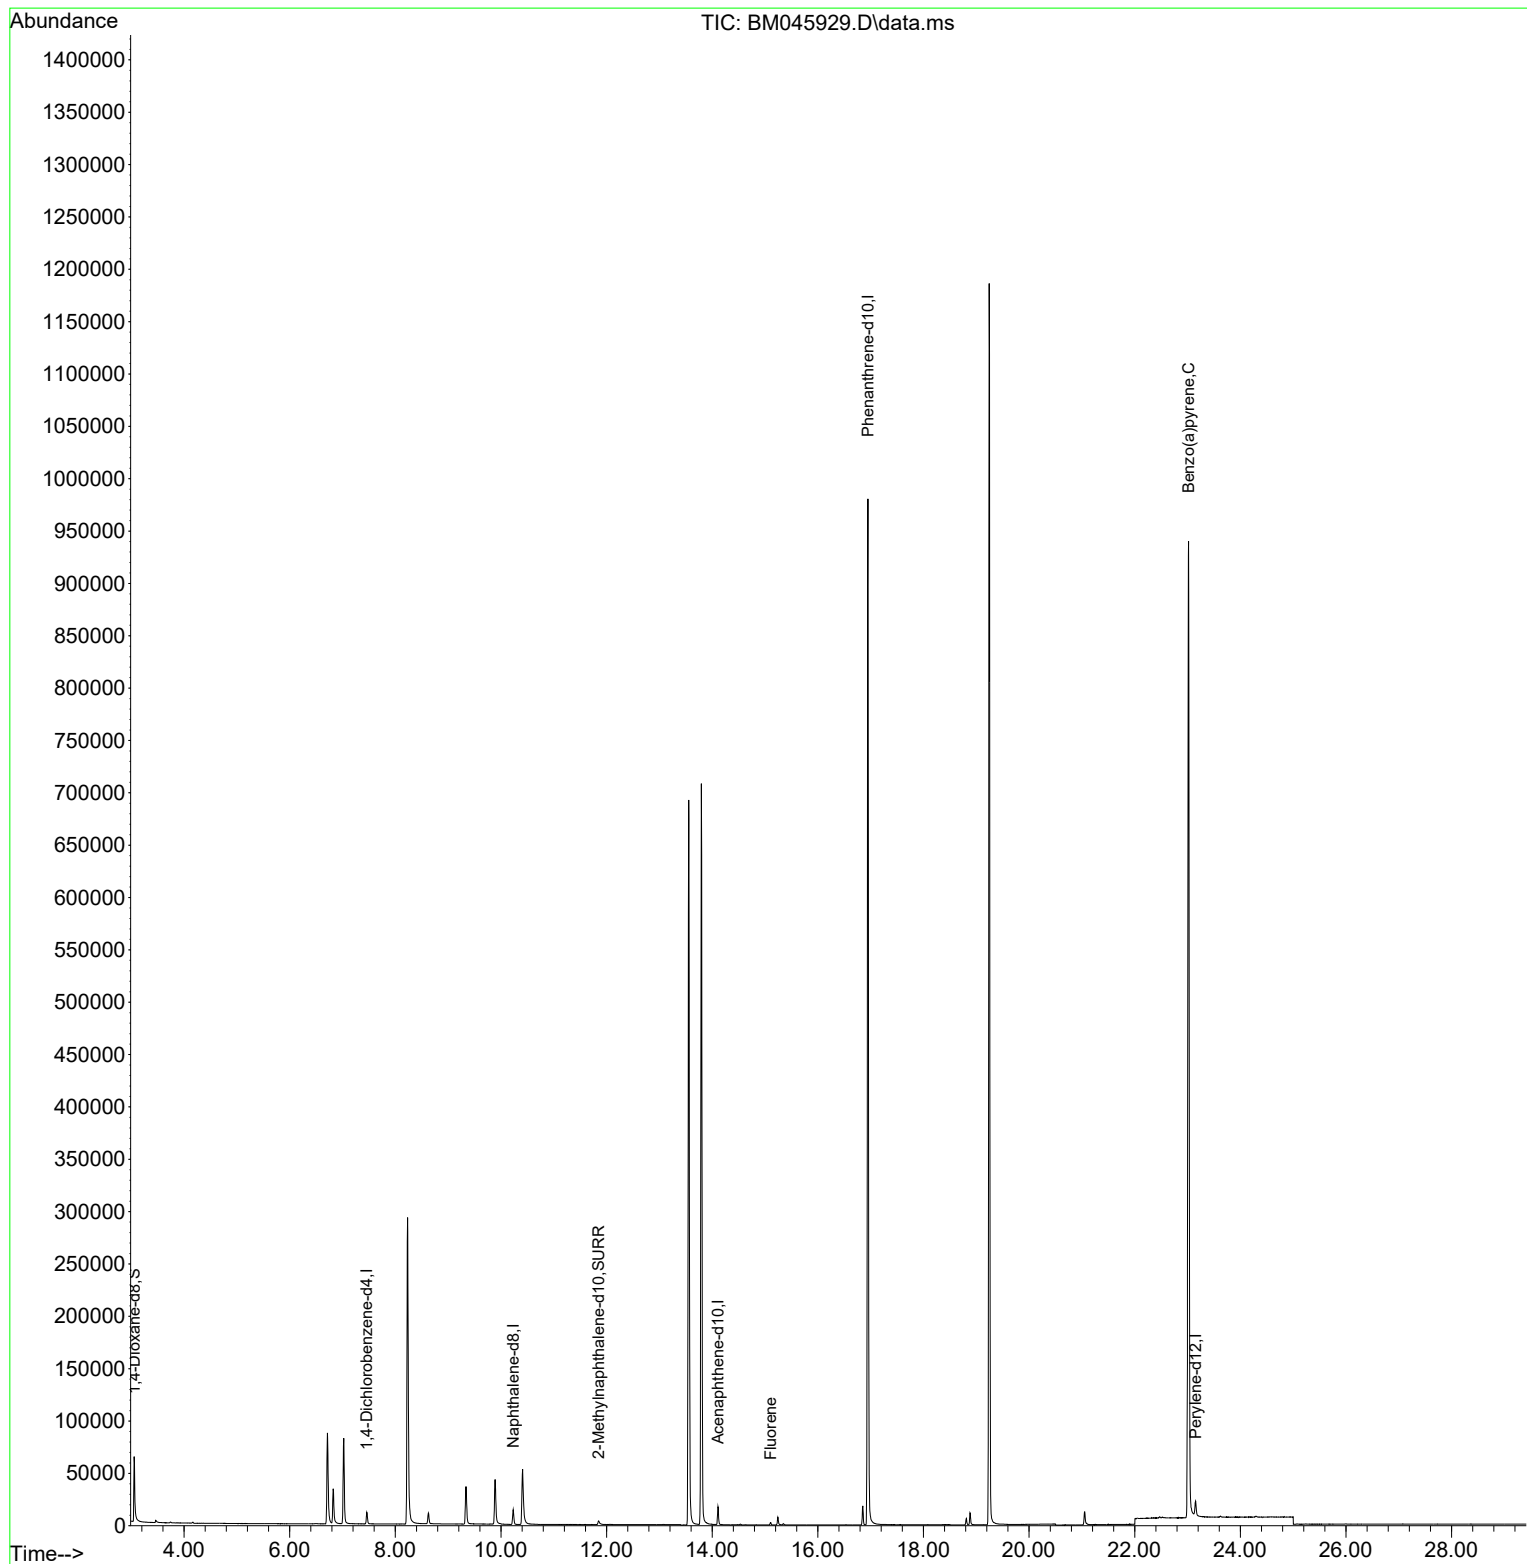


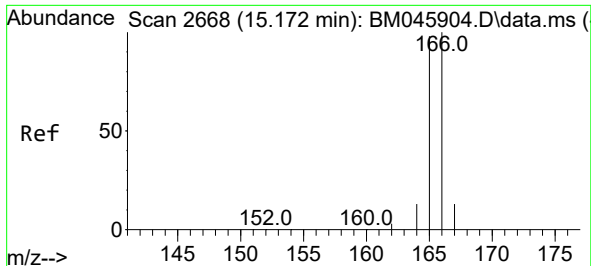

#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.104 min Scan# 2167
Delta R.T. -0.073 min
Lab File: BM045929.D
Acq: 08 Jun 2024 23:31

Instrument :
BNA_M
ClientSampleId :
SBLK252

Tgt Ion	Ratio	Lower	Upper
166	100		
165	9.5	79.7	119.5#
167	33.4	11.3	16.9#

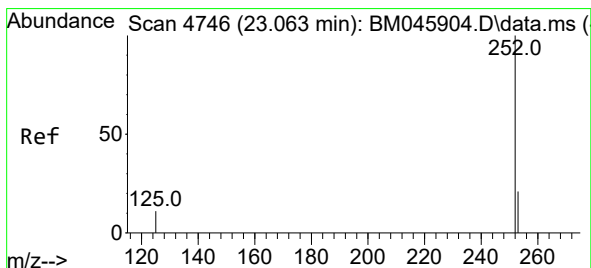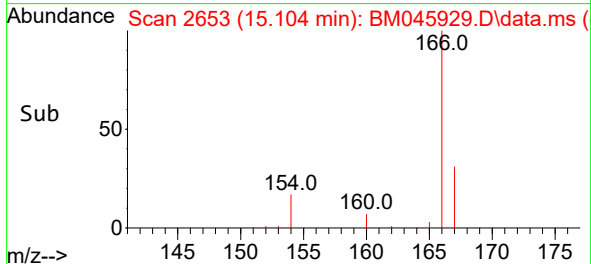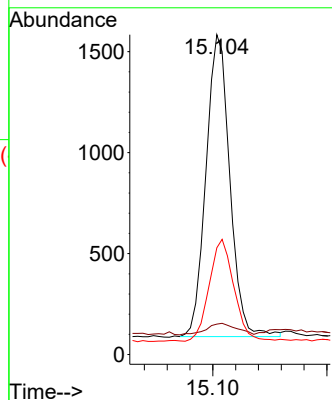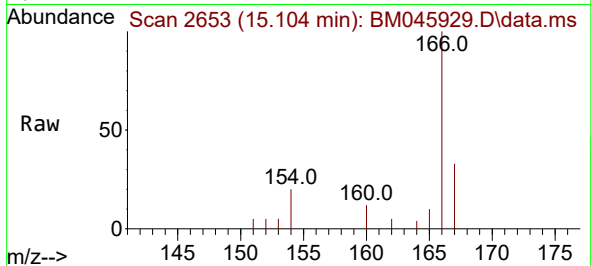

#26
Benzo(a)pyrene
Concen: 0.061 ng/ul
RT: 23.016 min Scan# 4730
Delta R.T. -0.056 min
Lab File: BM045929.D
Acq: 08 Jun 2024 23:31

Tgt Ion	Ratio	Lower	Upper
252	100		
253	63.0	28.8	43.2#
125	51.9	17.3	25.9#

