

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045925.D
 Acq On : 08 Jun 2024 20:30
 Operator : MA/JU
 Sample : P2696-13
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D66

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/10/2024
 Supervised By :mohammad ahmed 06/13/2024

Quant Time: Jun 10 01:29:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.463	152	5452	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.231	136	17102	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.107	164	8497	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.849	188	17960m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.050	240	14209m	0.400	ng/ul	0.00
23) Perylene-d12	23.154	264	15113m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.058	96	23455	3.777	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.837	152	6417	0.261	ng/ul	-0.01
18) Fluoranthene-d10	18.885	212	14853	0.349	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.281	128	1284	0.029	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045925.D
Acq On : 08 Jun 2024 20:30
Operator : MA/JU
Sample : P2696-13
Misc :
ALS Vial : 53 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4D66

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/10/2024
Supervised By :mohammad ahmed 06/13/2024


Quant Time: Jun 10 01:29:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration

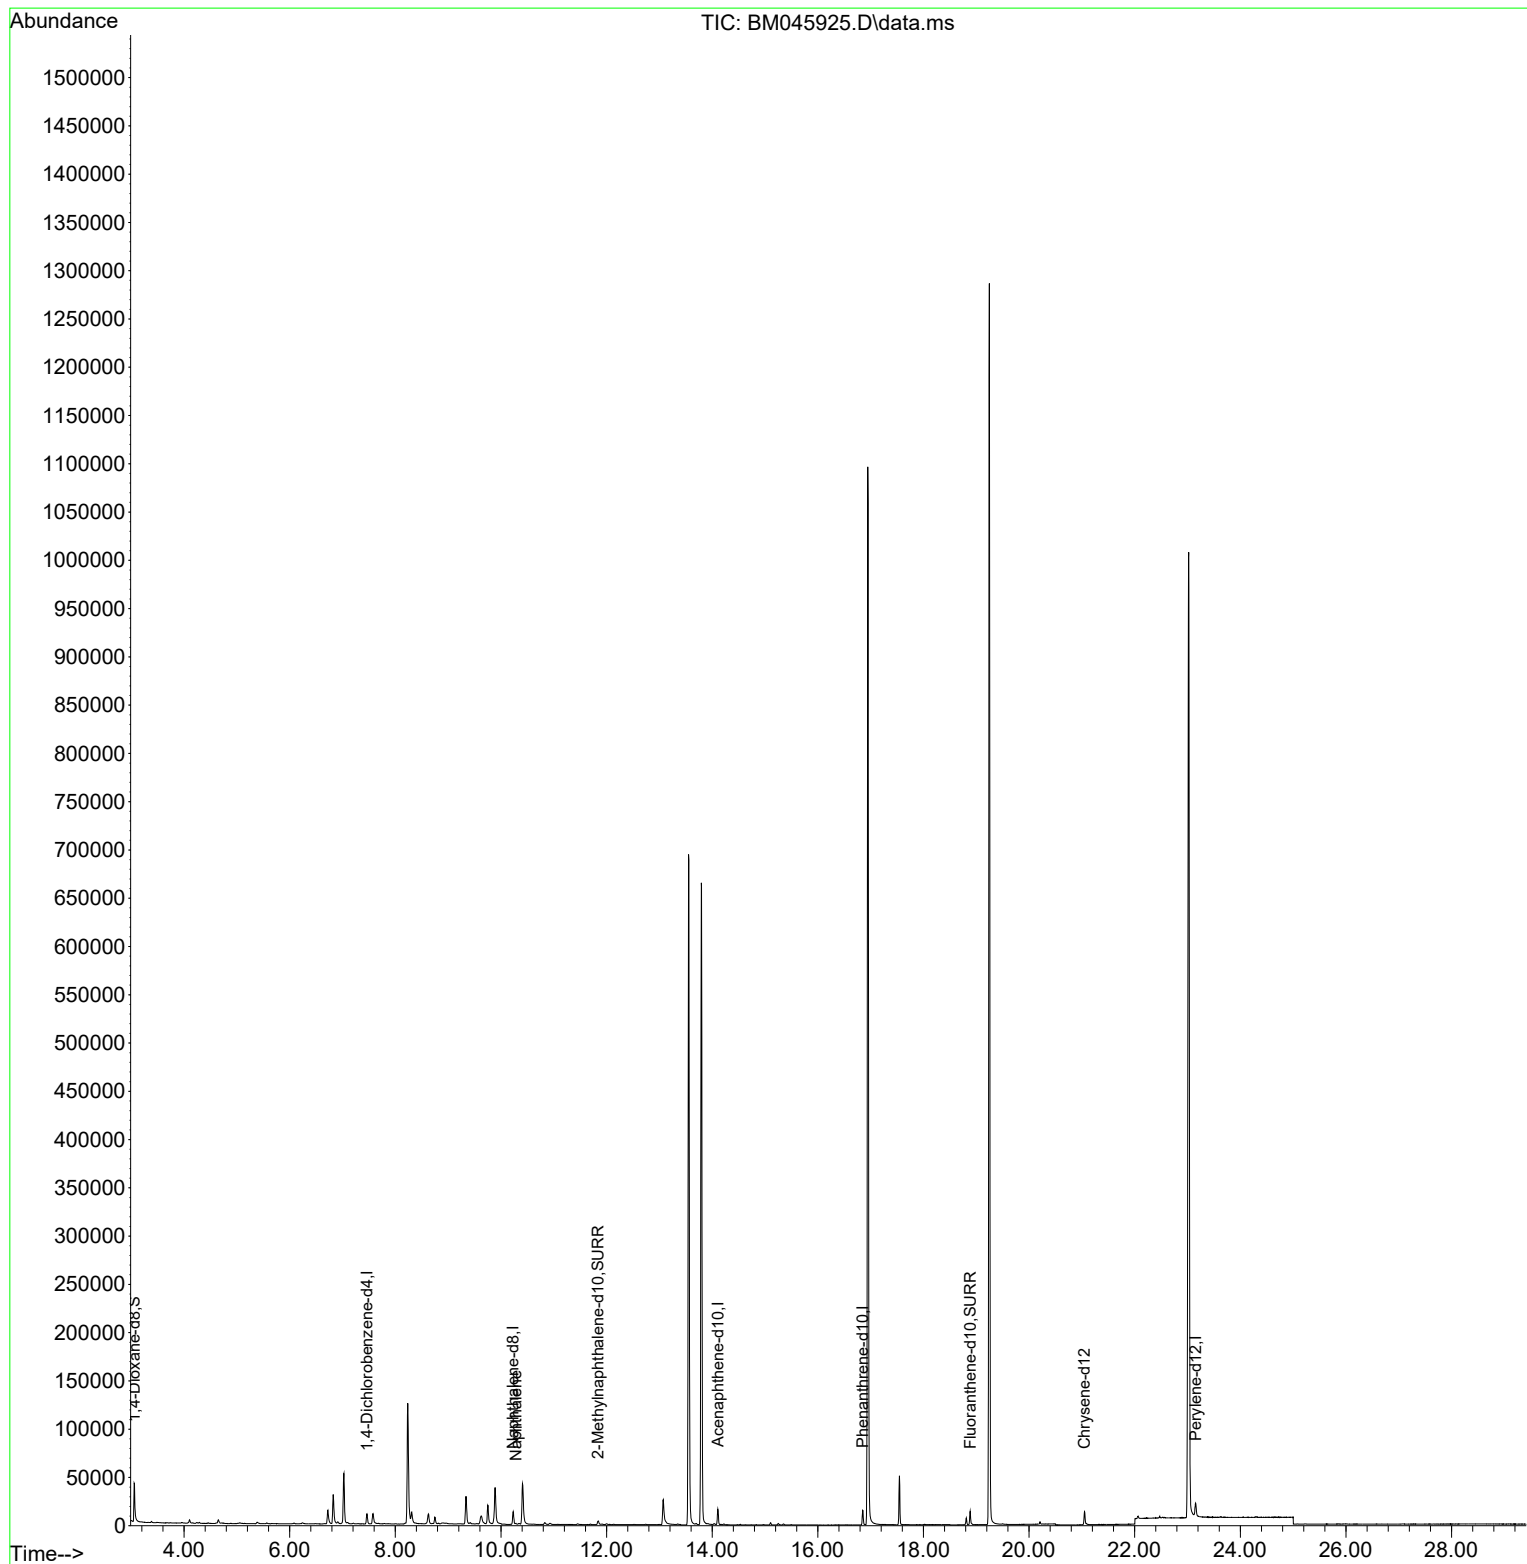

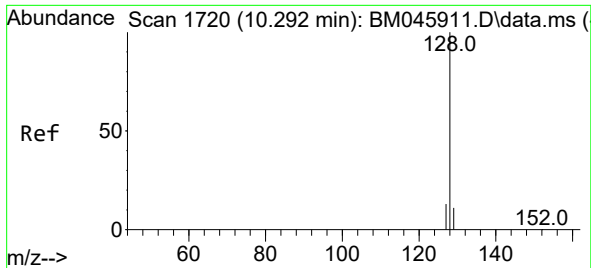

#5
Naphthalene
Concen: 0.029 ng/ul
RT: 10.281 min Scan# 1718
Delta R.T. -0.022 min
Lab File: BM045925.D
Acq: 08 Jun 2024 20:30

Instrument :
BNA_M
ClientSampleId :
A4D66

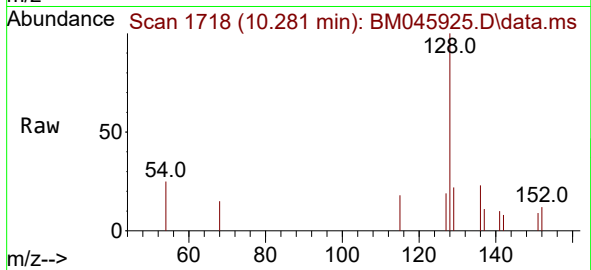

Tgt Ion:128 Resp: 1284
Ion Ratio Lower Upper
128 100
129 21.6 9.4 14.0
127 18.8 10.6 15.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

