

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
 Data File : BM045938.D
 Acq On : 09 Jun 2024 05:00
 Operator : MA/JU
 Sample : P2640-21DL 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4C25DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/10/2024
 Supervised By :mohammad ahmed 06/13/2024

Quant Time: Jun 10 01:32:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 22:59:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.464	152	6110	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.242	136	19450	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.112	164	10610	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.853	188	20899	0.400	ng/ul	-0.01
17) Chrysene-d12	21.041	240	17303	0.400	ng/ul	-0.01
23) Perylene-d12	23.148	264	19211m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.063	96	4626	0.665	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.854	152	1085	0.039	ng/ul	0.00
18) Fluoranthene-d10	18.880	212	2388	0.046	ng/ul	-0.01
Target Compounds					Qvalue	
5) Naphthalene	10.286	128	4250	0.084	ng/ul#	94
7) 2-Methylnaphthalene	11.931	142	1199	0.037	ng/ul	100
8) 1-Methylnaphthalene	12.145	142	1051	0.030	ng/ul	98
10) Acenaphthylene	13.830	152	2409	0.050	ng/ul#	90
11) Acenaphthene	14.172	153	2952	0.083	ng/ul	98
12) Fluorene	15.162	166	3513	0.089	ng/ul	97
15) Phenanthrene	16.891	178	56795	0.968	ng/ul	100
16) Anthracene	16.984	178	11722	0.234	ng/ul#	95
19) Fluoranthene	18.913	202	74234	1.076	ng/ul	98
20) Pyrene	19.275	202	63156	0.877	ng/ul	96
21) Benzo(a)anthracene	21.026	228	29611	0.466	ng/ul	97
22) Chrysene	21.079	228	31328	0.453	ng/ul	98
24) Benzo(b)fluoranthene	22.528	252	38322m	0.601	ng/ul	
25) Benzo(k)fluoranthene	22.563	252	14420m	0.206	ng/ul	
26) Benzo(a)pyrene	23.054	252	26705	0.421	ng/ul	90
27) Indeno(1,2,3-cd)pyrene	25.212	276	19797	0.242	ng/ul#	89
28) Dibenzo(a,h)anthracene	25.219	278	4592	0.070	ng/ul#	65
29) Benzo(g,h,i)perylene	25.843	276	19488	0.276	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060724\
Data File : BM045938.D
Acq On : 09 Jun 2024 05:00
Operator : MA/JU
Sample : P2640-21DL 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4C25DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024


Quant Time: Jun 10 01:32:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 22:59:16 2024
Response via : Initial Calibration

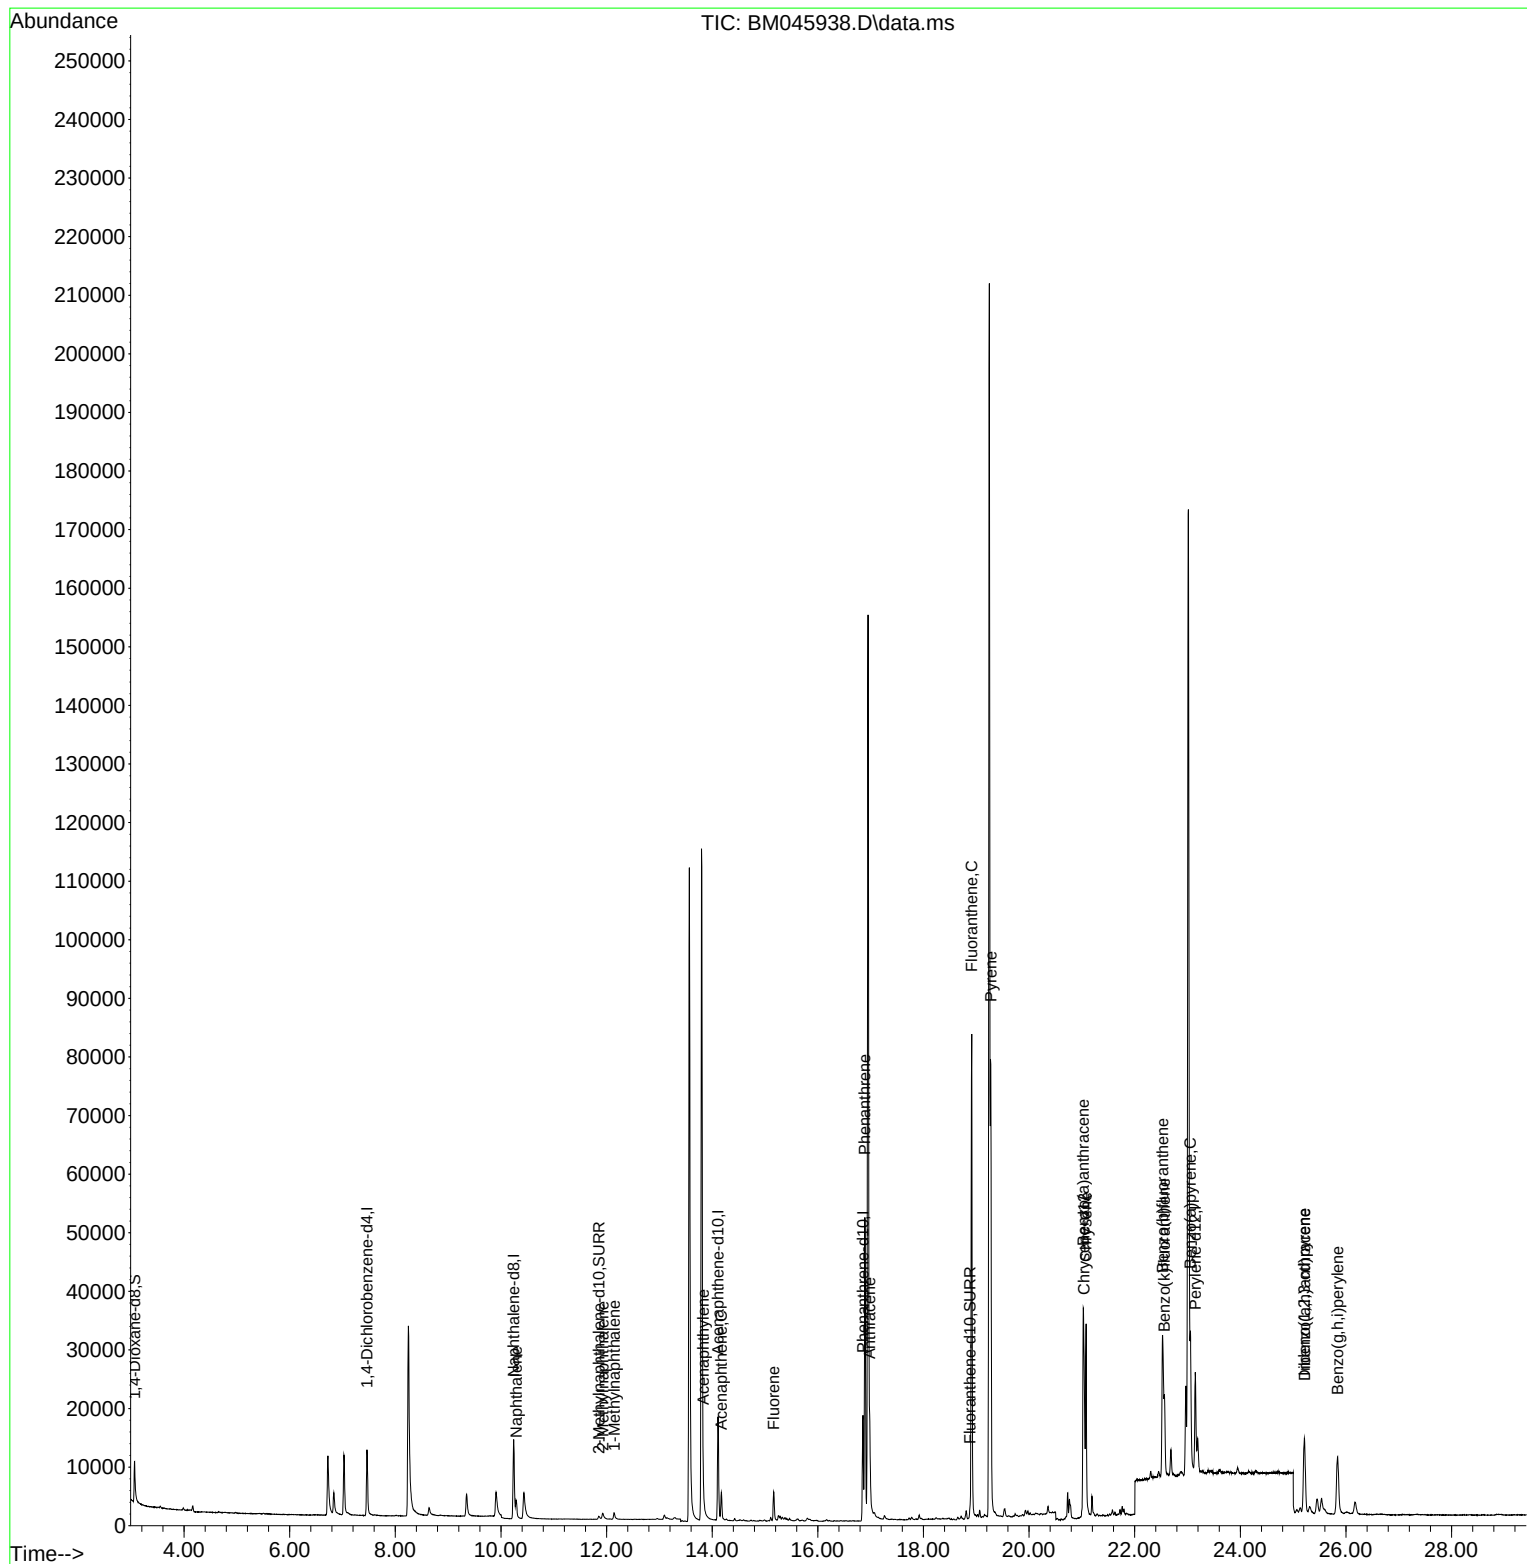



#5
Naphthalene
Concen: 0.084 ng/ul
RT: 10.286 min Scan# 1719
Delta R.T. -0.017 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00




Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:128 Resp: 4250
Ion Ratio Lower Upper
128 100
129 14.7 9.4 14.0
127 14.8 10.6 15.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

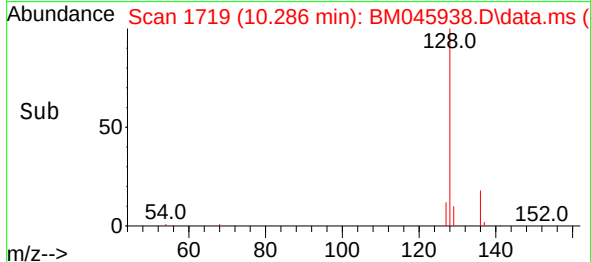

#7
2-Methylnaphthalene
Concen: 0.037 ng/ul
RT: 11.931 min Scan# 2018
Delta R.T. 0.011 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:142 Resp: 1199
Ion Ratio Lower Upper
142 100
141 90.0 72.2 108.4

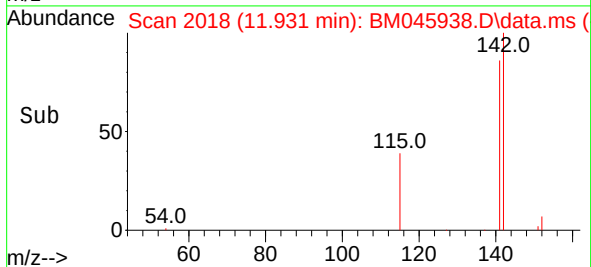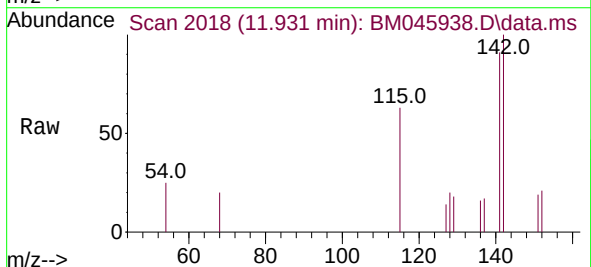



#8
1-Methylnaphthalene
Concen: 0.030 ng/ul
RT: 12.145 min Scan# 2057
Delta R.T. -0.000 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00




Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:142 Resp: 105
Ion Ratio Lower Upper
142 100
141 93.5 73.5 110.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024



#10
Acenaphthylene
Concen: 0.050 ng/ul
RT: 13.830 min Scan# 2378
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:152 Resp: 2409
Ion Ratio Lower Upper
152 100
151 24.2 16.4 24.6
153 19.1 11.1 16.7#

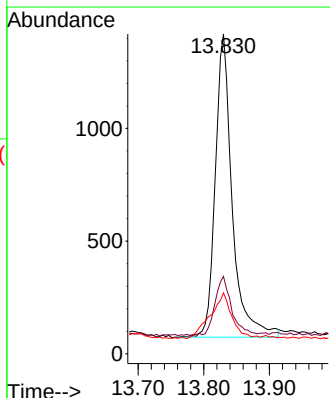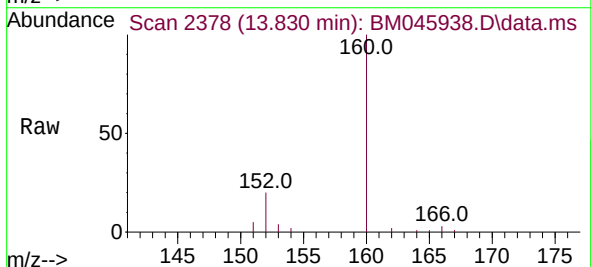



#11
Acenaphthene
Concen: 0.083 ng/ul
RT: 14.172 min Scan# 2452
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00




Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:153 Resp: 2952
Ion Ratio Lower Upper
153 100
152 51.0 39.0 58.4
154 86.3 69.4 104.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

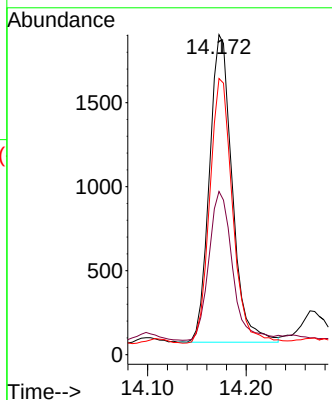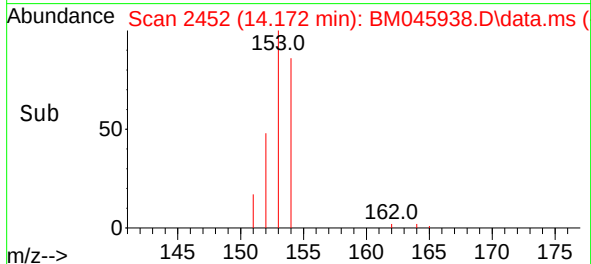

#12
Fluorene
Concen: 0.089 ng/ul
RT: 15.162 min Scan# 2666
Delta R.T. -0.014 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00

Tgt Ion:166 Resp: 3513
Ion Ratio Lower Upper
166 100
165 97.0 79.7 119.5
167 16.4 11.3 16.9

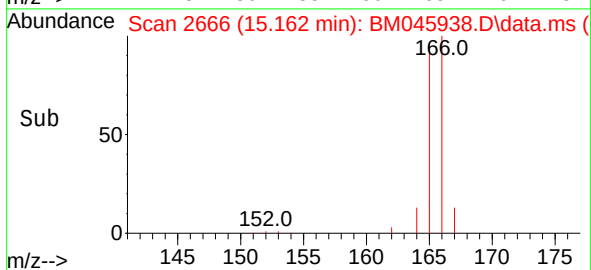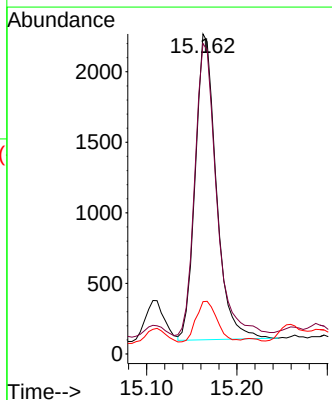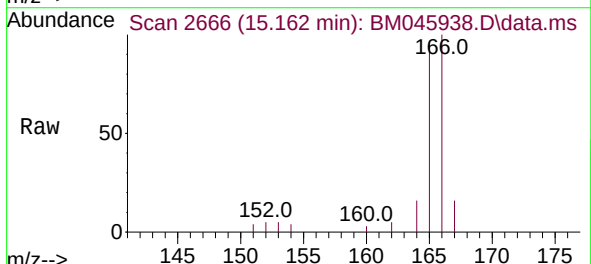







#15
Phenanthrene
Concen: 0.968 ng/ul
RT: 16.891 min Scan# 3058
Delta R.T. -0.013 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00

Instrument :
BNA_M
ClientSampleId :
A4C25DL

Tgt Ion:178 Resp: 5679
Ion Ratio Lower Upper
178 100
179 15.6 12.7 19.1
176 19.5 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

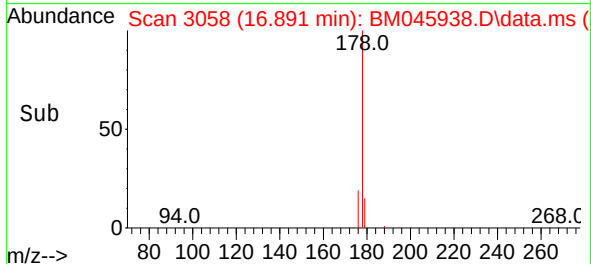

#16
Anthracene
Concen: 0.234 ng/ul
RT: 16.984 min Scan# 3080
Delta R.T. -0.013 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:178 Resp: 11722
Ion Ratio Lower Upper
178 100
179 20.5 13.1 19.7#
176 19.5 15.5 23.3

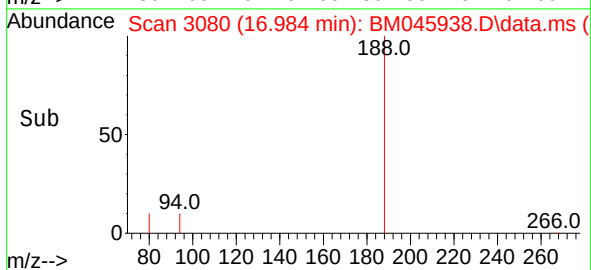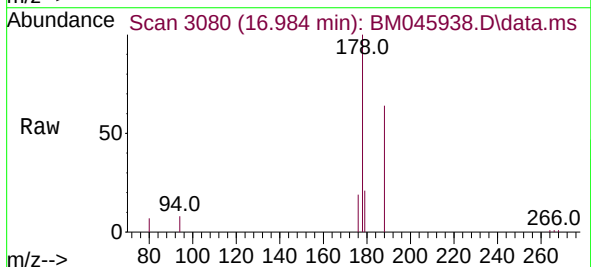



#19
Fluoranthene
Concen: 1.076 ng/ul
RT: 18.913 min Scan# 3528
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00



Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:202 Resp: 74234
Ion Ratio Lower Upper
202 100
101 10.3 9.0 13.6
100 7.9 7.0 10.6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

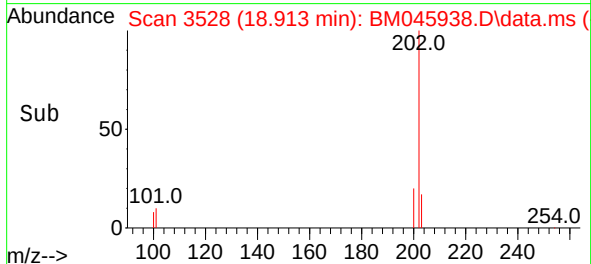




06/10/2024
Supervised By :mohammad
ahmed


06/13/2024



#20
Pyrene
Concen: 0.877 ng/ul
RT: 19.275 min Scan# 3606
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:202 Resp: 63156
Ion Ratio Lower Upper
202 100
101 11.9 10.6 16.0
100 9.8 9.1 13.7

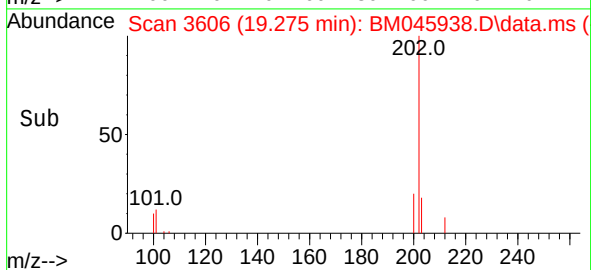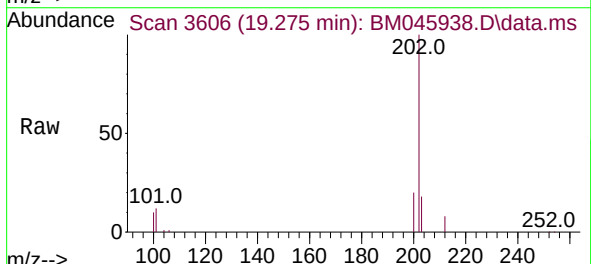



#21
Benzo(a)anthracene
Concen: 0.466 ng/ul
RT: 21.026 min Scan# 4051
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00



Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:228 Resp: 2961
Ion Ratio Lower Upper
228 100
229 21.1 15.7 23.5
226 28.7 22.0 33.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

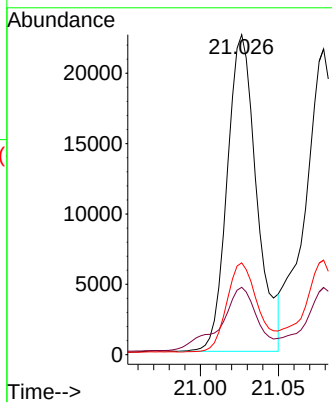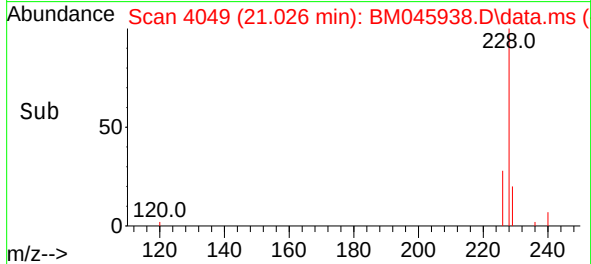




06/10/2024
Supervised By :mohammad
ahmed


06/13/2024



#22
Chrysene
Concen: 0.453 ng/ul
RT: 21.079 min Scan# 4067
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:228 Resp: 31328
Ion Ratio Lower Upper
228 100
226 30.9 24.5 36.7
229 22.0 16.2 24.2

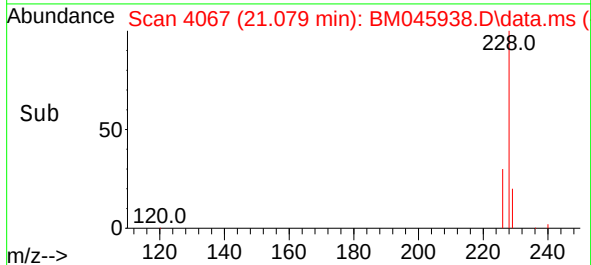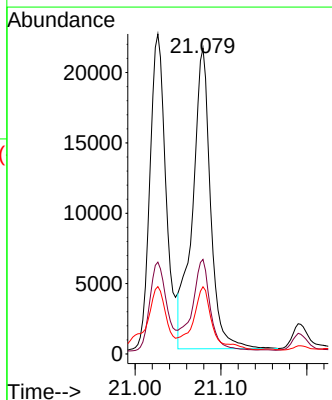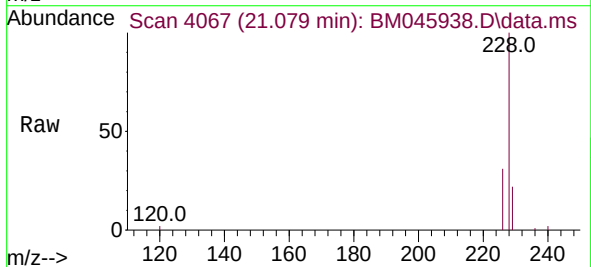



#24
Benzo(b)fluoranthene
Concen: 0.601 ng/ul m
RT: 22.528 min Scan# 4563
Delta R.T. -0.009 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00



Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:252 Resp: 3832
Ion Ratio Lower Upper
252 100
253 29.3 0.0 63.6
125 16.7 0.0 35.8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

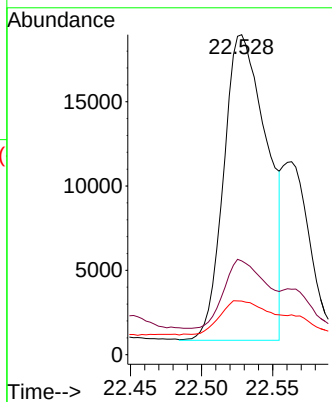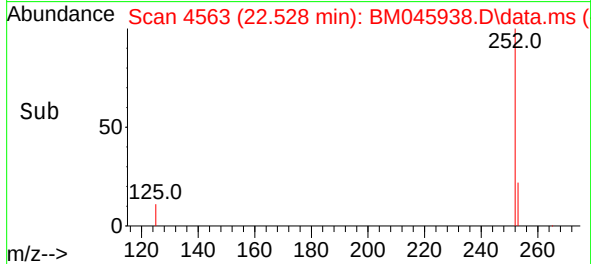




06/10/2024
Supervised By :mohammad
ahmed


06/13/2024



#25
Benzo(k)fluoranthene
Concen: 0.206 ng/ul m
RT: 22.563 min Scan# 4575
Delta R.T. -0.018 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:252 Resp: 14420
Ion Ratio Lower Upper
252 100
253 33.9 25.0 37.6
125 20.6 14.2 21.2

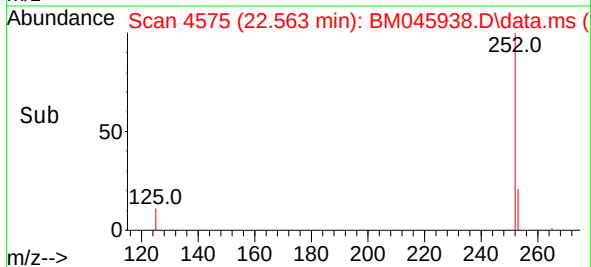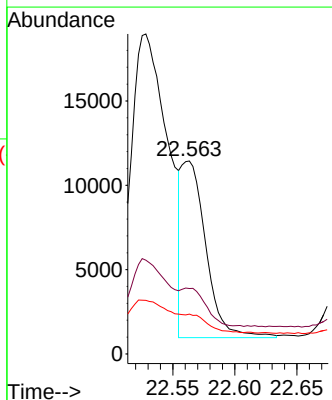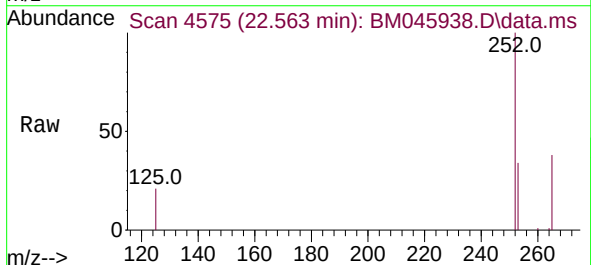



#26
Benzo(a)pyrene
Concen: 0.421 ng/ul
RT: 23.054 min Scan# 4743
Delta R.T. -0.018 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00



Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:252 Resp: 26709
Ion Ratio Lower Upper
252 100
253 30.2 28.8 43.2
125 17.3 17.3 25.9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

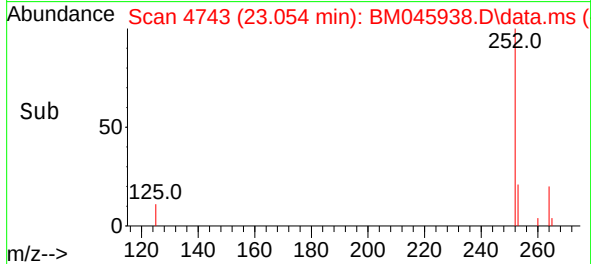




06/10/2024
Supervised By :mohammad
ahmed


06/13/2024



#27
Indeno(1,2,3-cd)pyrene
Concen: 0.242 ng/ul
RT: 25.212 min Scan# 5472
Delta R.T. -0.020 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00


Tgt Ion:276 Resp: 19797
Ion Ratio Lower Upper
276 100
138 20.2 20.7 31.1#
227 0.0 0.2 0.2#

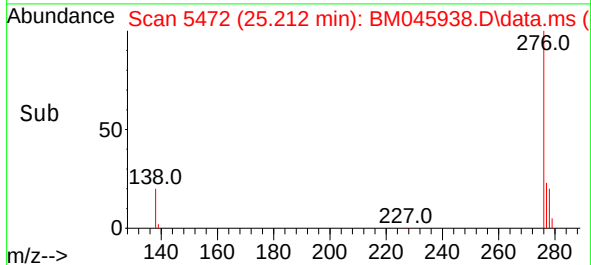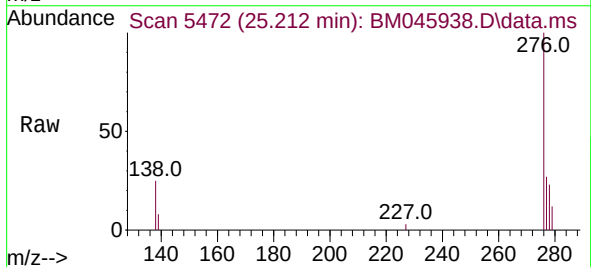



#28
Dibenzo(a,h)anthracene
Concen: 0.070 ng/ul
RT: 25.219 min Scan# 5477
Delta R.T. -0.030 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00



Instrument :
BNA_M
ClientSampleId :
A4C25DL



Tgt Ion:278 Resp: 4592
Ion Ratio Lower Upper
278 100
139 33.4 16.6 25.0
279 53.2 24.6 37.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :mohammad ahmed 06/13/2024

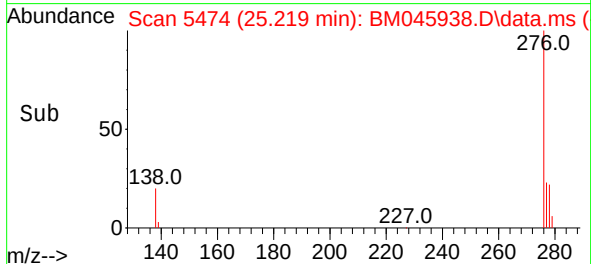

06/10/2024
Supervised By :mohammad
ahmed

06/13/2024



#29
Benzo(g,h,i)perylene
Concen: 0.276 ng/ul
RT: 25.843 min Scan# 5660
Delta R.T. -0.020 min
Lab File: BM045938.D
Acq: 09 Jun 2024 05:00

Tgt Ion:276 Resp: 19488
Ion Ratio Lower Upper
276 100
138 26.1 21.0 31.4
277 26.2 20.5 30.7

