


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060815\
 Data File : BM001595.D
 Acq On : 08 Jun 2015 20:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 17:36:38 2015

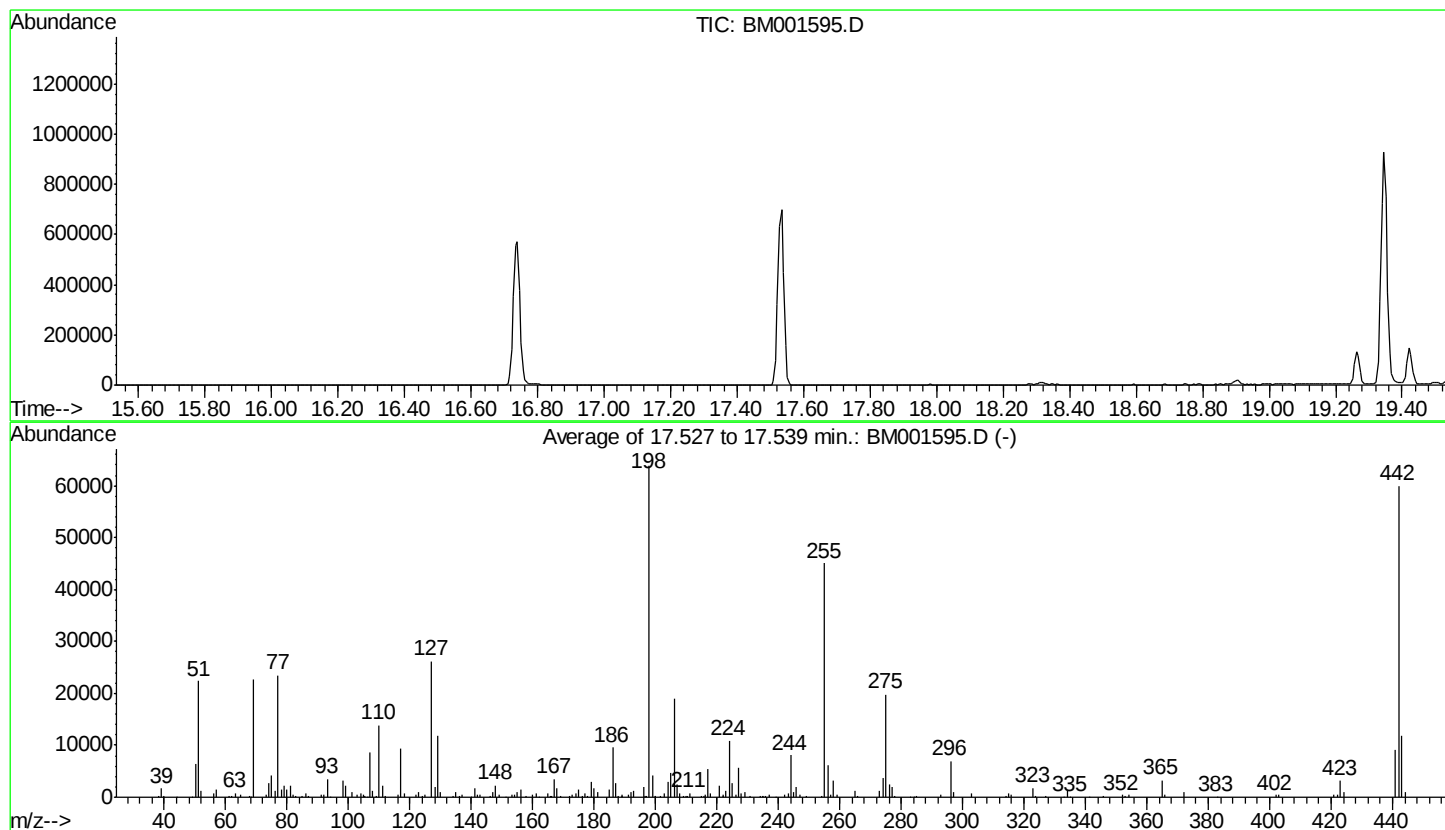

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	22391	PASS
68	69	0.00	2	1.4	312	PASS
69	198	0.00	100	35.6	22718	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	26173	PASS
197	198	0.00	2	0.5	327	PASS
198	198	100	100	100.0	63866	PASS
199	198	5	9	6.7	4282	PASS
275	198	10	60	30.9	19735	PASS
365	198	1	100	5.0	3216	PASS
441	442	0.01	24	15.1	9030	PASS
442	198	50	100	93.9	59968	PASS
443	442	15	24	19.8	11886	PASS