


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060815\
 Data File : BM001611.D
 Acq On : 09 Jun 2015 08:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 17:36:38 2015

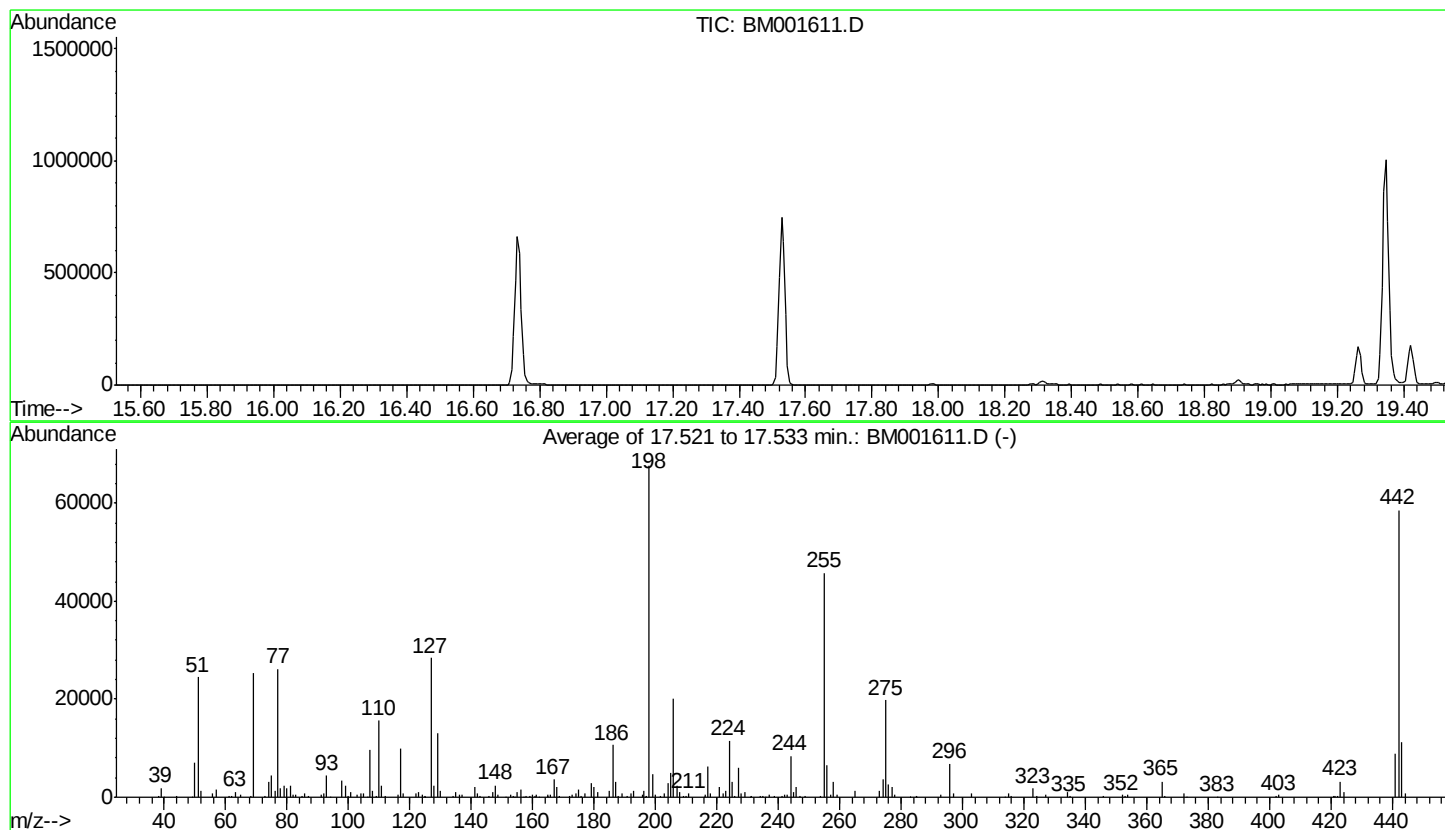

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	24448	PASS
68	69	0.00	2	1.3	323	PASS
69	198	0.00	100	37.5	25381	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	28354	PASS
197	198	0.00	2	0.2	160	PASS
198	198	100	100	100.0	67634	PASS
199	198	5	9	6.9	4673	PASS
275	198	10	60	29.3	19790	PASS
365	198	1	100	4.6	3140	PASS
441	442	0.01	24	15.2	8894	PASS
442	198	50	100	86.5	58528	PASS
443	442	15	24	19.2	11221	PASS