

Data File : BM010443.D
Acq On : 07 Jun 2017 22:46
Operator : SJ/MA
Sample : I3490-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0AC9

Quant Time: Jun 08 07:10:44 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	720	0.40	ng/ul	0.00
2) Naphthalene-d8	10.72	136	2290	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	1489	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.30
16) Chrysene-d12	21.45	240	2509	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	203787	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	1207	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	3278	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.68	202	725	0.07	ng/ul#	Qvalue 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM010443.D

Acq On : 07 Jun 2017 22:46

Operator : SJ/MA

Sample : I3490-02

Misc :

ALS Vial : 5 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

B0AC9


Quant Time: Jun 08 07:10:44 2017




Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 08 07:10:23 2017

Response via : Initial Calibration

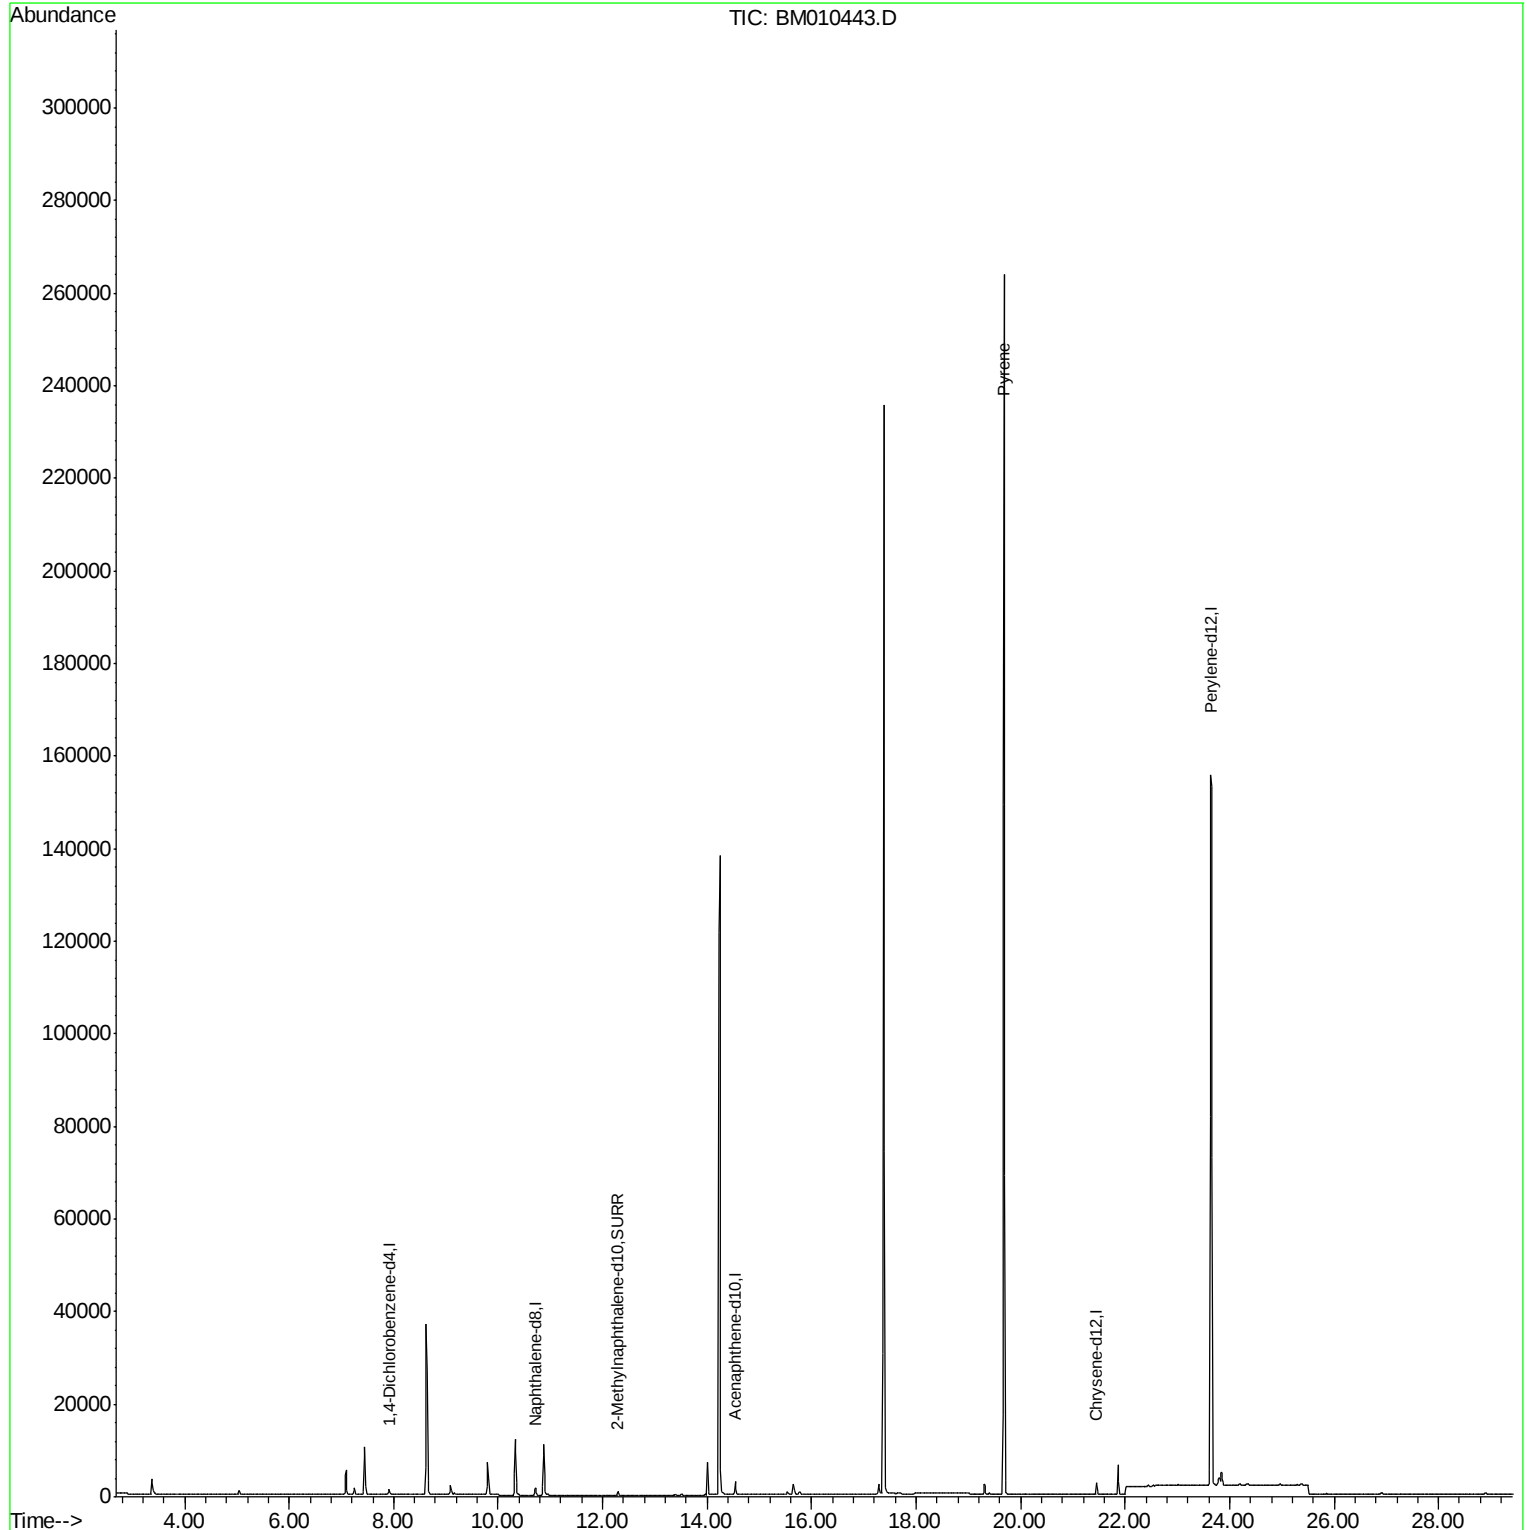

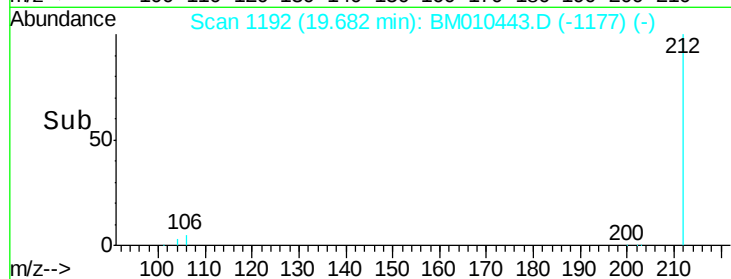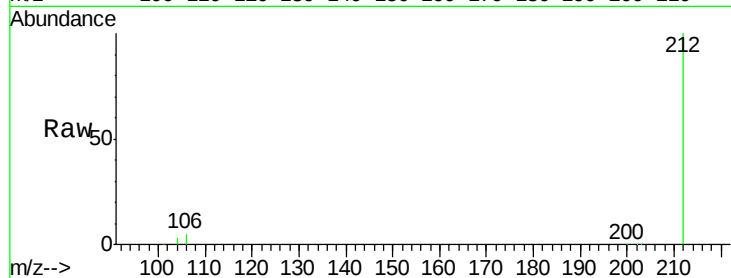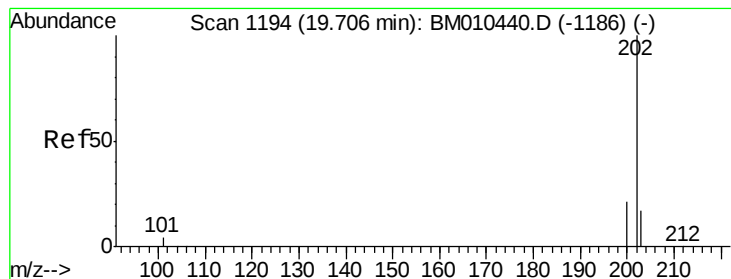

#17

Pyrene

Concen: 0.07 ng/ul

RT: 19.68 min Scan# 1192

Delta R.T. -0.02 min

Lab File: BM010443.D

Acq: 07 Jun 2017 22:46

Instrument :

BNA_M

ClientSampleId :

B0AC9

Tgt Ion: 202 Resp: 725

Ion Ratio Lower Upper

202 100

200 16.4 18.2 27.4#

203 199.0 15.6 23.4#

