

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (Qedit)




Data File : BM010441.D
Acq On : 07 Jun 2017 21:35
Operator : SJ/MA
Sample : PB99539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 08 07:10:34 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK39

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:53 AM

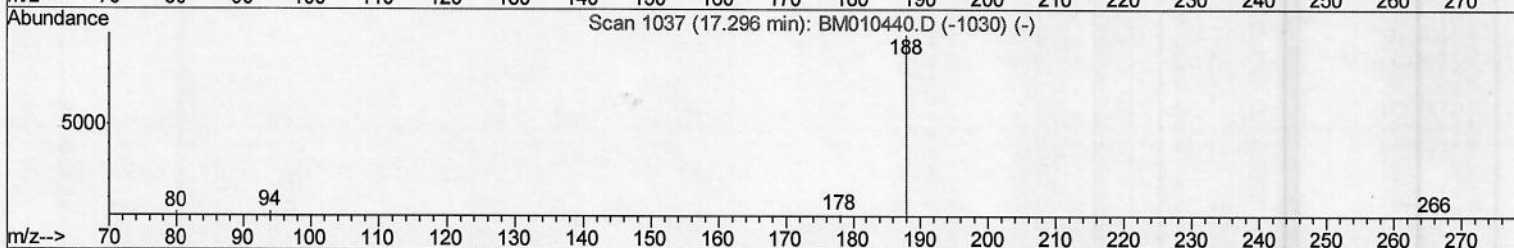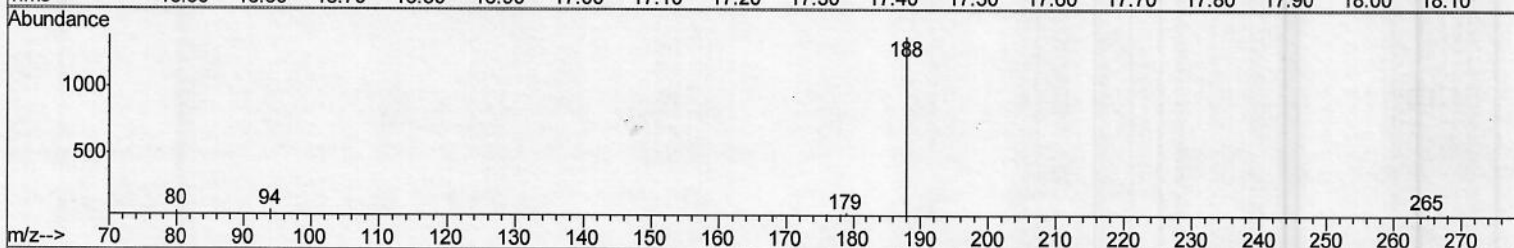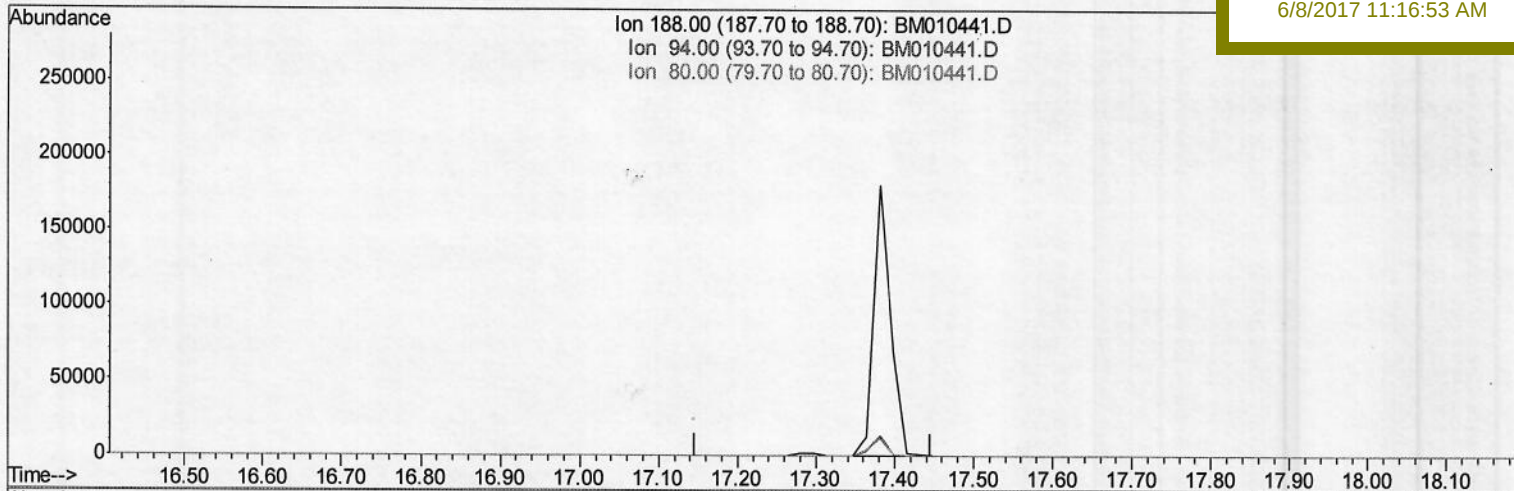

TIC: BM010441.D

(10) Phenanthrene-d10 (I)
17.296min (-17.296) 0.00ng/ul
response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (Qedit)




Data File : BM010441.D
Acq On : 07 Jun 2017 21:35
Operator : SJ/MA
Sample : PB99539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 08 07:10:34 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK39

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:53 AM

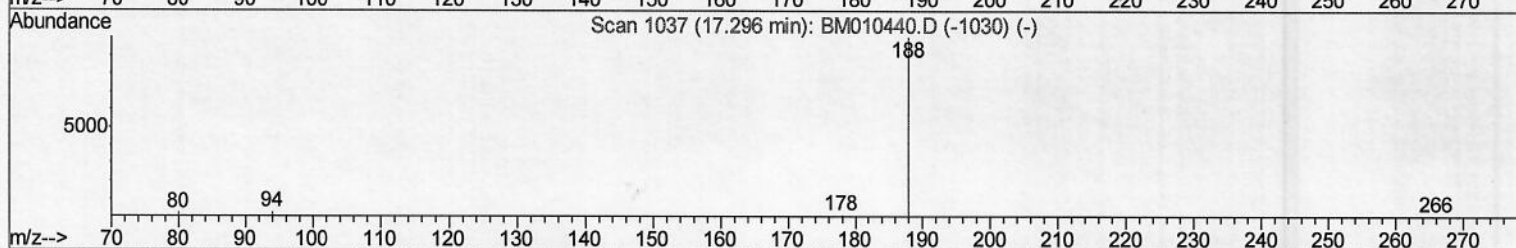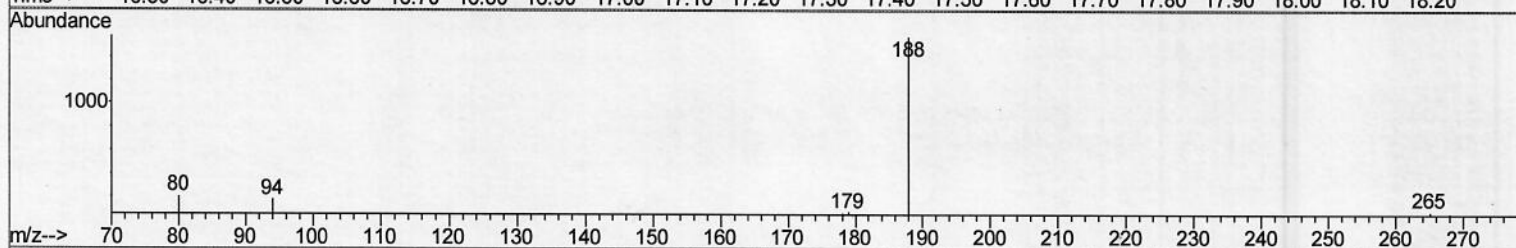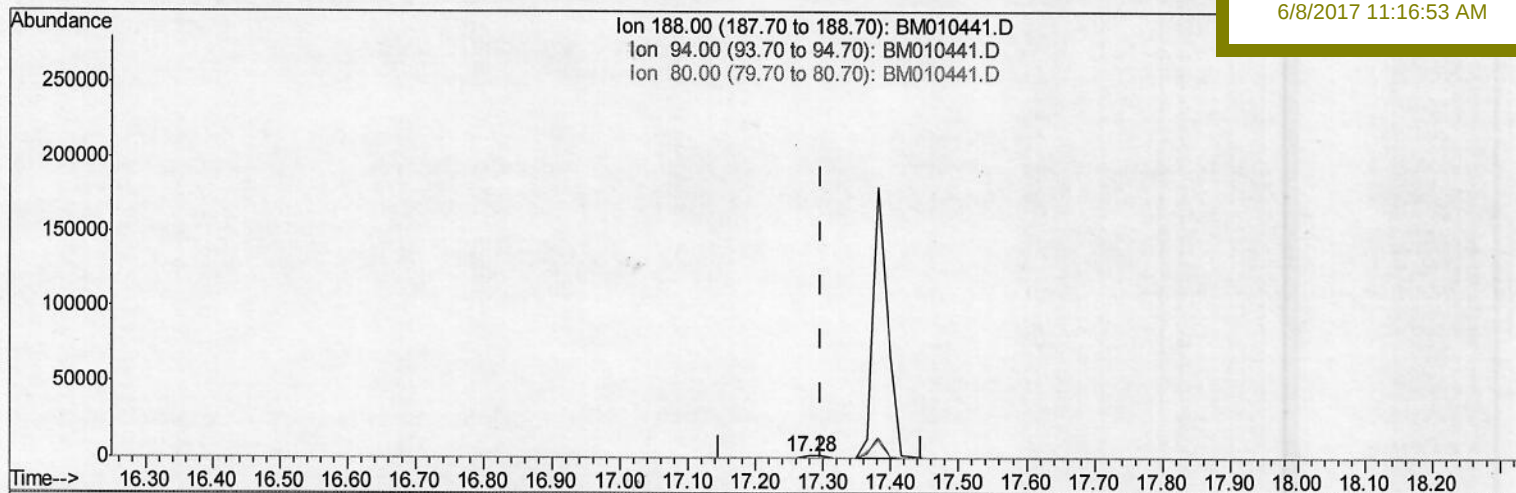

TIC: BM010441.D

(10) Phenanthrene-d10 (I)

17.279min (-0.017) 0.40ng/ul m

response 2903

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.21
80.00	11.80	12.98
0.00	0.00	0.00

5.7
0.6/10/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (Qedit)




Data File : BM010441.D
Acq On : 07 Jun 2017 21:35
Operator : SJ/MA
Sample : PB99539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 08 07:15:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK39

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:53 AM

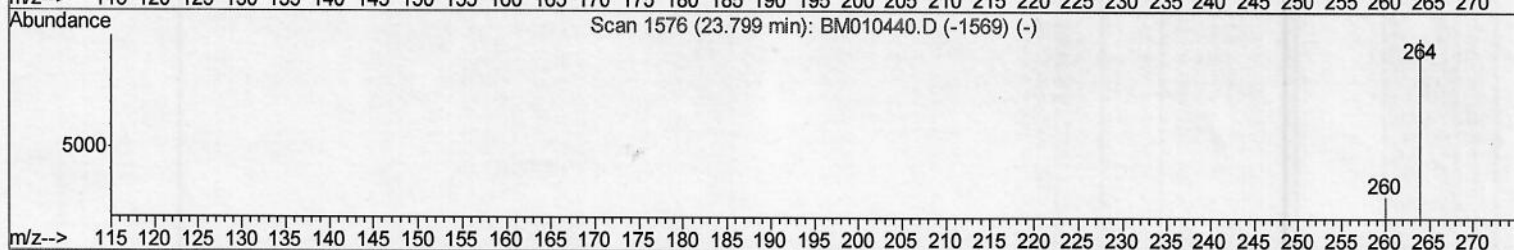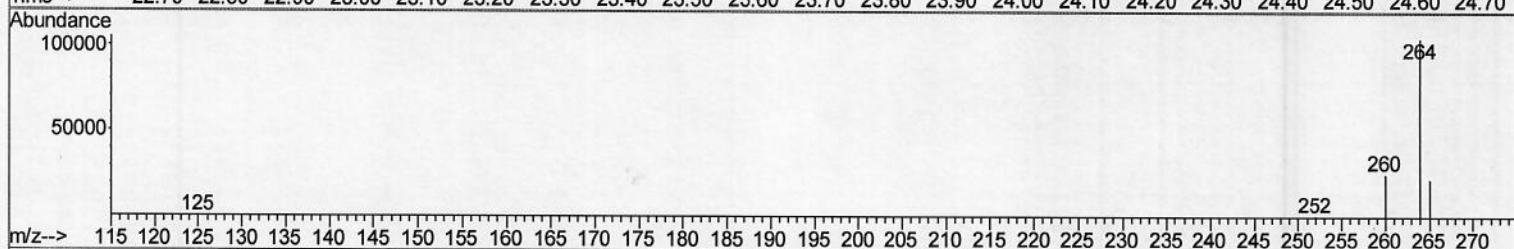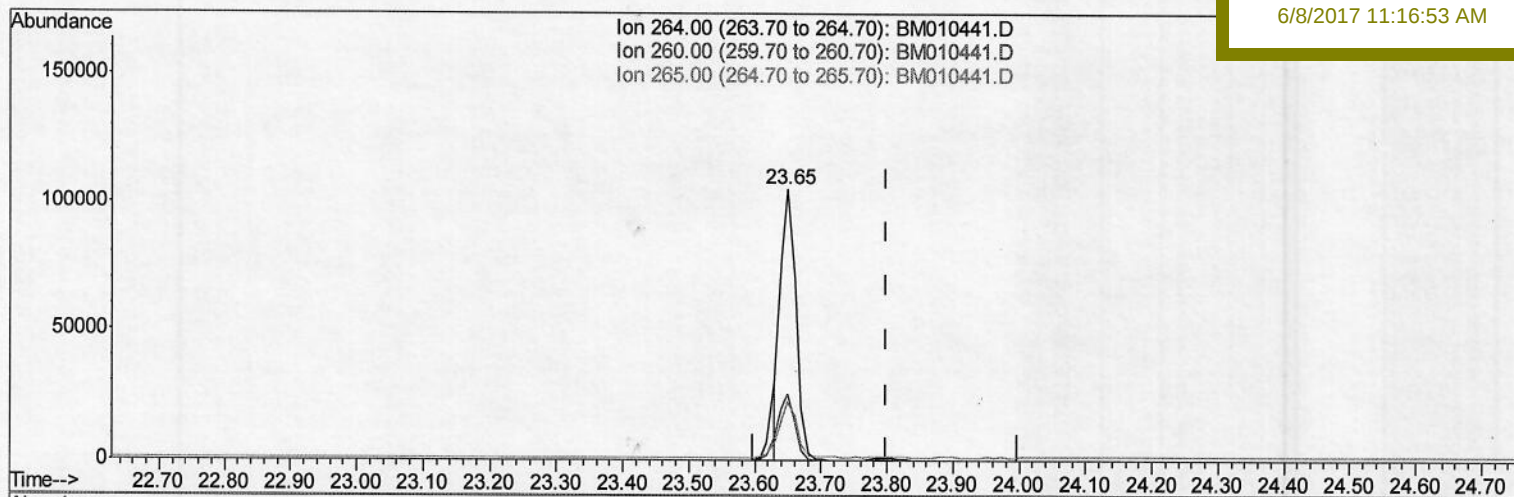

TIC: BM010441.D

(20) Perylene-d12 (I)

23.649min (-0.149) 0.40ng/ul

response 172306

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.08#
265.00	103.50	21.34#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (Qedit)




Data File : BM010441.D
Acq On : 07 Jun 2017 21:35
Operator : SJ/MA
Sample : PB99539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 08 07:15:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK39

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:53 AM

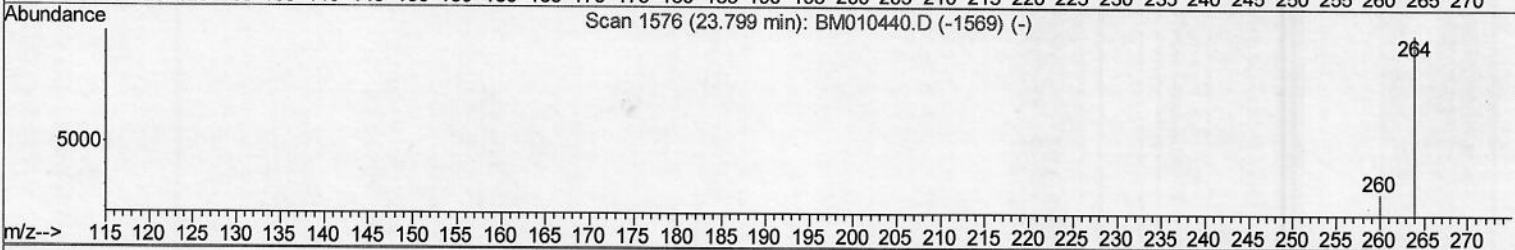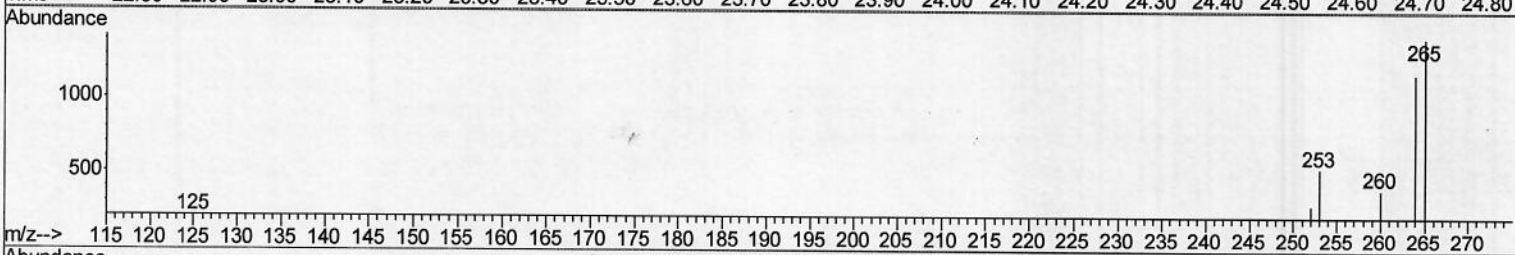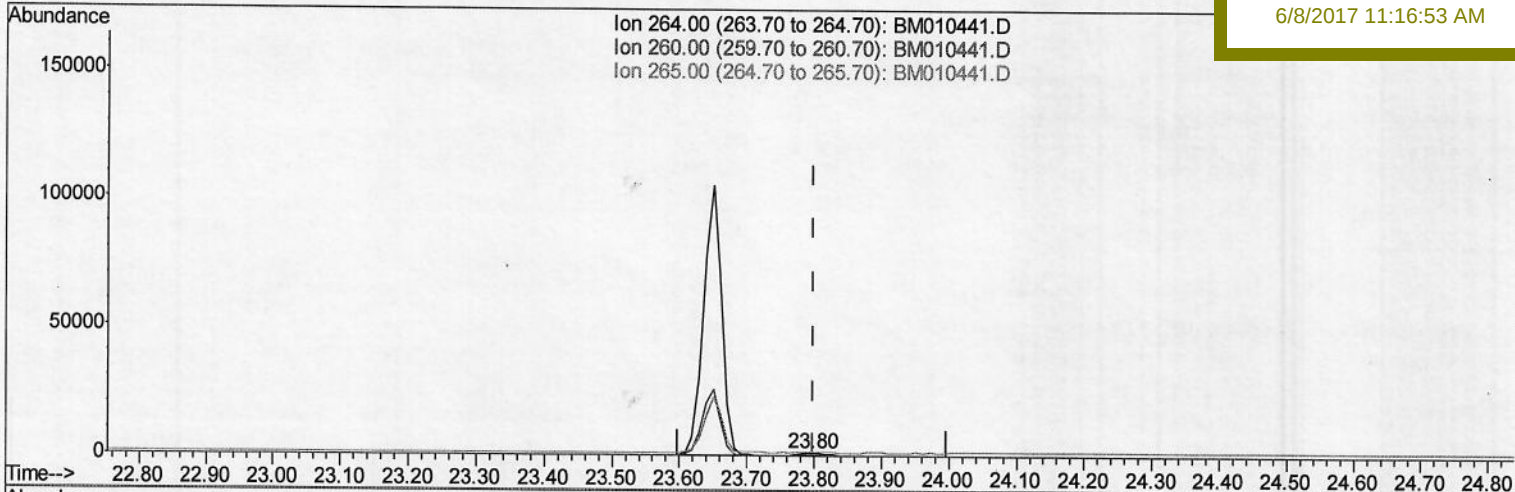

TIC: BM010441.D

(20) Perylene-d12 (I)

23.795min (-0.003) 0.40ng/ul m

response 2364

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	33.14
265.00	103.50	120.73
0.00	0.00	0.00

> 9.9
06/10/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (QT Reviewed)

Data File : BM010441.D
Acq On : 07 Jun 2017 21:35
Operator : SJ/MA
Sample : PB99539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 08 07:16:21 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK39

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:53 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	738	0.40	ng/ul	0.00
2) Naphthalene-d8	10.72	136	2276	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	1509	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	2903m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.46	240	2277	0.40	ng/ul	0.00
20) Perylene-d12	23.80	264	2364m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	1200	0.36	ng/ul	0.01
14) Fluoranthene-d10	19.31	212	2578	0.33	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (QT Reviewed)

Data File : BM010441.D
Acq On : 07 Jun 2017 21:35
Operator : SJ/MA
Sample : PB99539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 08 07:16:21 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK39

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:53 AM

