

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\

Quantitation Report (Qedit)

Data File : BM010442.D

Acq On : 07 Jun 2017 22:10

Operator : SJ/MA

Sample : I3490-01

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 08 07:10:39 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 08 07:10:23 2017

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




B0AC8

Manual Integrations

APPROVED

mohammad

6/8/2017 11:16:56 AM

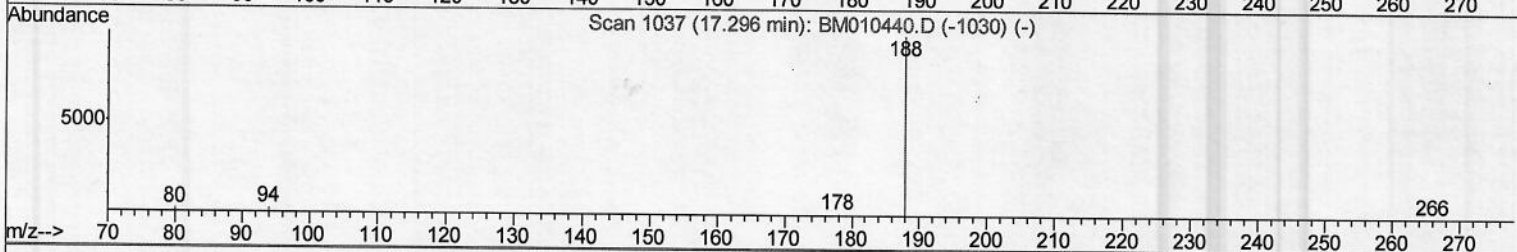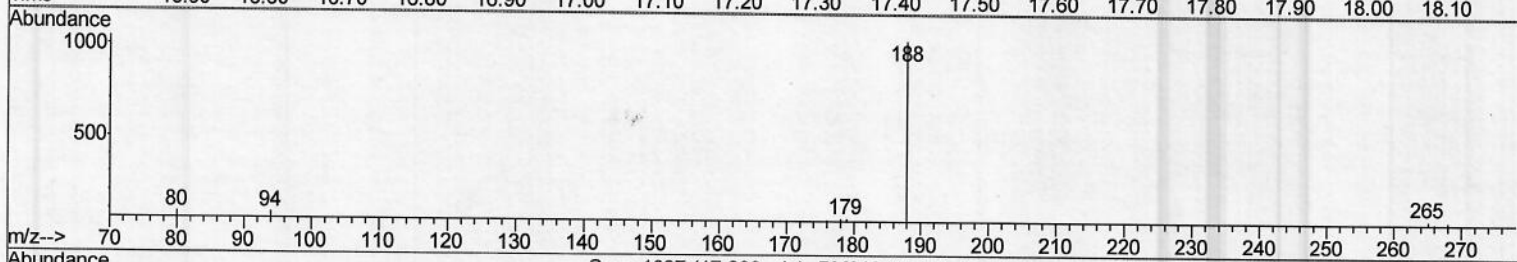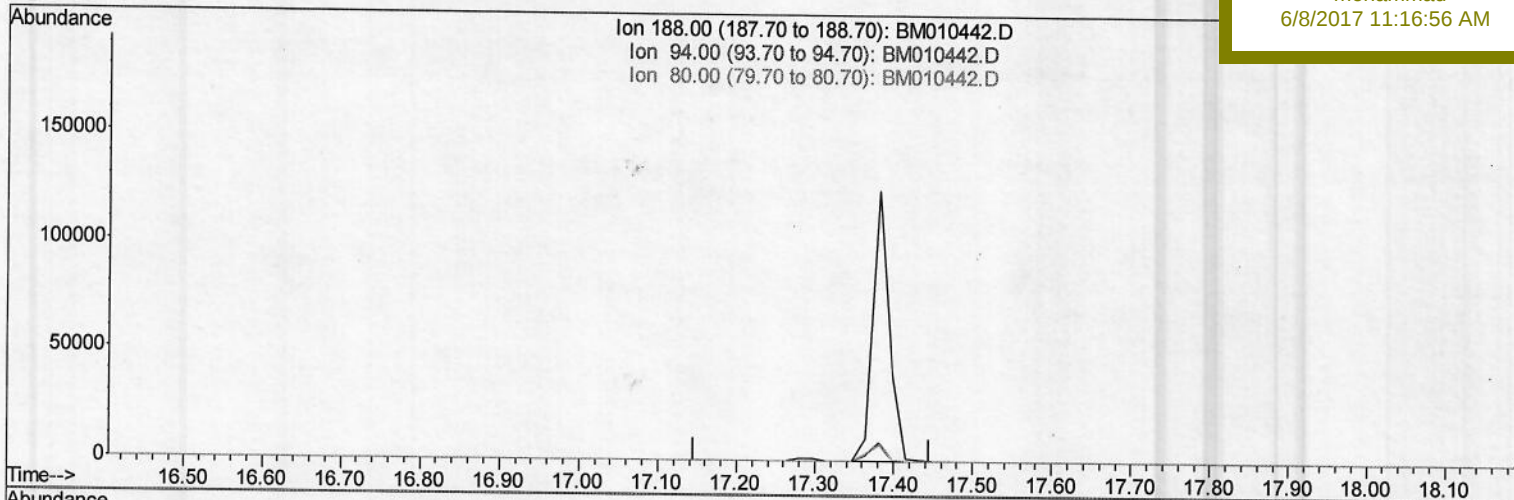

TIC: BM010442.D

(10) Phenanthrene-d10 (I)

17.296min (-17.296) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (Qedit)

Data File : BM010442.D

Acq On : 07 Jun 2017 22:10

Operator : SJ/MA

Sample : I3490-01

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 08 07:10:39 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 08 07:10:23 2017

Response via : Initial Calibration

Instrument :




BNA_M

ClientSampleId :

B0AC8

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:56 AM

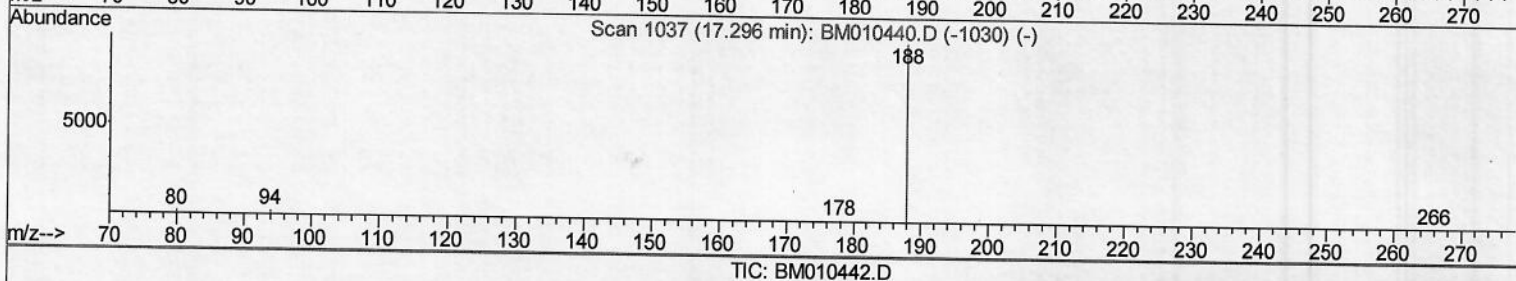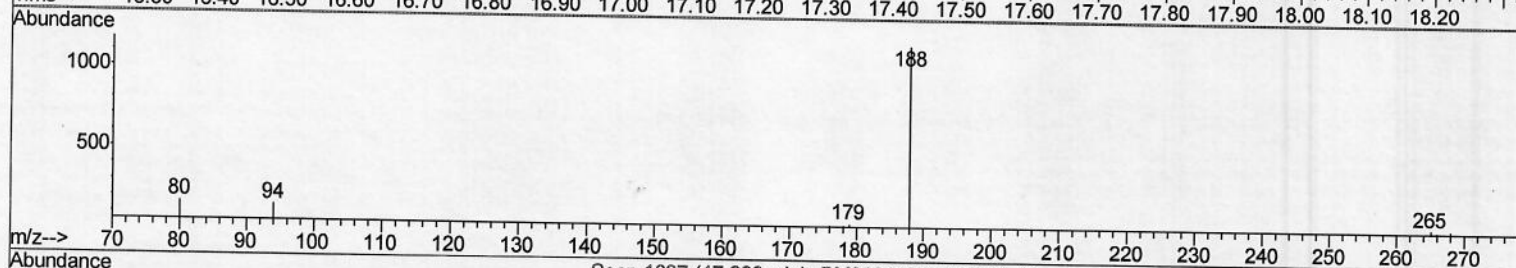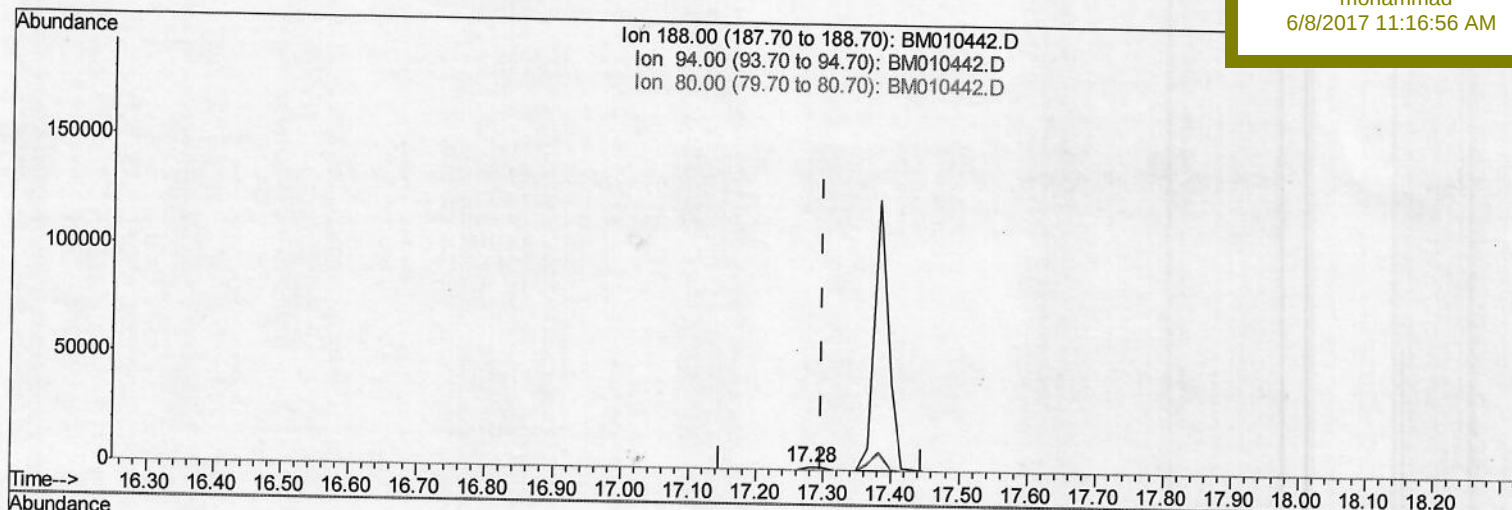

(10) Phenanthrene-d10 (I)

17.279min (-0.017) 0.40ng/ul m

response 2114

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.84
80.00	11.80	14.37#
0.00	0.00	0.00

7 S.J
06/10/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\

Quantitation Report (Qedit)

Data File : BM010442.D

Acq On : 07 Jun 2017 22:10

Operator : SJ/MA

Sample : I3490-01

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 08 07:18:09 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 08 07:10:23 2017

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




B0AC8

Manual Integrations

APPROVED

mohammad

6/8/2017 11:16:56 AM

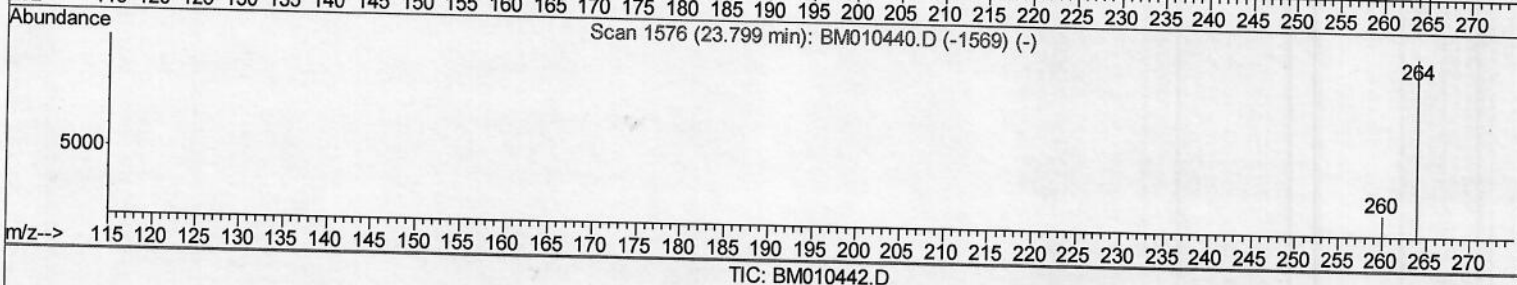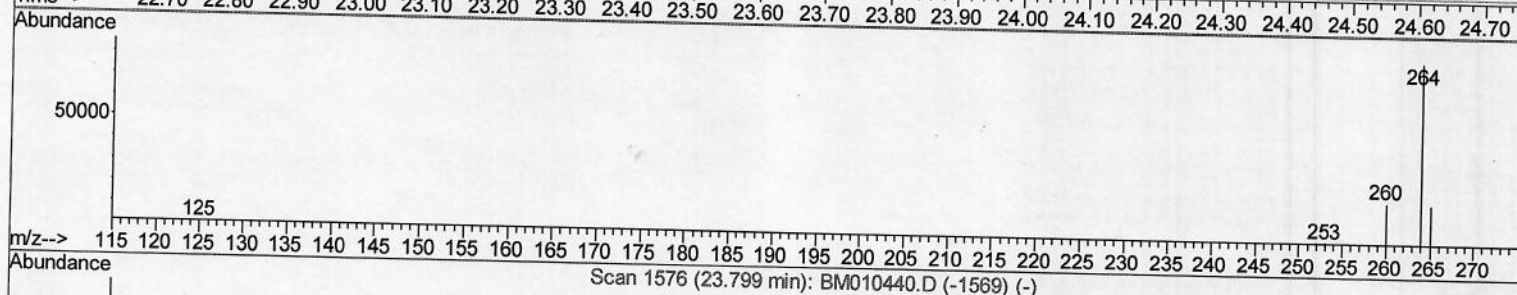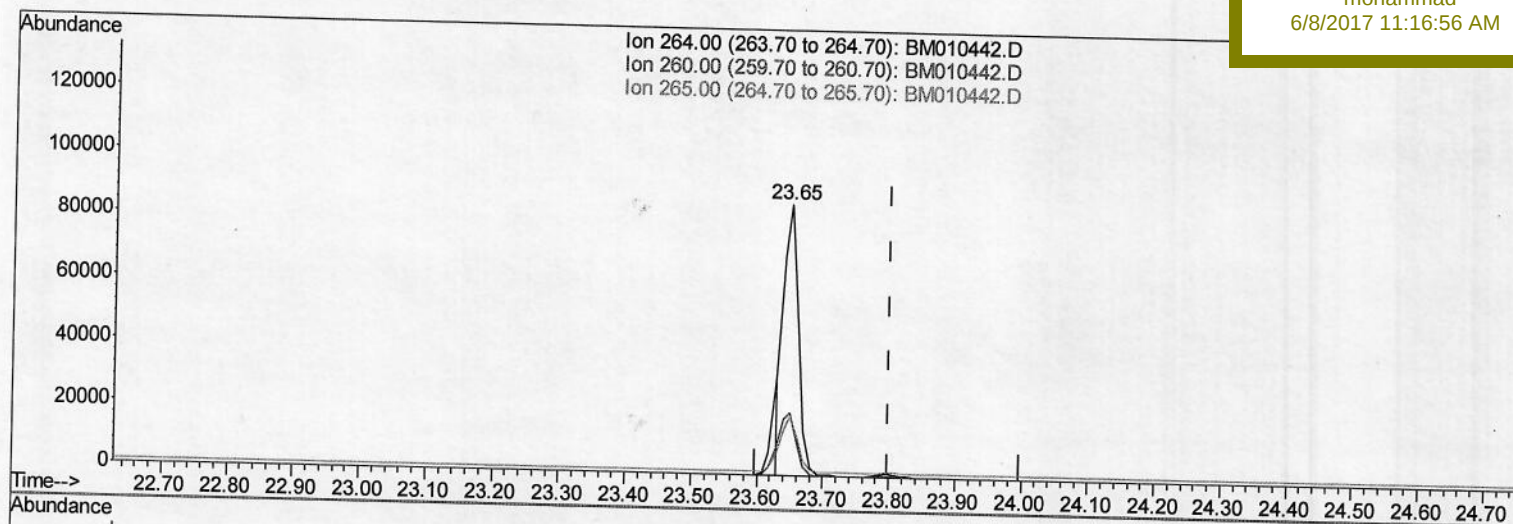

(20) Perylene-d12 (I)

23.649min (-0.150) 0.40ng/ul

response 137372

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.06#
265.00	103.50	21.94#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (Qedit)




Data File : BM010442.D
Acq On : 07 Jun 2017 22:10
Operator : SJ/MA
Sample : I3490-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 08 07:18:09 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
B0AC8

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:56 AM

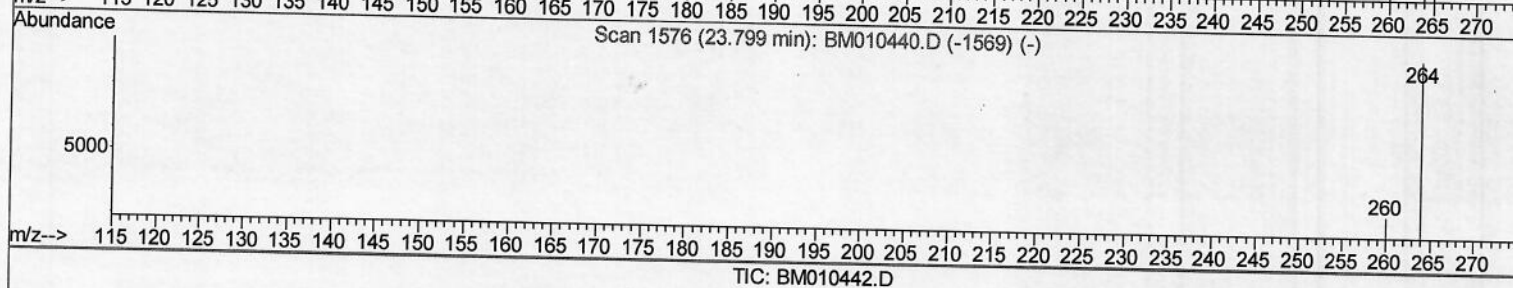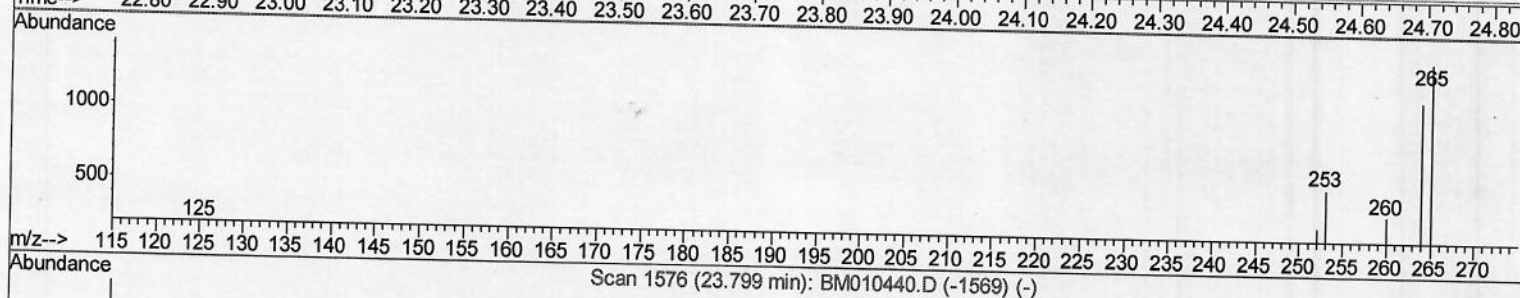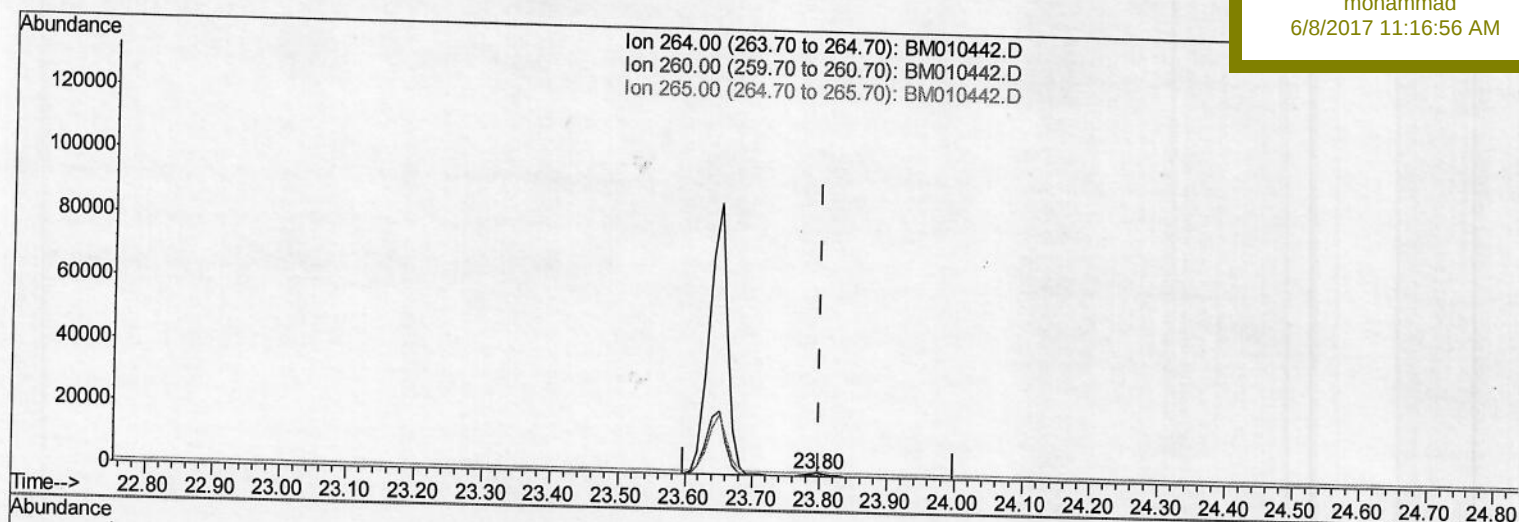

(20) Perylene-d12 (I)

23.795min (-0.004) 0.40ng/ul m

response 1983

Ion Exp% Act%

264.00 100 100

260.00 30.10 32.93

265.00 103.50 123.02

0.00 0.00 0.00

> 5.9
06/10/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (QT Reviewed)

Data File : BM010442.D
Acq On : 07 Jun 2017 22:10
Operator : SJ/MA
Sample : I3490-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0AC8

Quant Time: Jun 08 07:19:08 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:56 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	676	0.40	ng/ul	0.00
2) Naphthalene-d8	10.72	136	1949	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	1177	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	2114m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.46	240	1892	0.40	ng/ul	0.00
20) Perylene-d12	23.80	264	1983m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	1065	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	1839	0.33	ng/ul	0.00

Target Compounds

----- Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

9 5.9
06/10/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060817\
Quantitation Report (QT Reviewed)

Data File : BM010442.D
Acq On : 07 Jun 2017 22:10
Operator : SJ/MA
Sample : I3490-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 08 07:19:08 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 07:10:23 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
B0AC8

Manual Integrations
APPROVED

mohammad
6/8/2017 11:16:56 AM

