
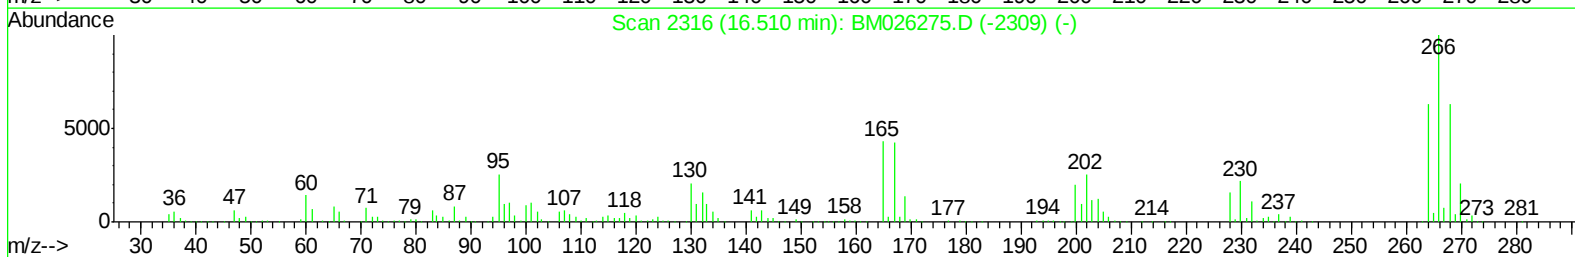
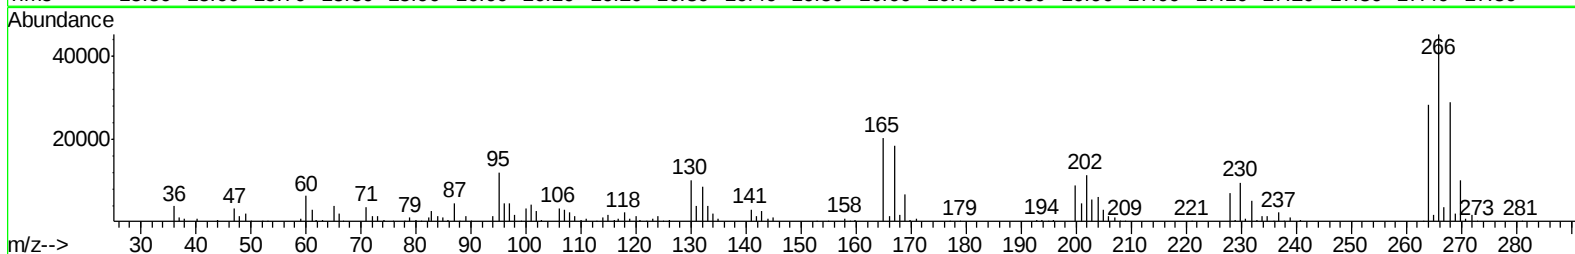


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060820\
 Data File : BM026283.D
 Acq On : 08 Jun 2020 12:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 03:36:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 08 15:00:18 2020
 Response via : Initial Calibration

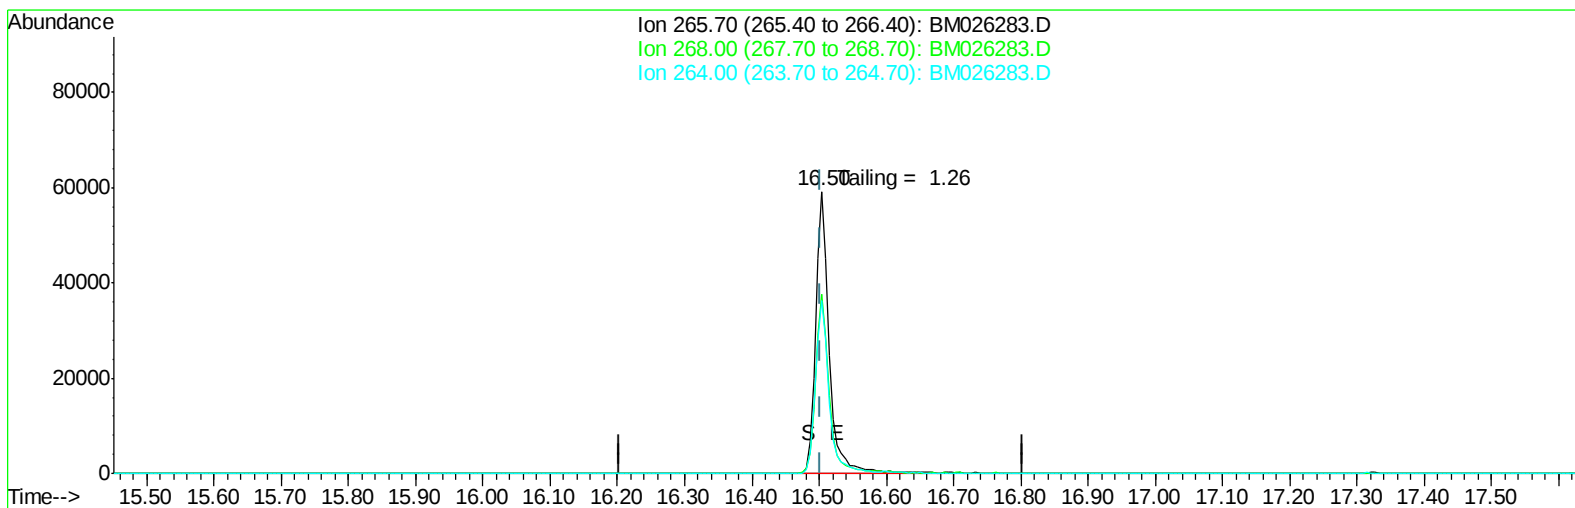

TIC: BM026283.D

(70) Pentachlorophenol (C)




16.504min (+0.000) 0.00ng

response 83930

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	63.64
264.00	62.80	61.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060820\
 Data File : BM026283.D
 Acq On : 08 Jun 2020 12:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 03:36:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 08 15:00:18 2020
 Response via : Initial Calibration

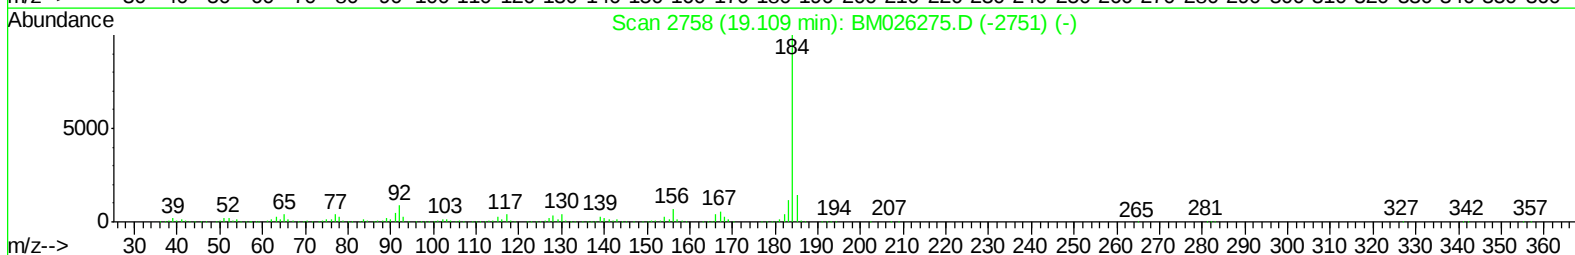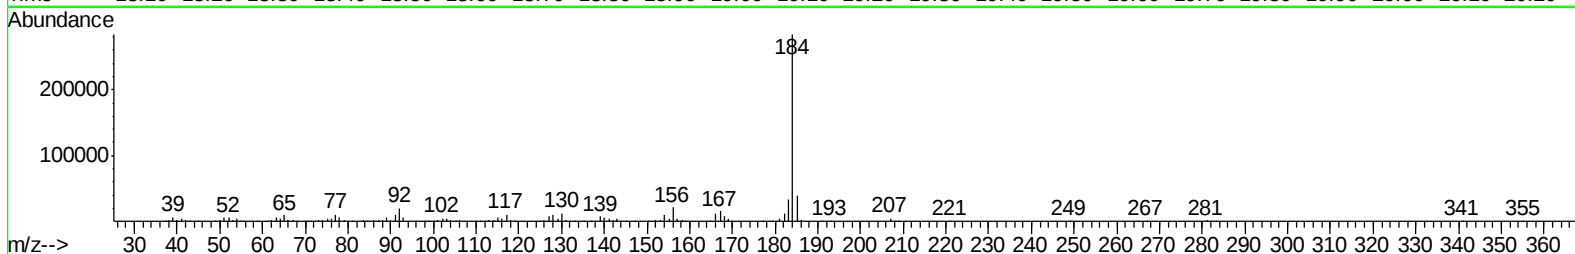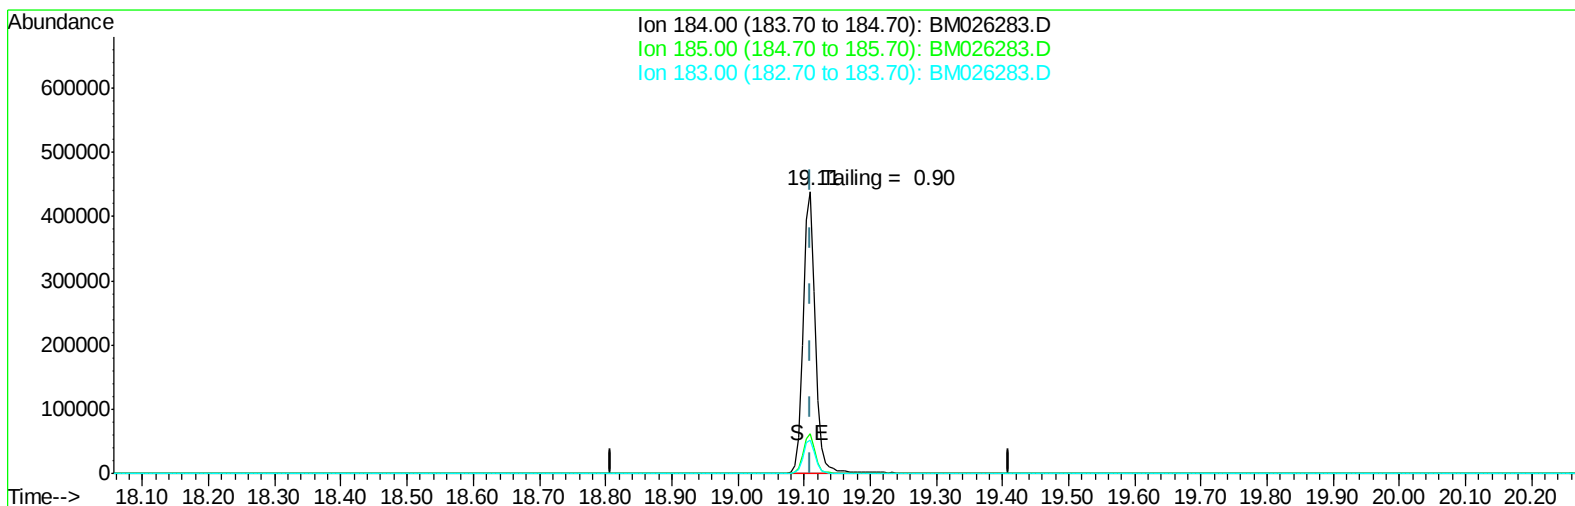

TIC: BM026283.D

(77) Benzidine

19.109min (+0.000) 0.00ng

response 567771

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	13.94
183.00	11.60	11.74
0.00	0.00	0.00