


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060820\
 Data File : BM026283.D
 Acq On : 08 Jun 2020 12:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 15:00:18 2020

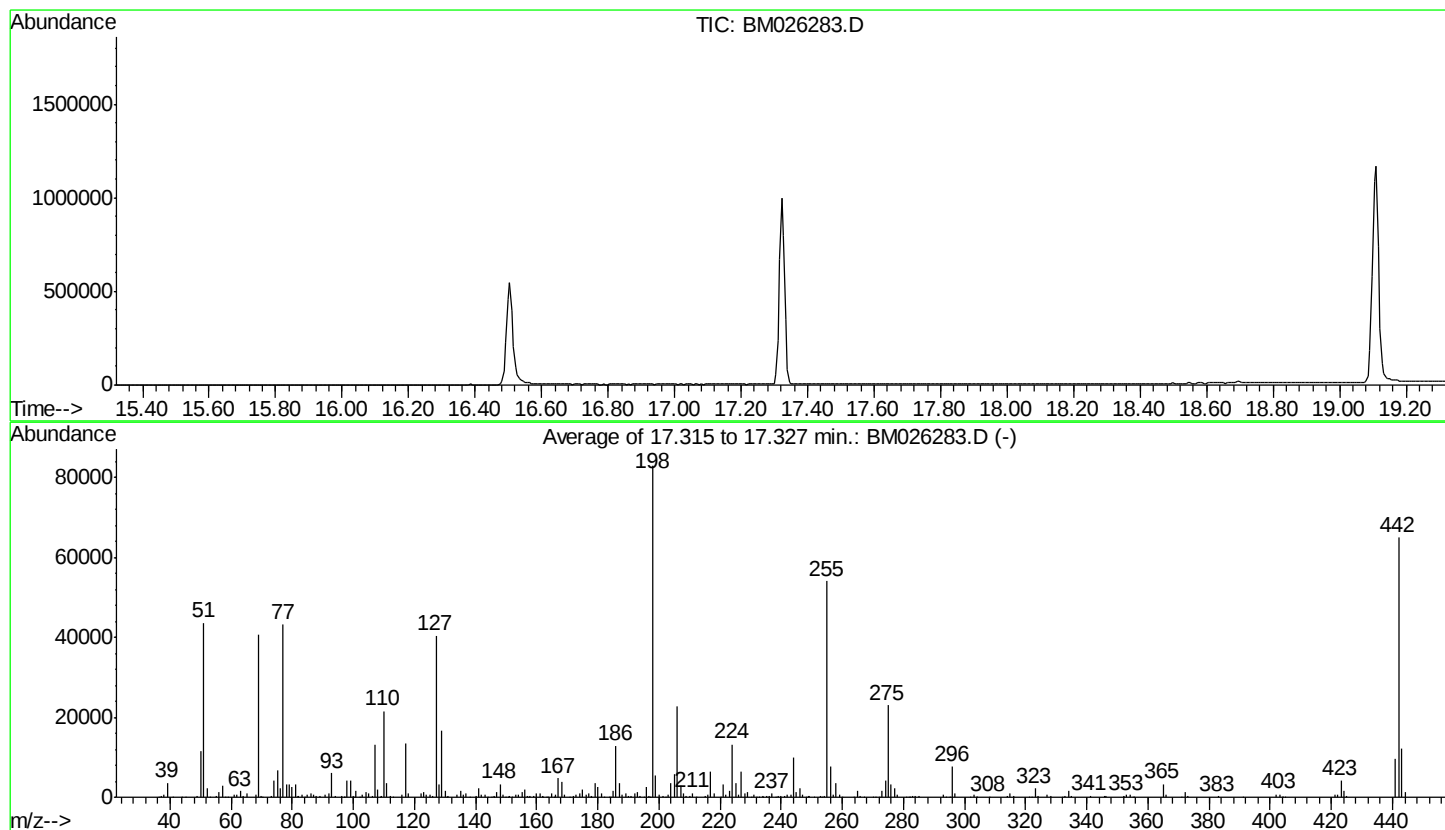

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	43605	PASS
68	69	0.00	2	1.9	791	PASS
69	198	0.00	100	48.9	40592	PASS
70	69	0.00	2	0.5	190	PASS
127	198	10	80	48.8	40456	PASS
197	198	0.00	2	0.5	397	PASS
198	198	100	100	100.0	82960	PASS
199	198	5	9	6.7	5559	PASS
275	198	10	60	27.6	22936	PASS
365	198	1	100	4.0	3296	PASS
441	198	0.01	100	11.4	9477	PASS
442	198	50	100	78.2	64866	PASS
443	442	15	24	18.6	12092	PASS