
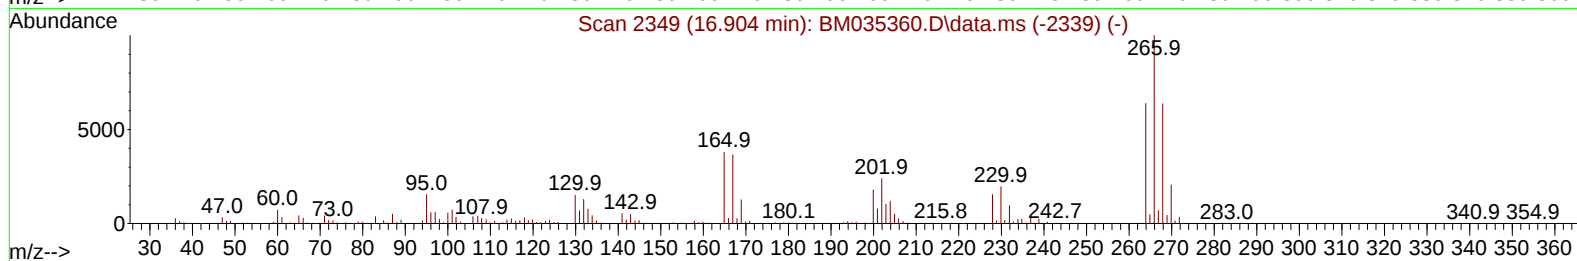
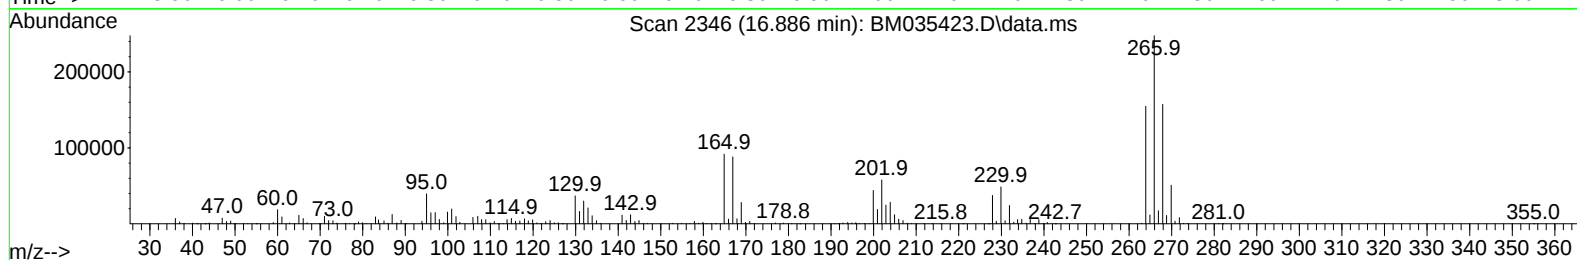


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035423.D
Acq On : 08 Jun 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 04:32:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 14:28:07 2022
Response via : Initial Calibration

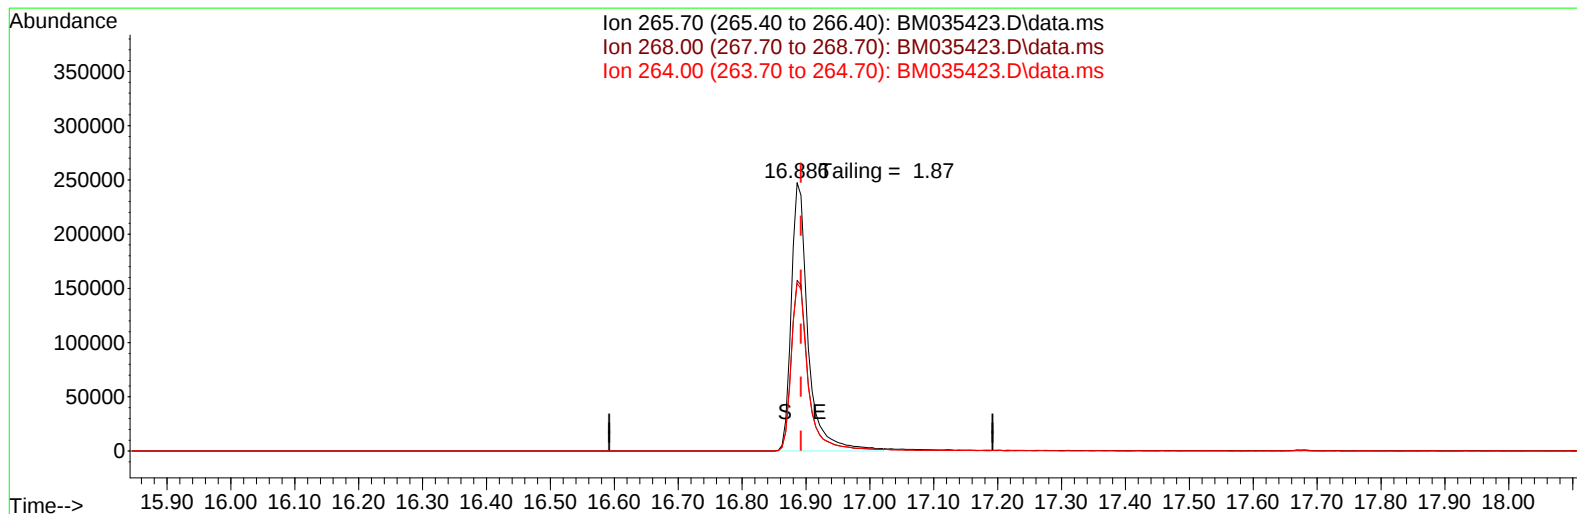

TIC: BM035423.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.006) 0.00 ng

response 460318

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.54
264.00	63.30	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035423.D
Acq On : 08 Jun 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 04:32:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 14:28:07 2022
Response via : Initial Calibration

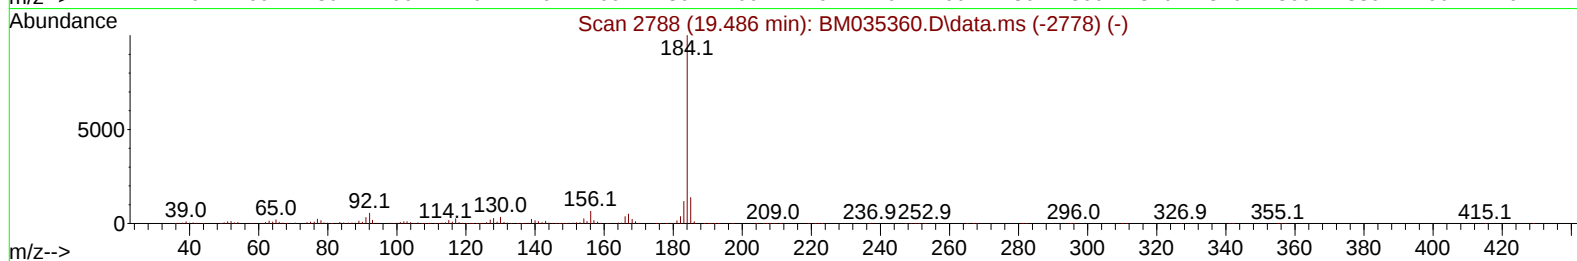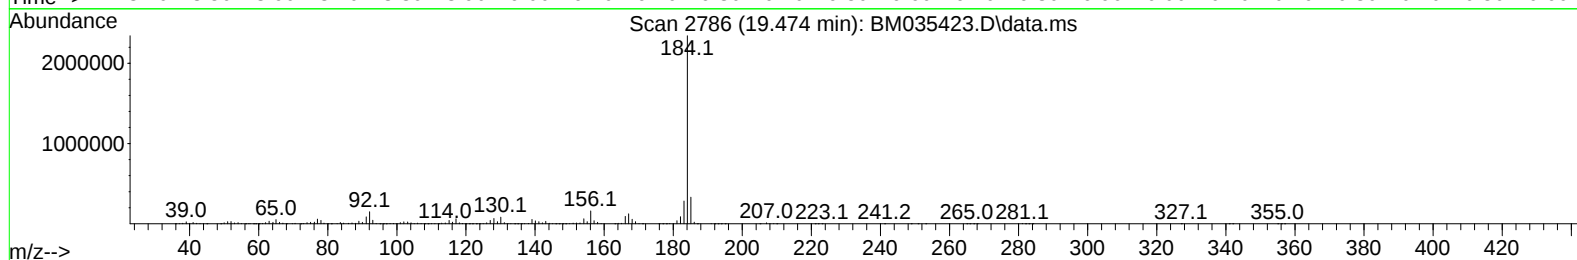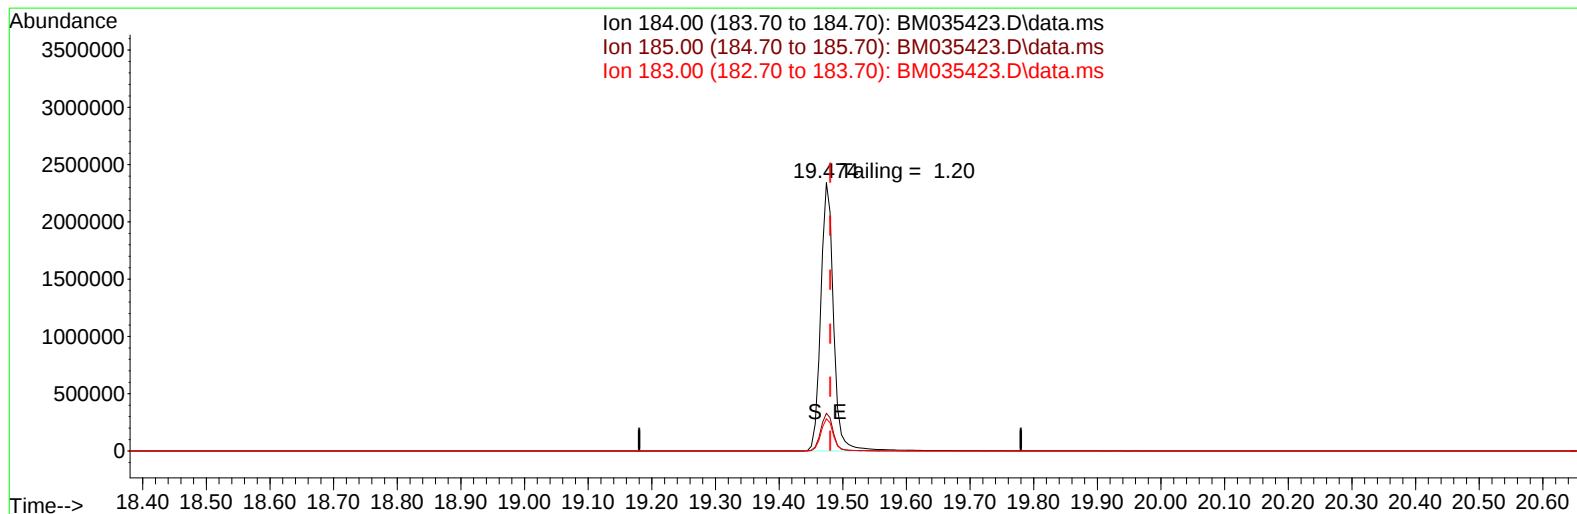

TIC: BM035423.D\data.ms

(77) Benzidine**19.474min (-0.006) 212929.25 ng****response 3278784**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.90	12.07
0.00	0.00	0.00