

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
 Data File : BM035435.D
 Acq On : 08 Jun 2022 18:24
 Operator : CG/JU
 Sample : N3189-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 20220400-C-2-TCLP

Quant Time: Jun 09 00:51:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 14:28:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.839	152	186446	20.000	ng	0.00
21) Naphthalene-d8	10.639	136	680893	20.000	ng	# 0.00
39) Acenaphthene-d10	14.480	164	437390	20.000	ng	0.00
64) Phenanthrene-d10	17.227	188	905447	20.000	ng	# 0.00
76) Chrysene-d12	21.415	240	825593	20.000	ng	# 0.00
86) Perylene-d12	23.768	264	897729	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1379066	155.426	ng	0.00
7) Phenol-d6	7.028	99	1570826	129.607	ng	0.00
23) Nitrobenzene-d5	9.004	82	1067887	99.585	ng	0.00
42) 2,4,6-Tribromophenol	15.974	330	951653	135.606	ng	0.00
45) 2-Fluorobiphenyl	13.104	172	3147837	103.366	ng	0.00
79) Terphenyl-d14	19.856	244	4621767	111.530	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035435.D
Acq On : 08 Jun 2022 18:24
Operator : CG/JU
Sample : N3189-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20220400-C-2-TCLP

Quant Time: Jun 09 00:51:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 14:28:07 2022
Response via : Initial Calibration




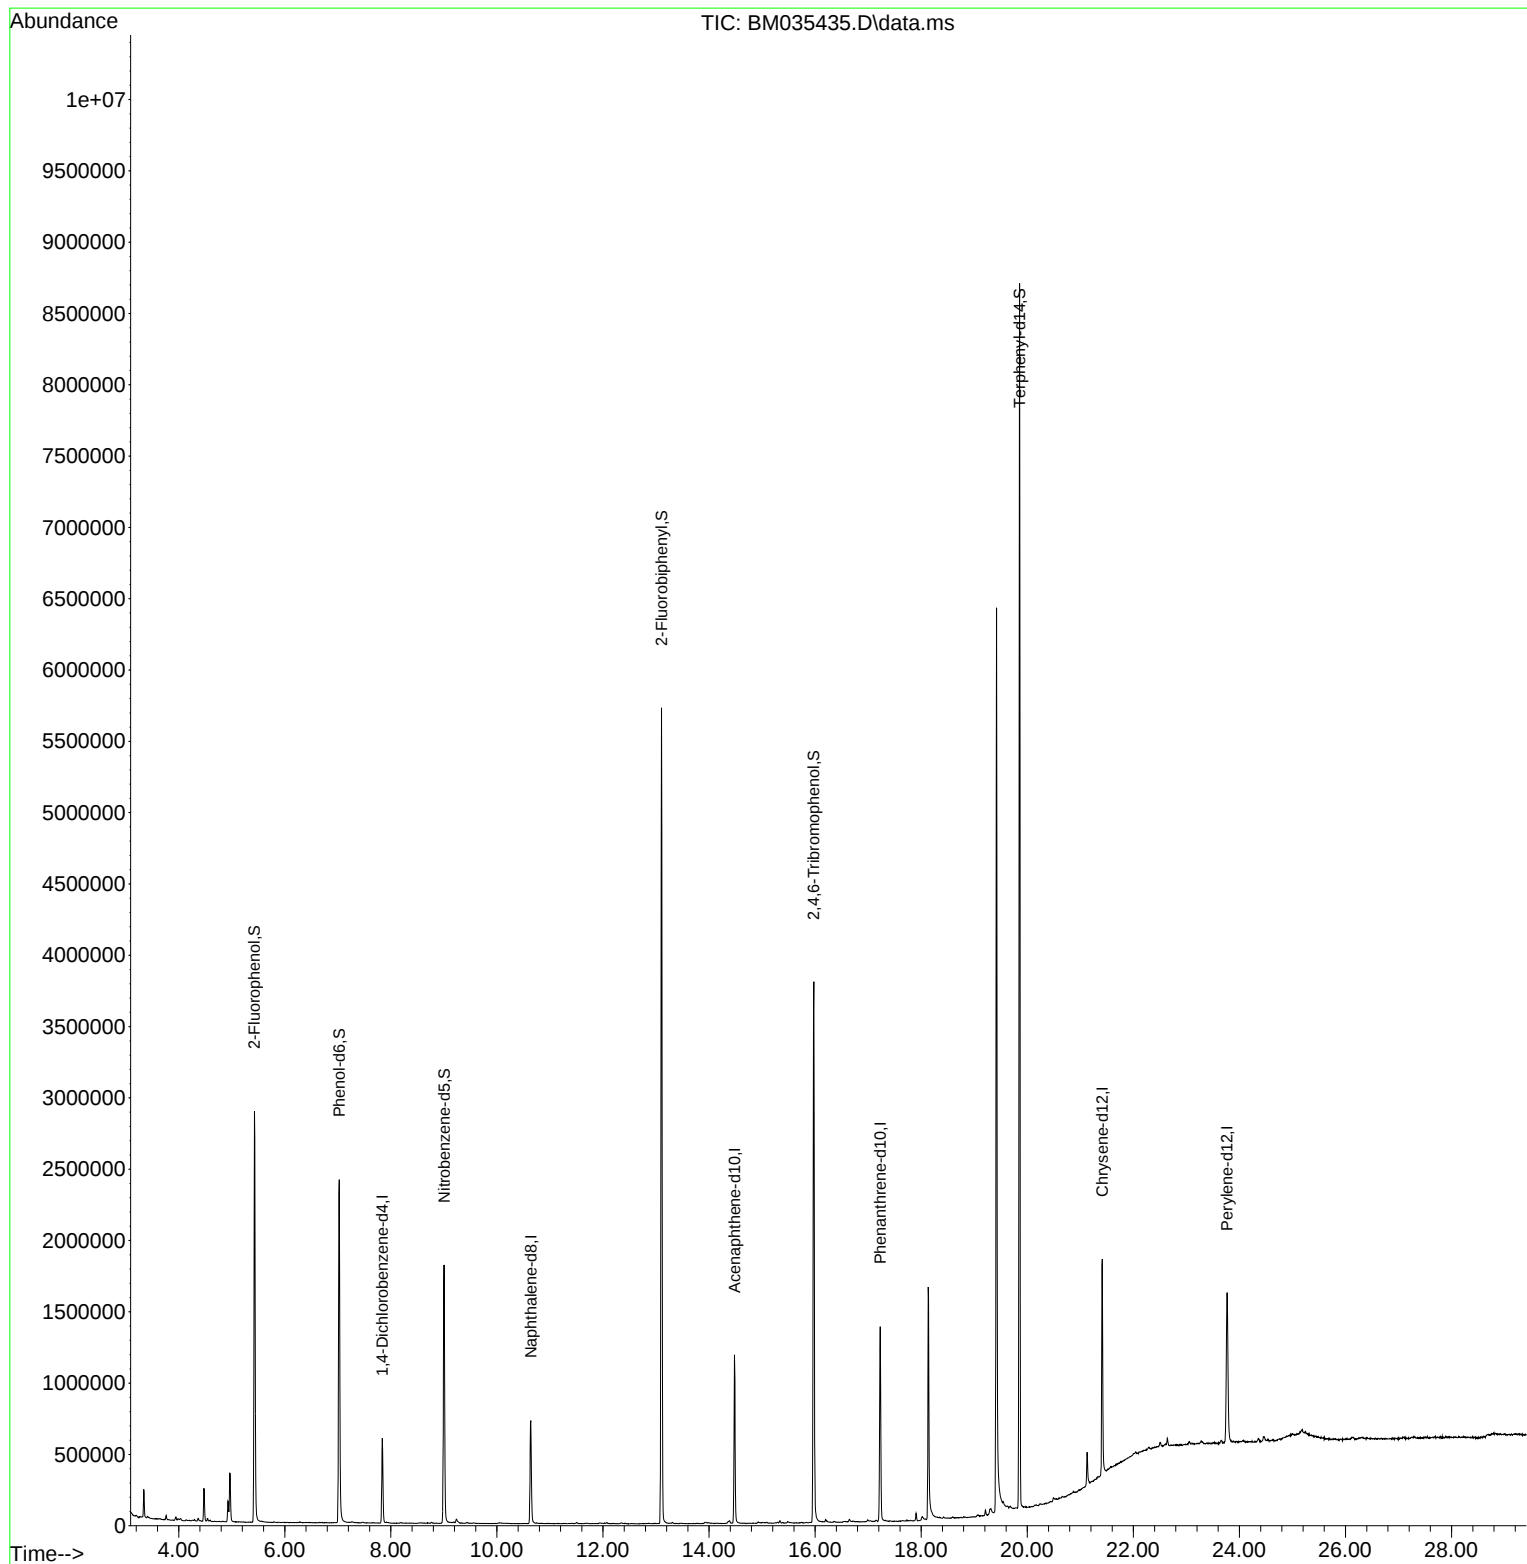


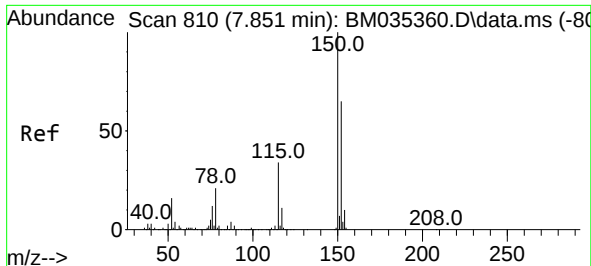

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.839 min Scan# 80
Delta R.T. -0.001 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24




Instrument :
BNA_M
ClientSampleId :
20220400-C-2-TCLP


Tgt Ion:152 Resp: 186446
Ion Ratio Lower Upper
152 100
150 155.5 124.9 187.3
115 52.4 47.9 71.9

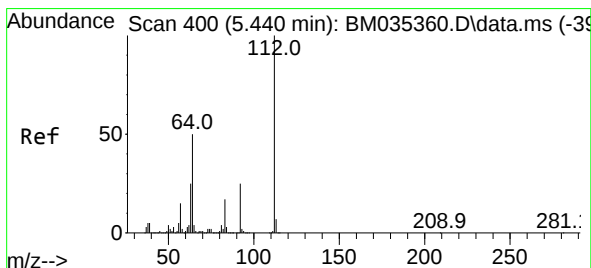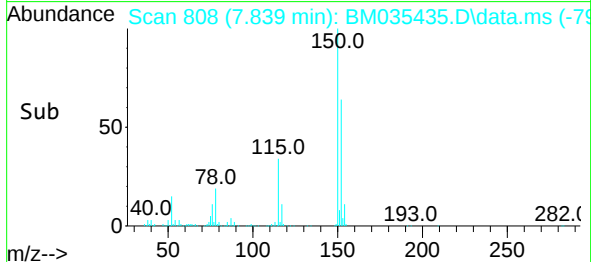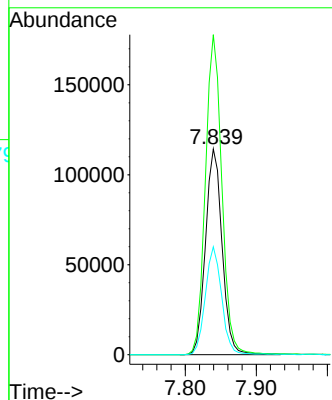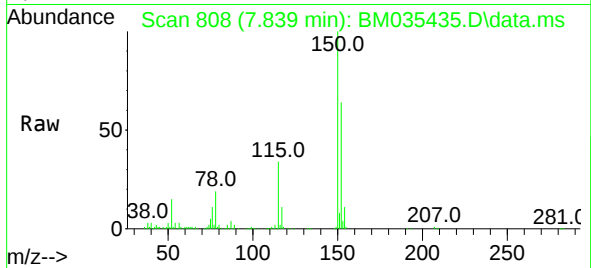

#5
2-Fluorophenol
Concen: 155.426 ng
RT: 5.428 min Scan# 398
Delta R.T. -0.000 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24

Tgt Ion:112 Resp: 1379066
Ion Ratio Lower Upper
112 100
64 51.0 47.8 71.6
63 25.9 26.6 40.0#


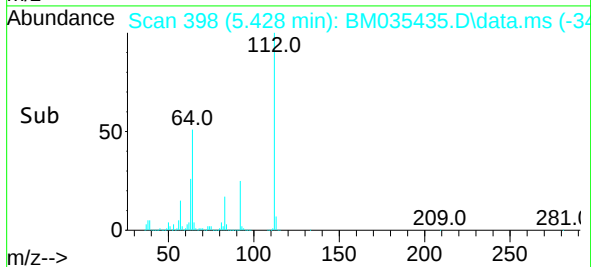
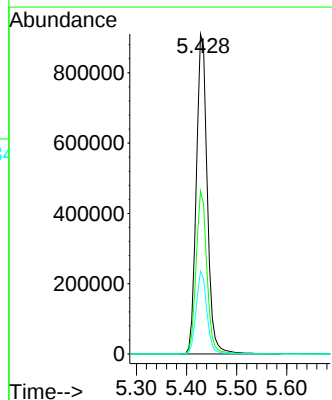
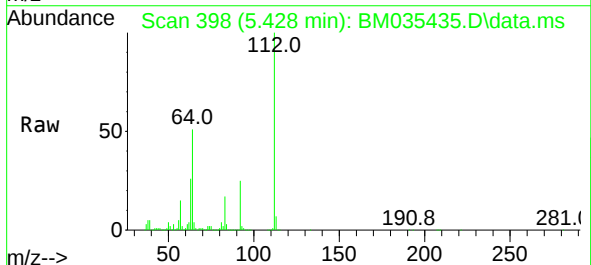


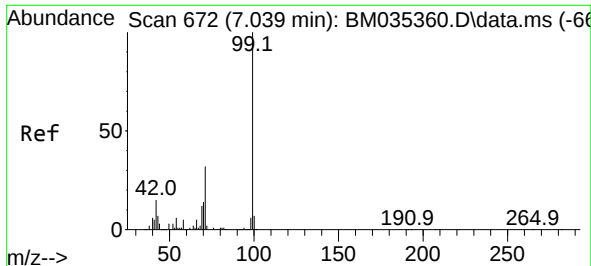

#7
Phenol-d6
Concen: 129.607 ng
RT: 7.028 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24




Instrument :
BNA_M
ClientSampleId :
20220400-C-2-TCLP


Tgt Ion: 99 Resp: 1570826
Ion Ratio Lower Upper
99 100
42 14.6 18.8 28.2#
71 30.5 30.2 45.2

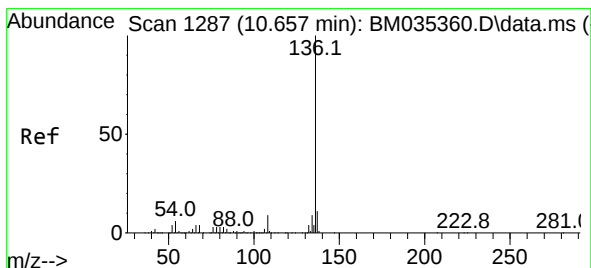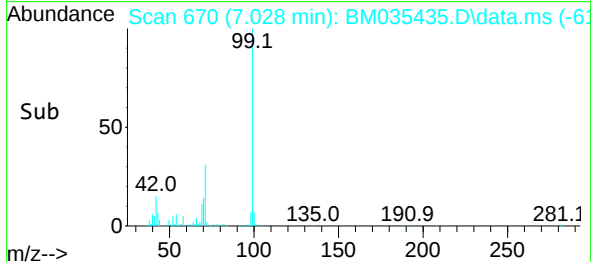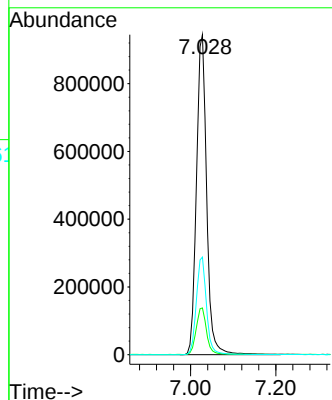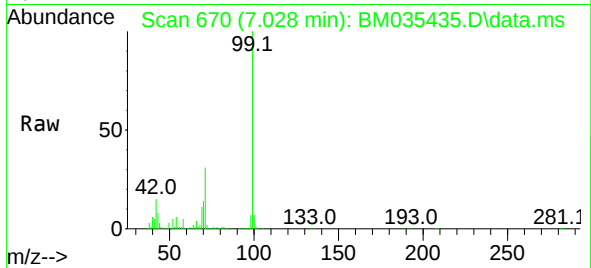

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.639 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24

Tgt Ion: 136 Resp: 680893
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 6.4 7.0 10.4#
68 5.2 4.3 6.5


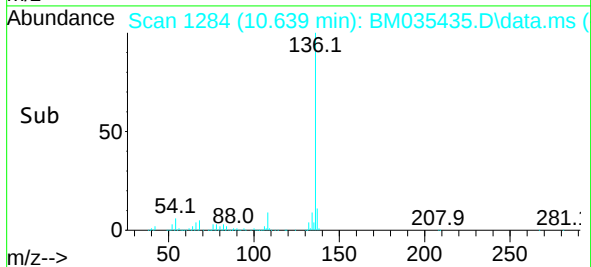
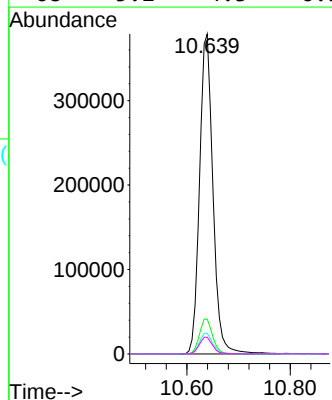
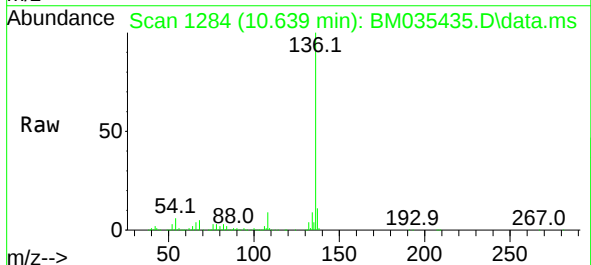


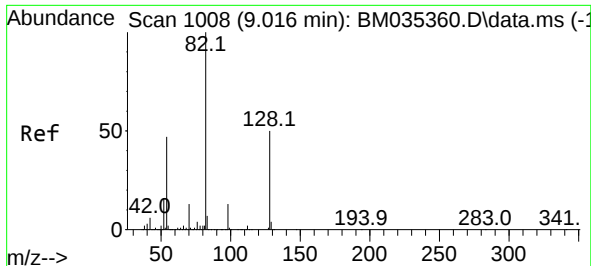

#23
Nitrobenzene-d5
Concen: 99.585 ng
RT: 9.004 min Scan# 10
Delta R.T. -0.000 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24




Instrument :
BNA_M
ClientSampleId :
20220400-C-2-TCLP


Tgt Ion: 82 Resp: 1067887
Ion Ratio Lower Upper
82 100
128 51.9 33.7 50.5#
54 44.5 43.2 64.8

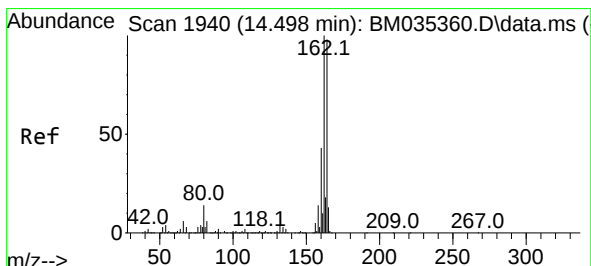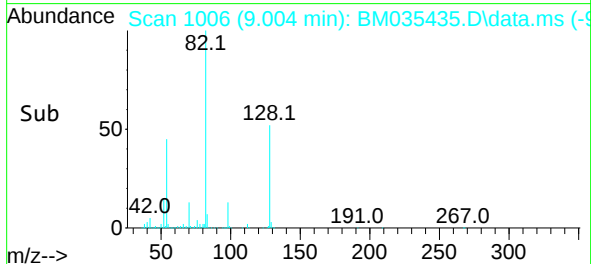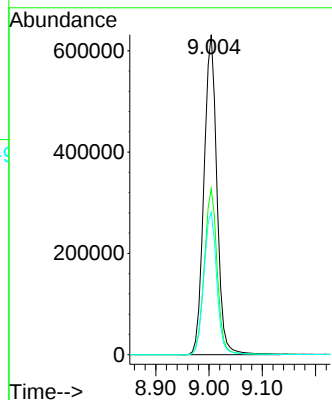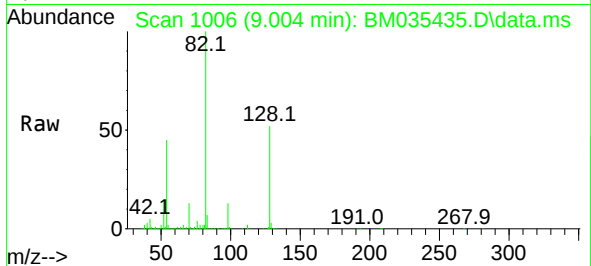

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.480 min Scan# 1937
Delta R.T. -0.006 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24

Tgt Ion: 164 Resp: 437390
Ion Ratio Lower Upper
164 100
162 101.0 83.0 124.6
160 43.1 37.0 55.4


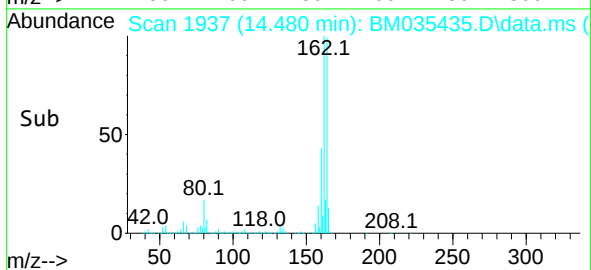
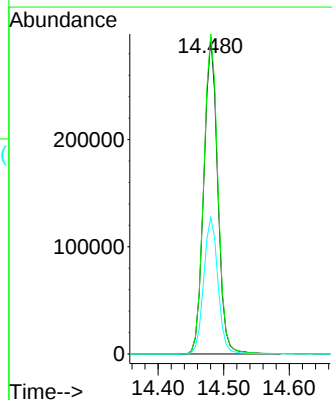
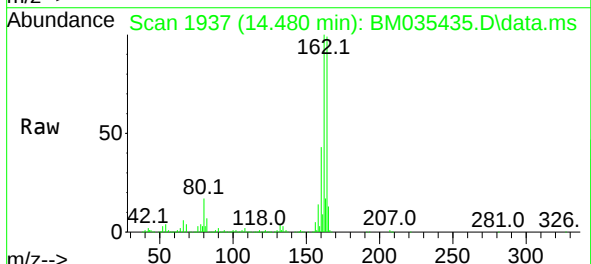


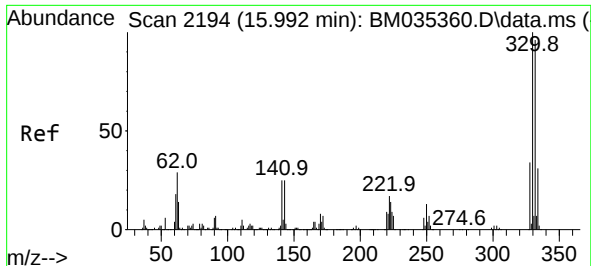

#42
2,4,6-Tribromophenol
Concen: 135.606 ng
RT: 15.974 min Scan# 2194
Delta R.T. -0.006 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24




Instrument :
BNA_M
ClientSampleId :
20220400-C-2-TCLP


Tgt Ion:330 Resp: 951653
Ion Ratio Lower Upper
330 100
332 96.3 77.0 115.4
141 23.6 35.3 52.9#

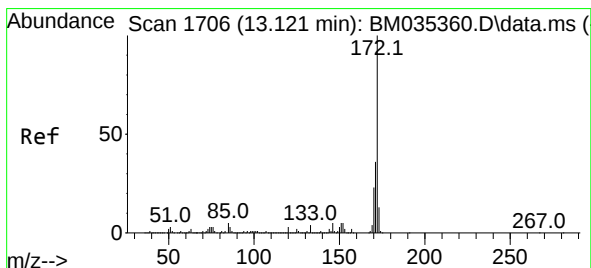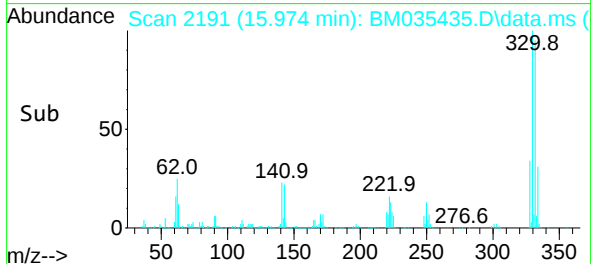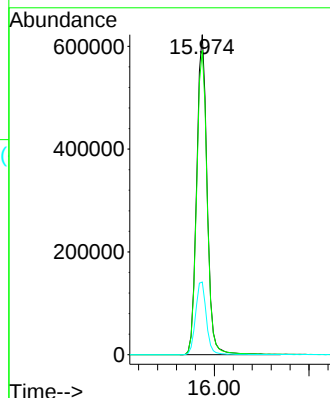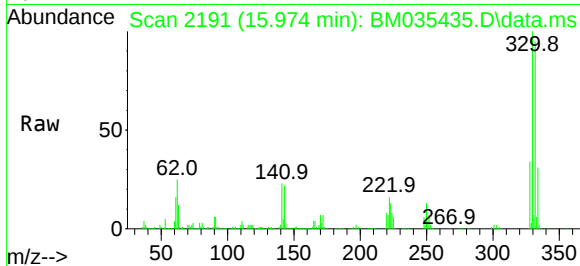

#45
2-Fluorobiphenyl
Concen: 103.366 ng
RT: 13.104 min Scan# 1703
Delta R.T. -0.006 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24

Tgt Ion:172 Resp: 3147837
Ion Ratio Lower Upper
172 100
171 35.9 28.5 42.7
170 23.5 18.7 28.1


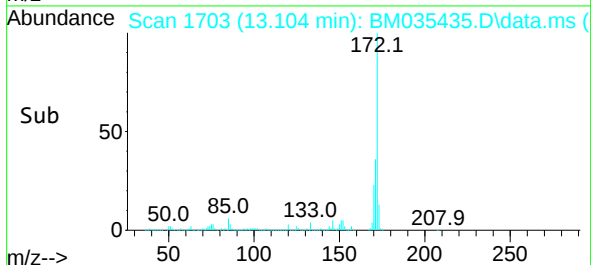
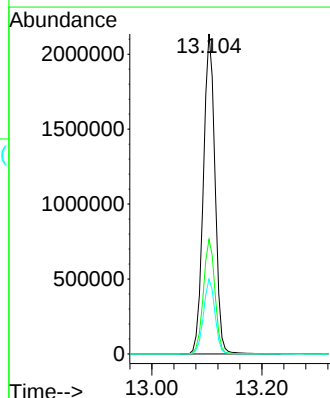
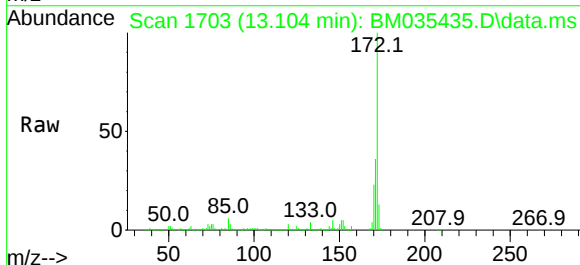


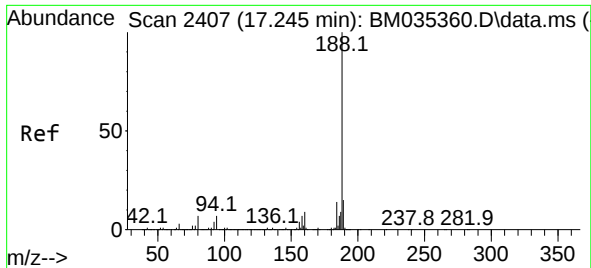

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.227 min Scan# 2404
Delta R.T. -0.000 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24




Instrument :
BNA_M
ClientSampleId :
20220400-C-2-TCLP


Tgt Ion:188 Resp: 905447
Ion Ratio Lower Upper
188 100
94 7.4 7.0 10.4
80 7.6 7.6 11.4#

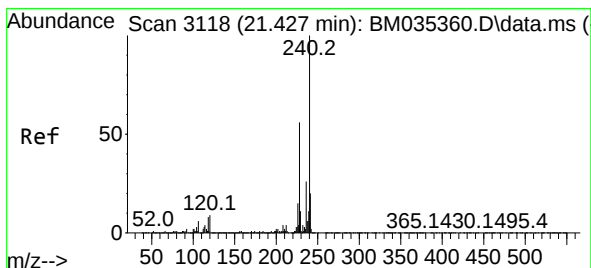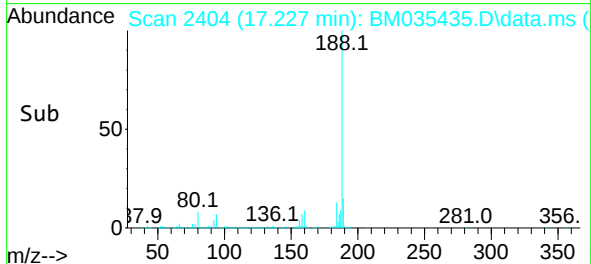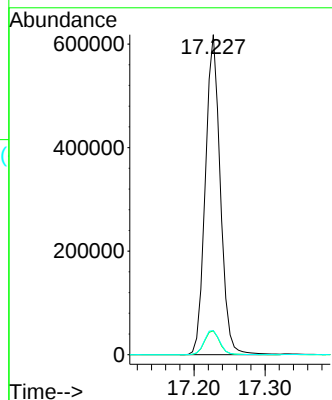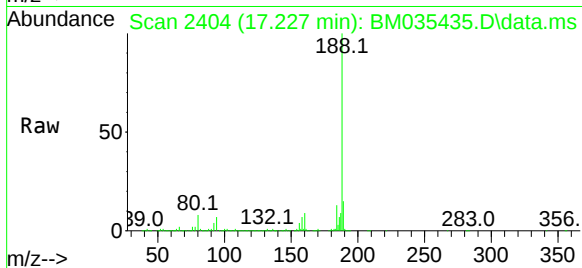

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.415 min Scan# 3116
Delta R.T. -0.006 min
Lab File: BM035435.D
Acq: 08 Jun 2022 18:24

Tgt Ion:240 Resp: 825593
Ion Ratio Lower Upper
240 100
120 8.2 9.4 14.0#
236 25.4 20.6 30.8

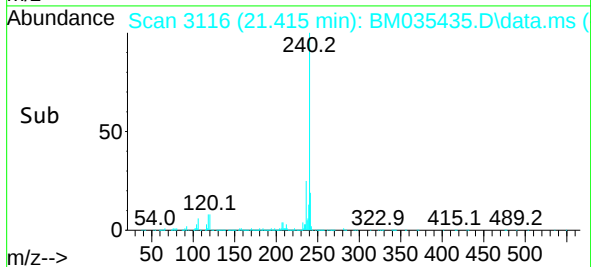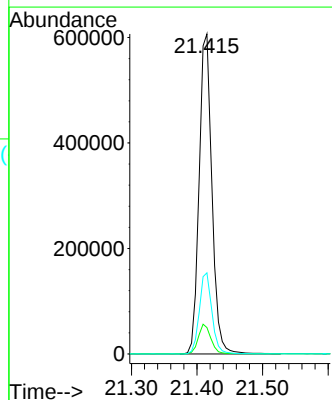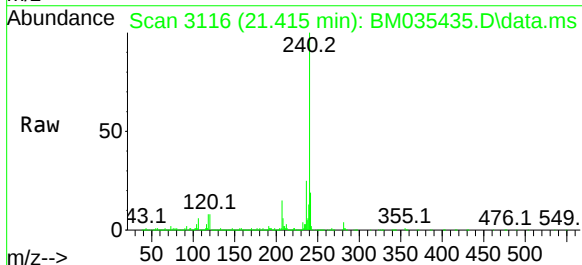

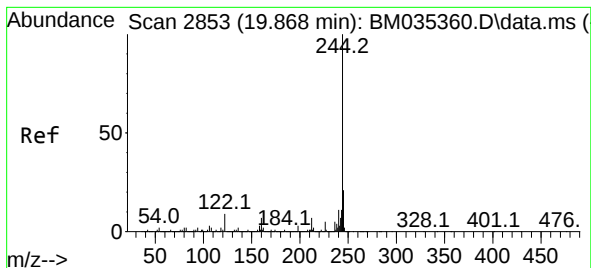

#79

Terphenyl-d14

Concen: 111.530 ng

RT: 19.856 min Scan# 21

Delta R.T. -0.000 min

Lab File: BM035435.D

Acq: 08 Jun 2022 18:24

Instrument :

BNA_M

ClientSampleId :

20220400-C-2-TCLP





Tgt Ion:244 Resp: 4621767

Ion Ratio Lower Upper

244 100

212 6.6 6.2 9.4

122 8.2 8.3 12.5#

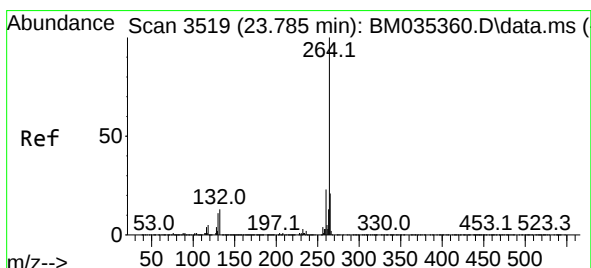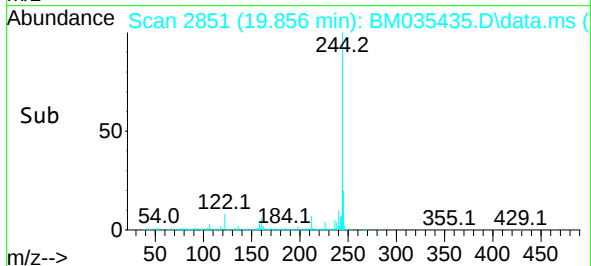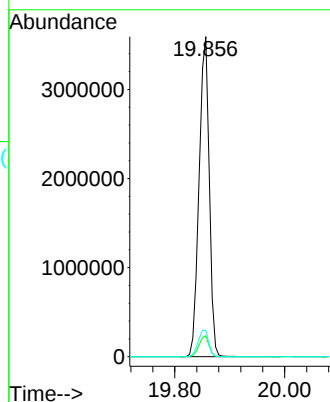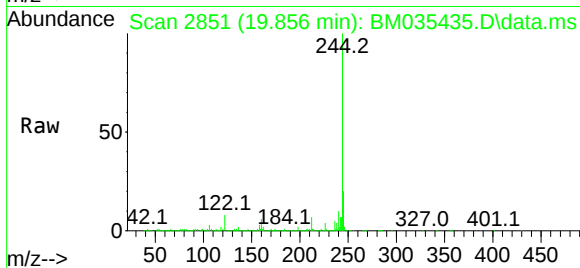

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.768 min Scan# 3516

Delta R.T. -0.006 min

Lab File: BM035435.D

Acq: 08 Jun 2022 18:24

Tgt Ion:264 Resp: 897729

Ion Ratio Lower Upper

264 100

260 23.3 18.9 28.3

265 22.3 17.5 26.3

