

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035425.D
Acq On : 08 Jun 2022 11:58
Operator : CG/JU
Sample : PB145396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145396BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	421	rBV	2421455	3752667	27.08%	7.354%
2	7.022	662	669	688	rBV	2311485	3859435	27.85%	7.563%
3	7.840	801	808	819	rBV	506805	836070	6.03%	1.638%
4	8.998	997	1005	1028	rBV	1338965	2461038	17.76%	4.823%
5	10.639	1276	1284	1305	rBV	640774	1221282	8.81%	2.393%
6	13.104	1696	1703	1721	rBV	4974422	7430256	53.61%	14.560%
7	14.480	1930	1937	1953	rBV	1267636	1912077	13.80%	3.747%
8	15.974	2184	2191	2217	rBV	3846730	6095158	43.98%	11.944%
9	17.227	2397	2404	2423	rBV	1680627	2521060	18.19%	4.940%
10	19.856	2844	2851	2863	rBV	10530517	13859808	100.00%	27.159%
11	21.409	3110	3115	3126	rBV	2423461	3499863	25.25%	6.858%
12	23.762	3509	3515	3529	rVB2	1671973	3582801	25.85%	7.021%




Sum of corrected areas: 51031515

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035425.D
Acq On : 08 Jun 2022 11:58
Operator : CG/JU
Sample : PB145396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145396BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

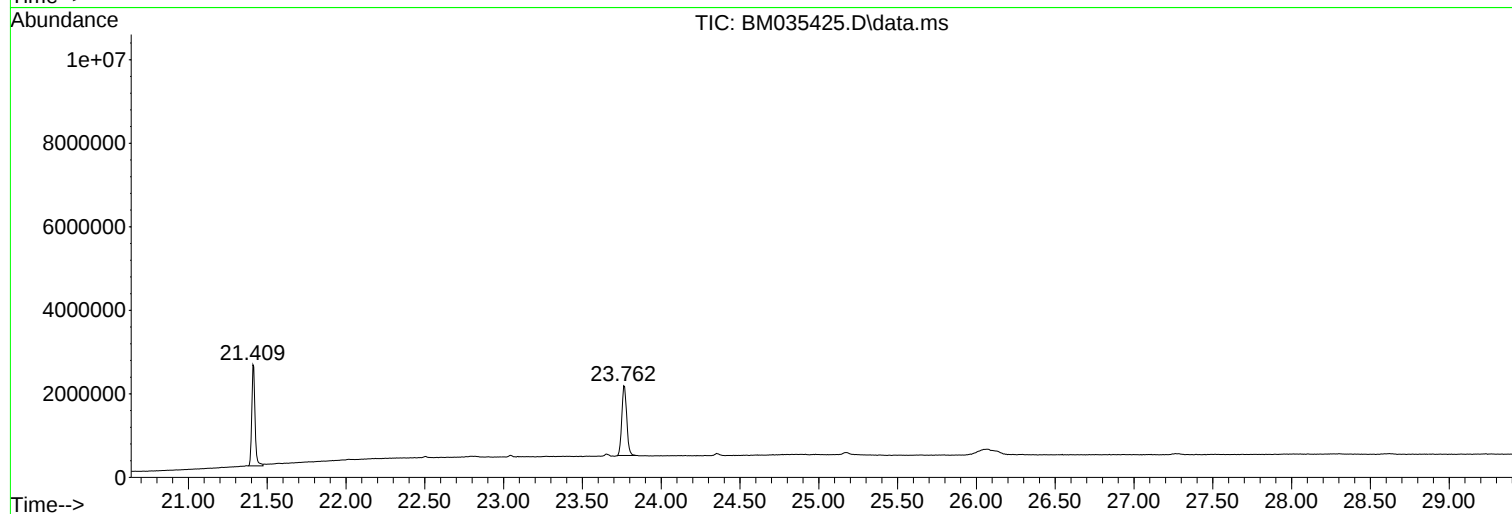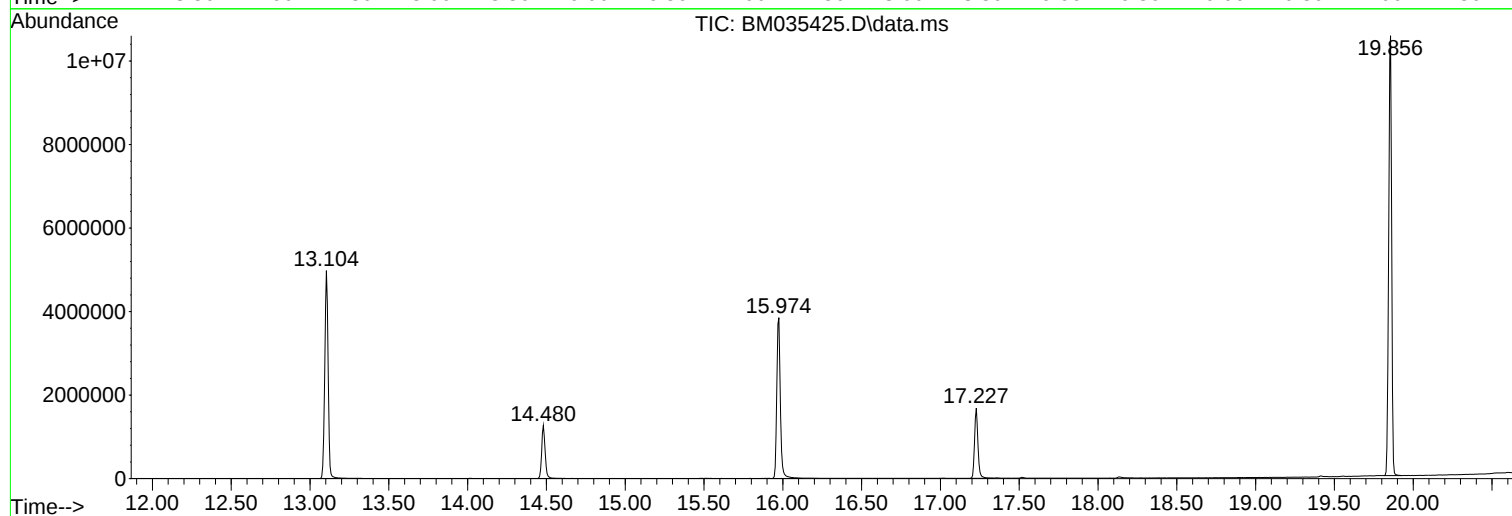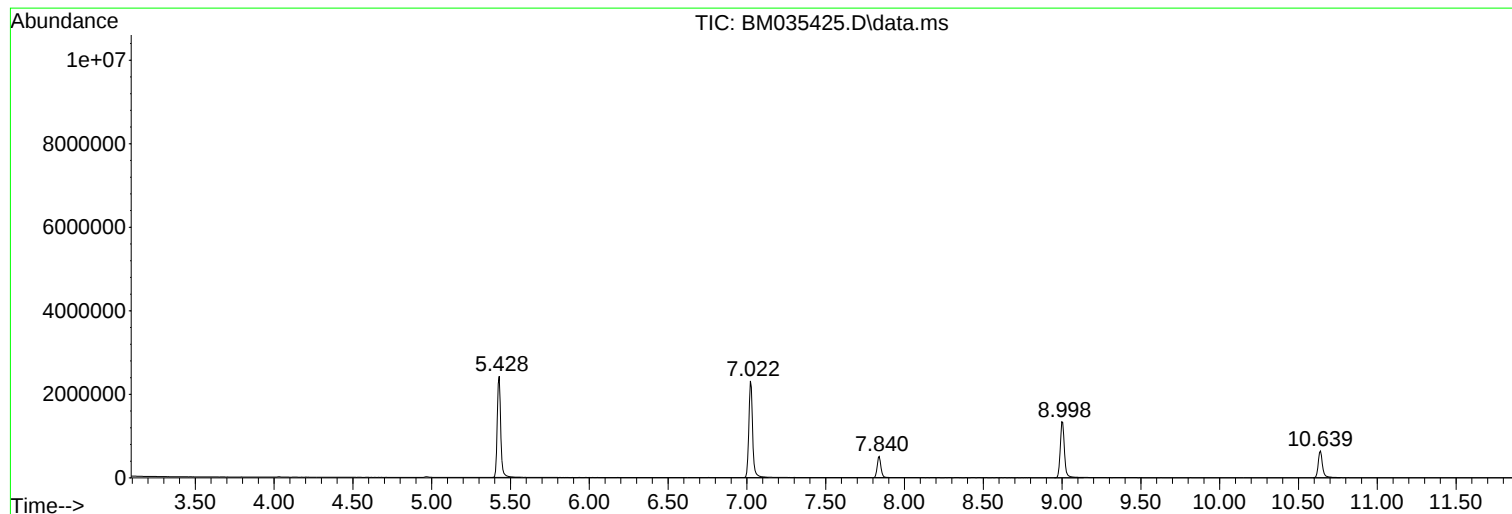

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035425.D
Acq On : 08 Jun 2022 11:58
Operator : CG/JU
Sample : PB145396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145396BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035425.D
Acq On : 08 Jun 2022 11:58
Operator : CG/JU
Sample : PB145396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145396BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------