

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
 Data File : BM035427.D
 Acq On : 08 Jun 2022 13:16
 Operator : CG/JU
 Sample : PB145400BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145400BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	417	rBV	2273703	3623182	26.14%	7.166%
2	7.022	662	669	688	rBV	2231642	3745070	27.02%	7.407%
3	7.840	801	808	818	rBV	484494	806575	5.82%	1.595%
4	9.004	998	1006	1025	rBV	1301386	2378050	17.16%	4.703%
5	10.639	1277	1284	1305	rBV	622999	1200870	8.66%	2.375%
6	13.104	1696	1703	1722	rBV	4891241	7360555	53.11%	14.557%
7	14.480	1930	1937	1955	rBV	1232134	1915554	13.82%	3.788%
8	15.974	2184	2191	2219	rBV	3858573	6062461	43.74%	11.990%
9	17.227	2398	2404	2421	rBV	1613740	2517085	18.16%	4.978%
10	19.857	2845	2851	2861	rBV	11425437	13859011	100.00%	27.409%
11	21.415	3111	3116	3126	rBV	2577843	3501314	25.26%	6.925%
12	23.768	3510	3516	3529	rVB2	1755066	3593775	25.93%	7.107%




Sum of corrected areas: 50563502

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035427.D
Acq On : 08 Jun 2022 13:16
Operator : CG/JU
Sample : PB145400BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145400BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

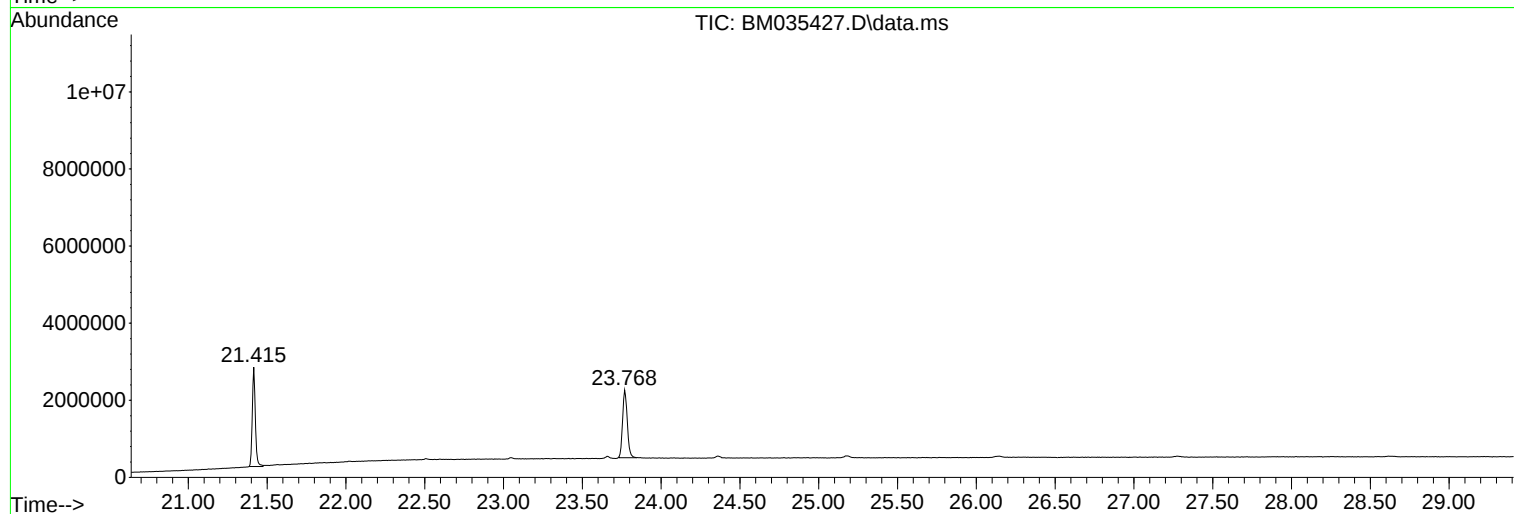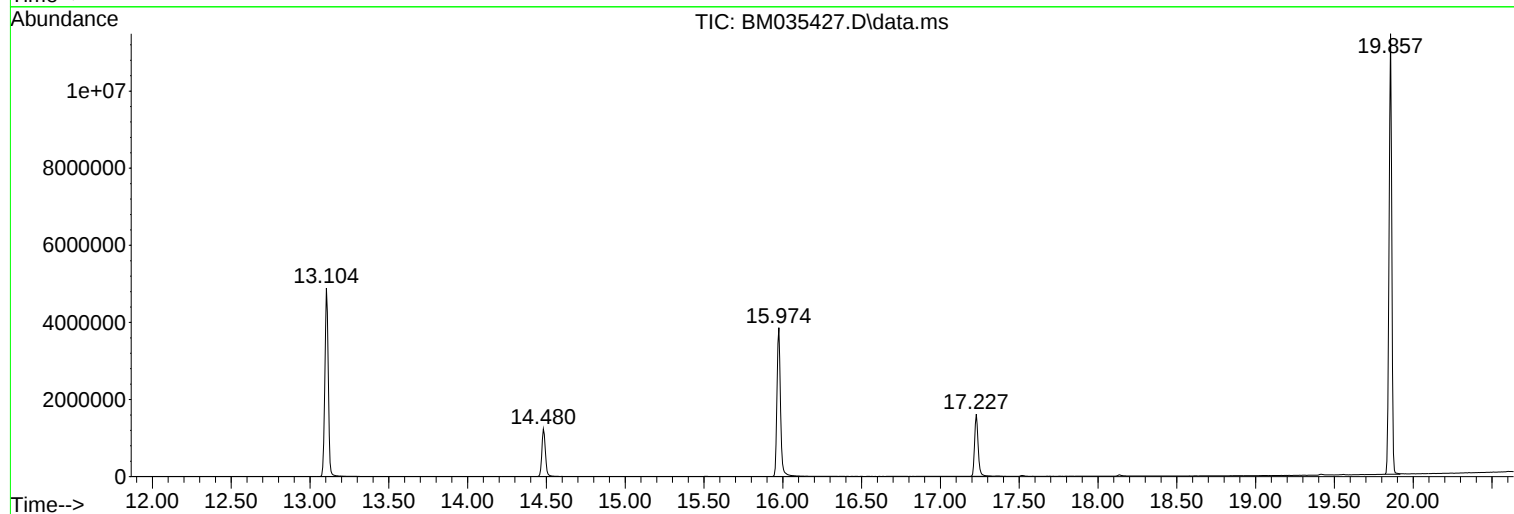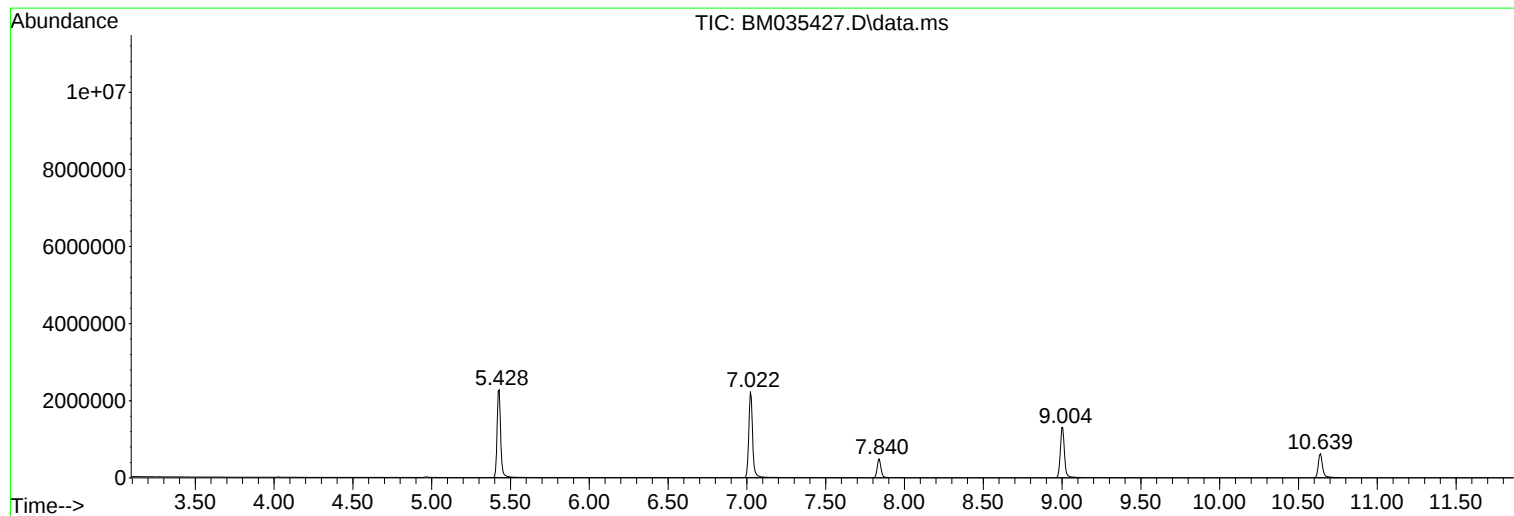

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035427.D
Acq On : 08 Jun 2022 13:16
Operator : CG/JU
Sample : PB145400BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145400BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035427.D
Acq On : 08 Jun 2022 13:16
Operator : CG/JU
Sample : PB145400BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145400BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------