

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
 Data File : BM035439.D
 Acq On : 08 Jun 2022 20:52
 Operator : CG/JU
 Sample : N3215-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 N48964

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	392	398	415	rBV	481311	825135	12.46%	2.982%
2	7.028	664	670	685	rBV	275824	552506	8.34%	1.997%
3	7.839	801	808	817	rBV	598788	986238	14.89%	3.564%
4	8.998	998	1005	1028	rBV	956685	1721699	25.99%	6.223%
5	10.639	1276	1284	1300	rBV	749433	1360610	20.54%	4.918%
6	13.104	1696	1703	1716	rBV	3045550	4671975	70.53%	16.886%
7	14.480	1930	1937	1951	rBV	1221220	1879899	28.38%	6.794%
8	15.974	2185	2191	2209	rBV	704656	1302074	19.66%	4.706%
9	17.227	2397	2404	2419	rBV	1401128	2221195	33.53%	8.028%
10	19.850	2844	2850	2858	rBV	5239746	6623649	100.00%	23.939%
11	21.121	3062	3066	3077	rBV	628454	1036138	15.64%	3.745%
12	21.409	3110	3115	3126	rBV	1572234	2266343	34.22%	8.191%
13	23.762	3509	3515	3527	rVB2	1059476	2220980	33.53%	8.027%




Sum of corrected areas: 27668441

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035439.D
Acq On : 08 Jun 2022 20:52
Operator : CG/JU
Sample : N3215-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
N48964

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

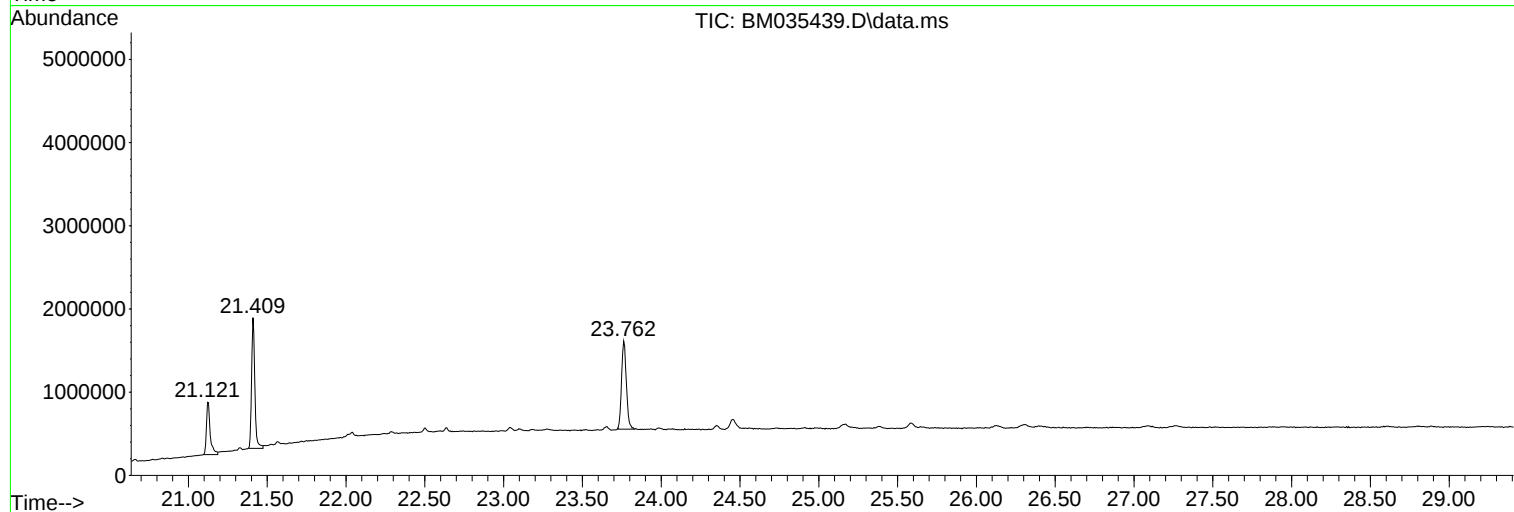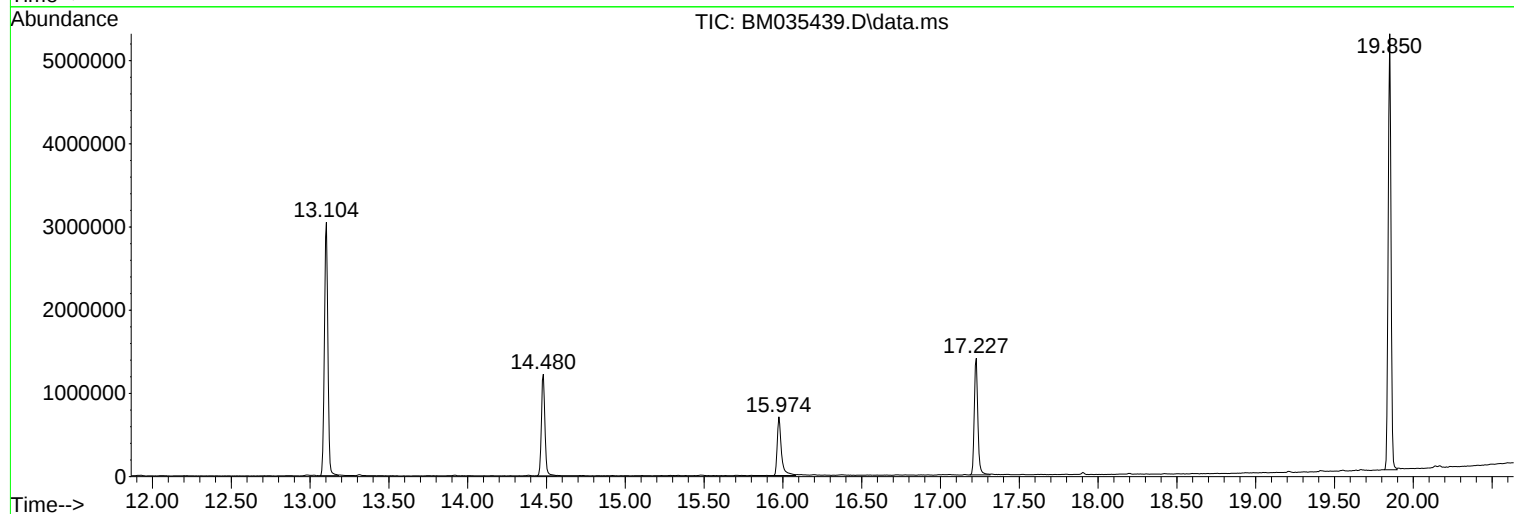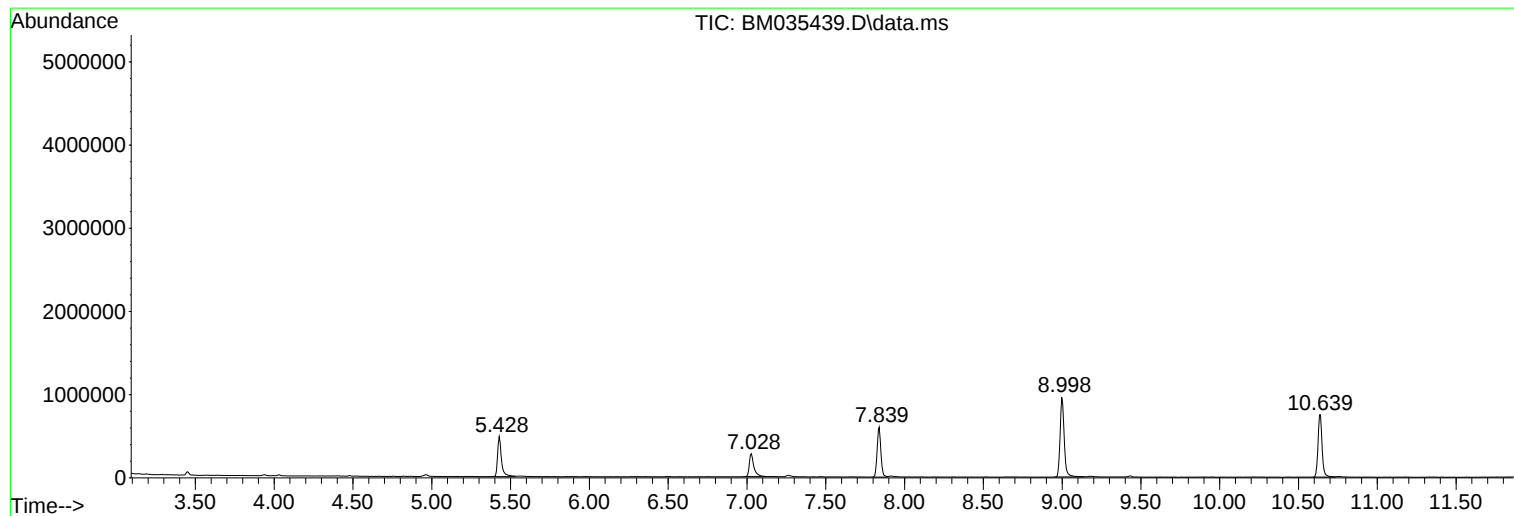

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035439.D
Acq On : 08 Jun 2022 20:52
Operator : CG/JU
Sample : N3215-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
N48964










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 E-15-Heptadecenal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.121	9.14 ng	1036140	Chrysene-d12	21.409

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		E-15-Heptadecenal	252	C17H32O	1000130-97-9	96
2		1-Hexacosene	364	C26H52	018835-33-1	95
3		n-Tetracosanol-1	354	C24H50O	000506-51-4	94
4		Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
5		1-Tetracosene	336	C24H48	010192-32-2	94

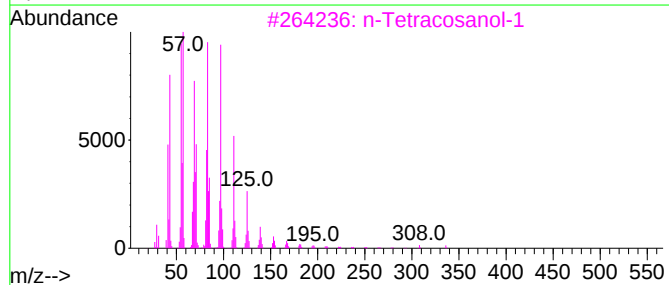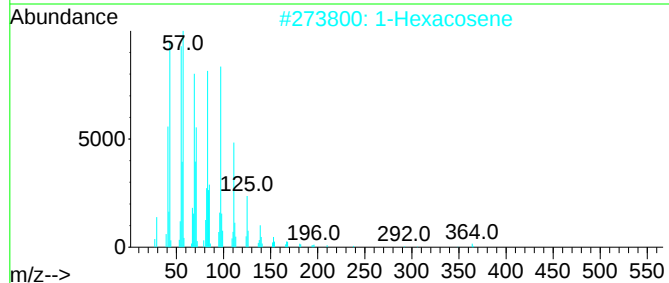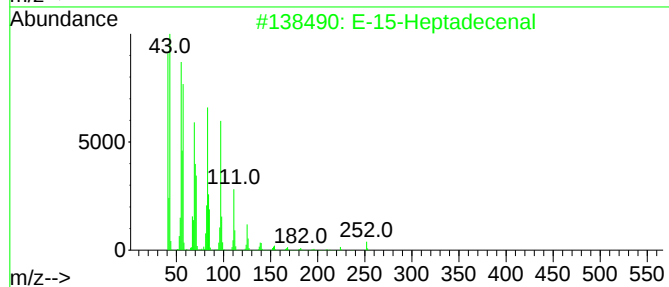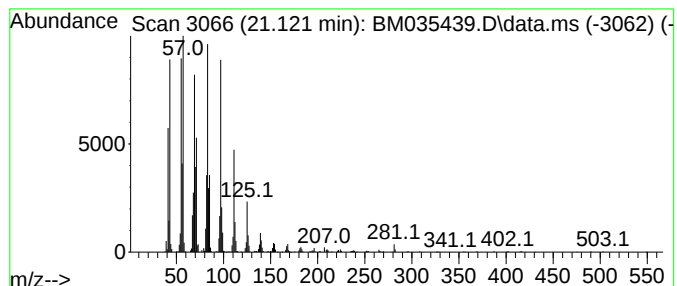

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035439.D
Acq On : 08 Jun 2022 20:52
Operator : CG/JU
Sample : N3215-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
N48964

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
E-15-Heptadecenal	21.121	9.1	ng	1036140	5	21.409	2266340	20.0