
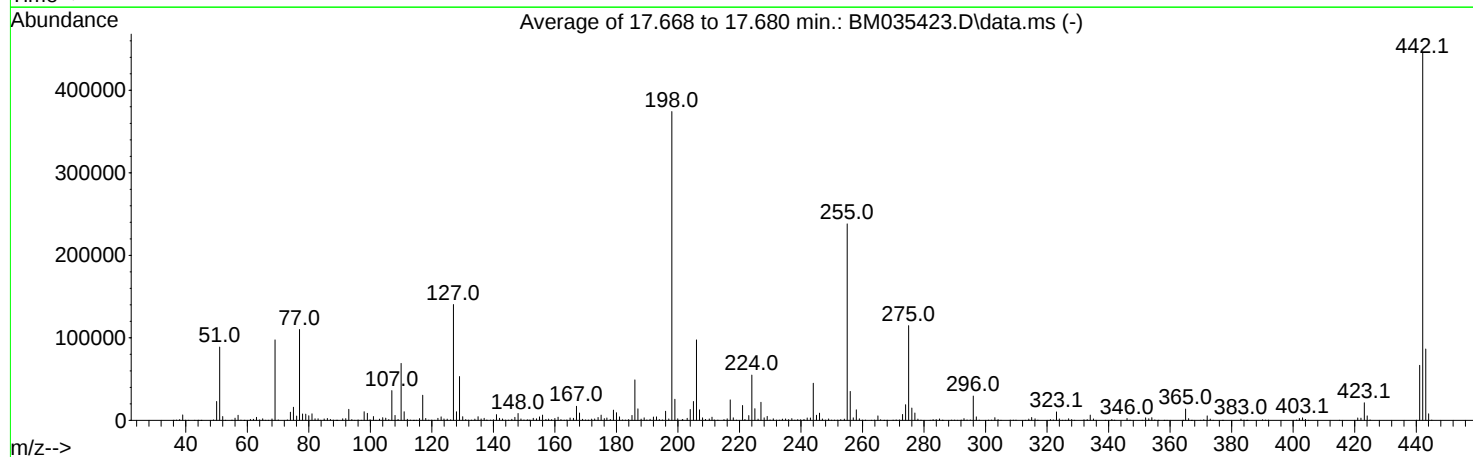


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
 Data File : BM035423.D
 Acq On : 08 Jun 2022 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 07 14:28:07 2022

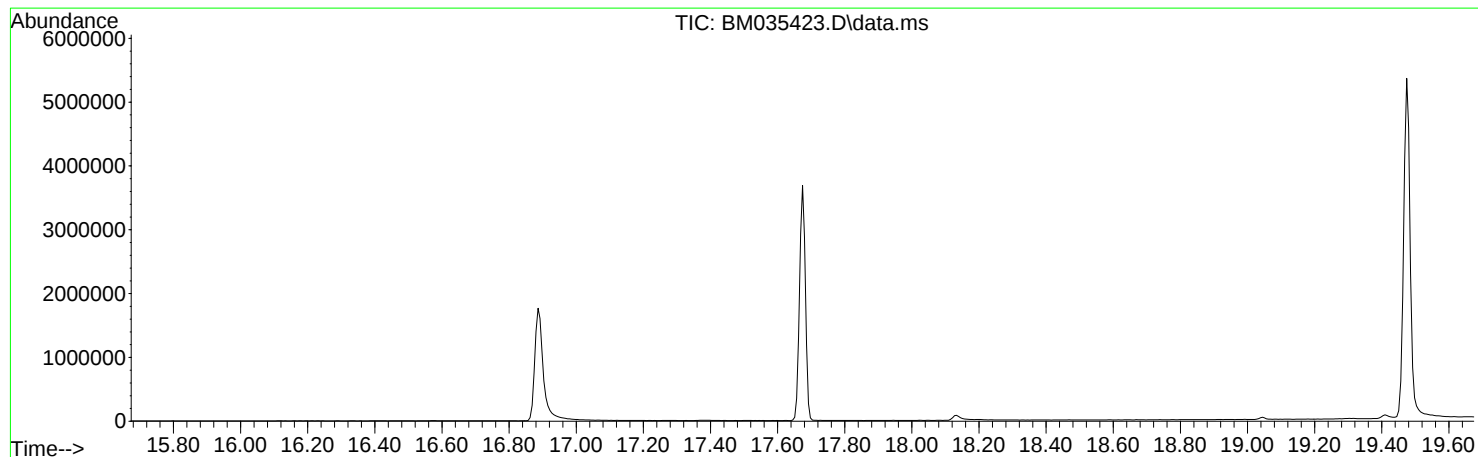




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.7	88843	PASS
68	69	0.00	2	1.8	1777	PASS
69	198	0.00	100	26.1	97525	PASS
70	69	0.00	2	0.5	519	PASS
127	198	10	80	37.5	140336	PASS
197	198	0.00	2	0.5	1850	PASS
198	198	100	100	100.0	374315	PASS
199	198	5	9	6.8	25541	PASS
275	198	10	60	30.7	114851	PASS
365	198	1	100	3.7	13741	PASS
441	198	0.01	100	17.8	66672	PASS
442	442	50	100	100.0	445845	PASS
443	442	15	24	19.4	86477	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
 Data File : BM035423.D
 Acq On : 08 Jun 2022 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 04:32:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 14:28:07 2022
 Response via : Initial Calibration

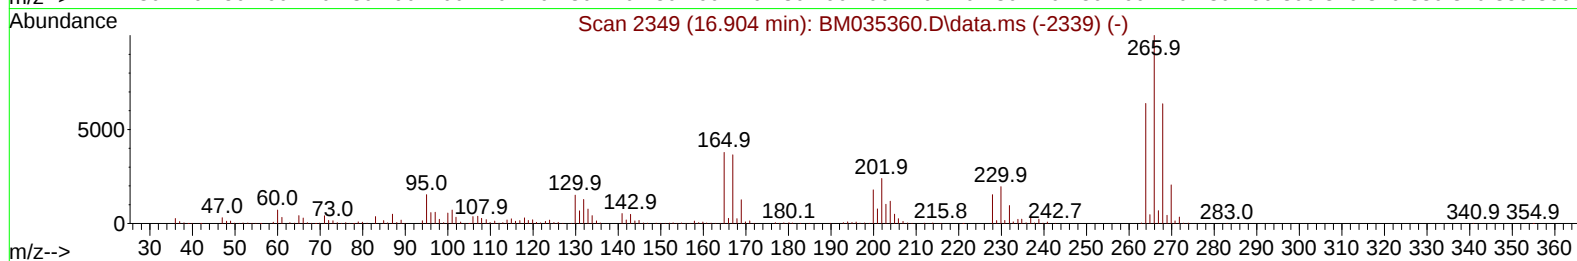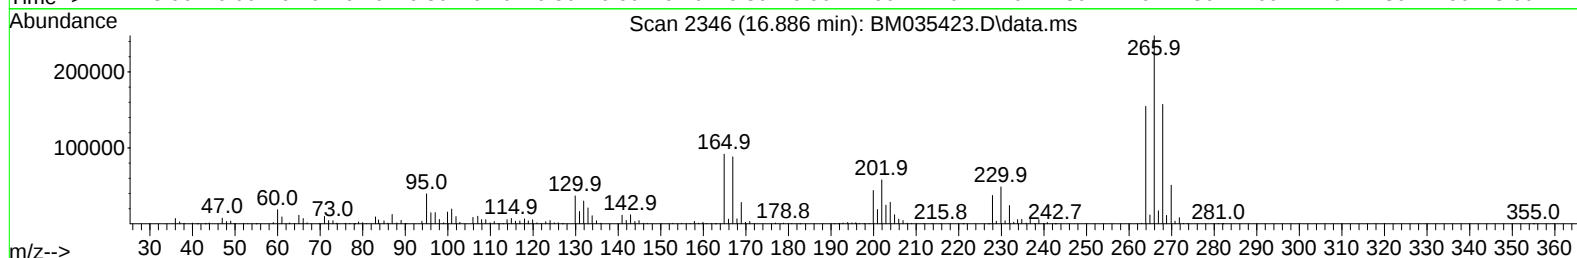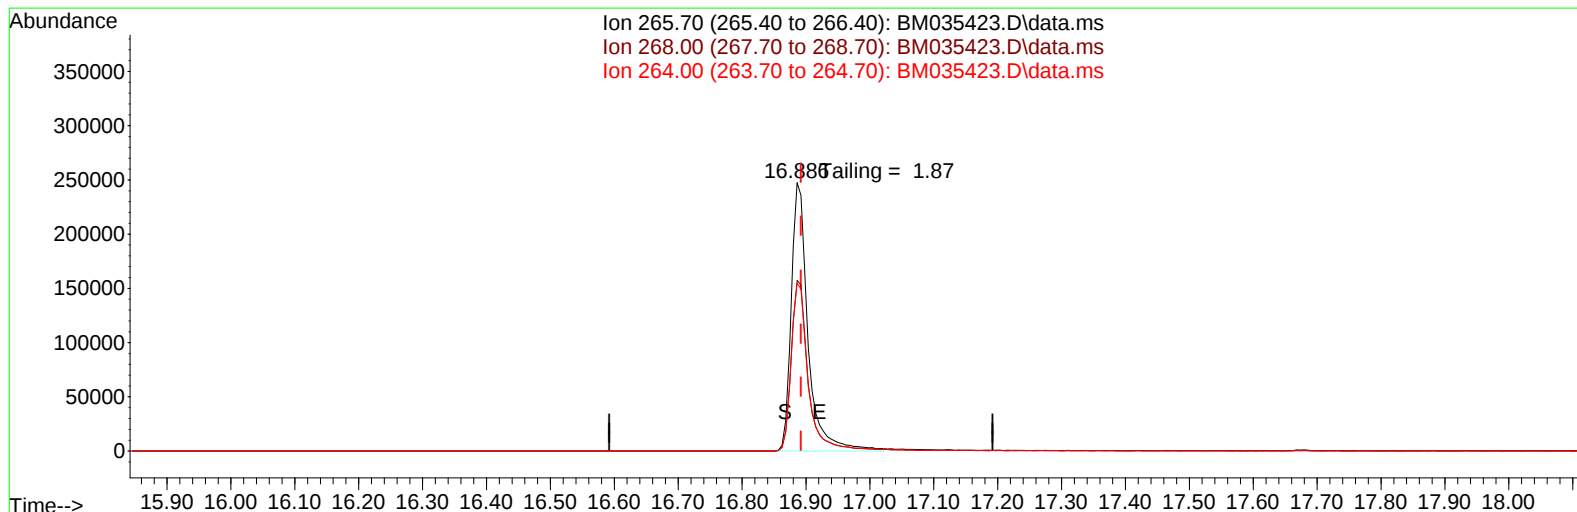

TIC: BM035423.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 0.00 ng




response 460318

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.54
264.00	63.30	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060822\
Data File : BM035423.D
Acq On : 08 Jun 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 09 04:32:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 14:28:07 2022
Response via : Initial Calibration

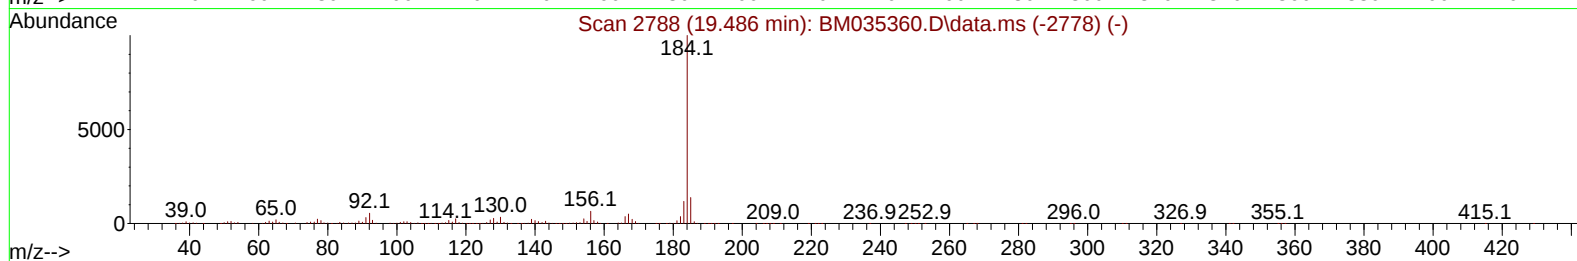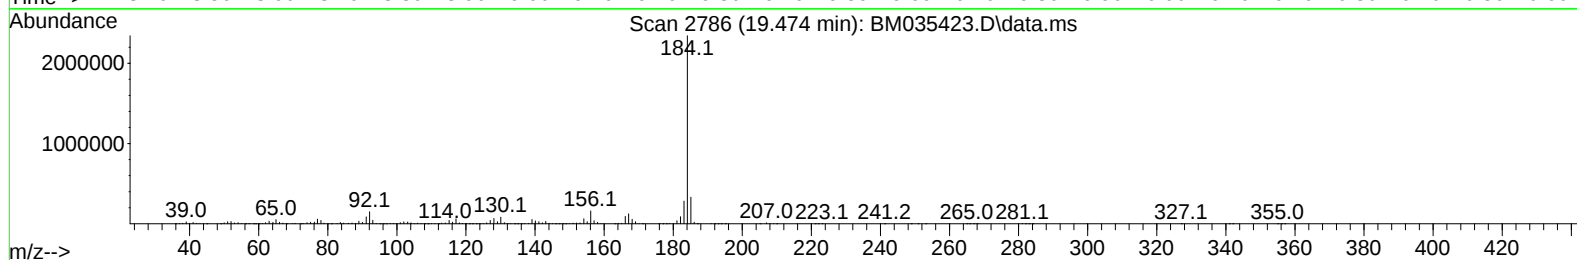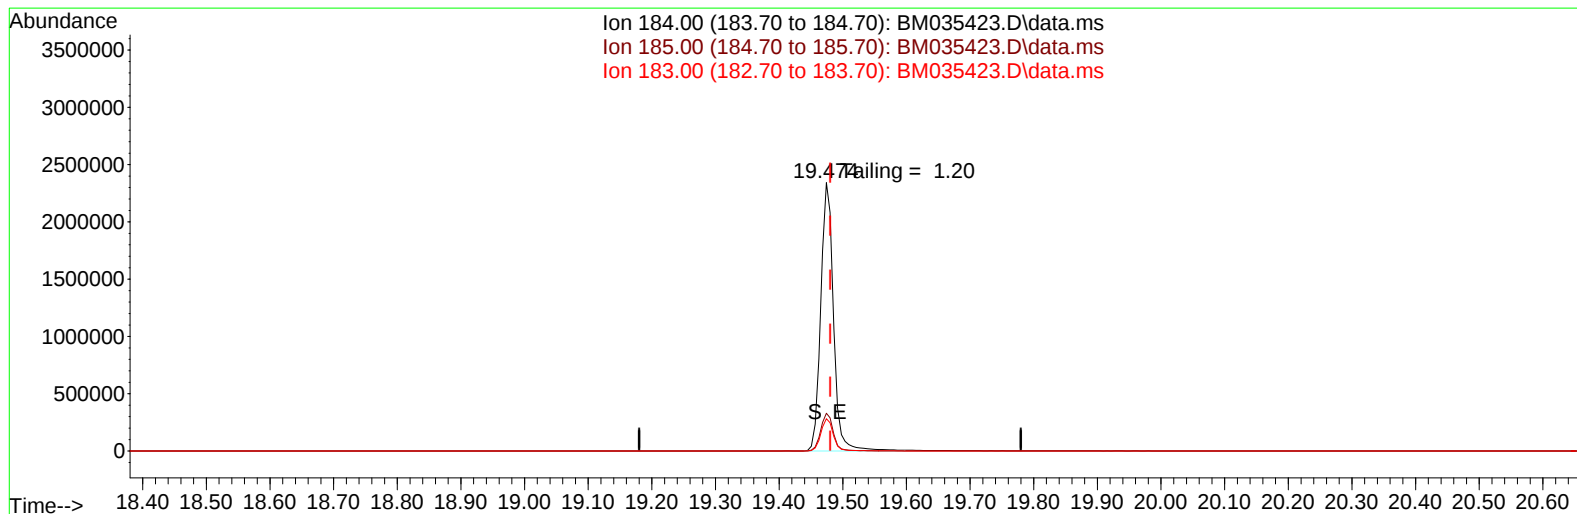

TIC: BM035423.D\data.ms

(77) Benzidine

19.474min (-0.006) 212929.25 ng

response 3278784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.90	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2022	BNA_M	BM035423.D
Compound Name	Response	Retention Time
DDT	1601273	20.709
DDD	19961	20.268
DDE	4031	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23992	1625265	1.48

Instrument :
BNA_M
ClientSampleId :
DFTPP