

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010447.D
 Acq On : 09 Jun 2017 11:16
 Operator : SJ/MA
 Sample : PB99575BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK75

Quant Time: Jun 10 01:46:54 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 10 01:45:50 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	238115	20.00	ng/ul	0.00
18) Naphthalene-d8	10.71	136	891144	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.54	164	616702	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	1498325	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	1540107	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1456566	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	27100	4.67	ng/uL	0.00
5) Phenol-d5	7.09	99	459031	25.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	251907	24.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	390997	27.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	388967	26.72	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	190093	29.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	233275	30.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	458660	29.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	516921	34.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	1749582	34.15	ng/ul	0.00
46) Acenaphthylene-d8	14.24	160	1830068	30.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.78	143	194859	25.42	ng/ul	0.00
57) Fluorene-d10	15.53	176	1437482	31.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	285379	26.89	ng/ul	0.00
70) Anthracene-d10	17.39	188	2450959	33.62	ng/ul	0.00
76) Pyrene-d10	19.67	212	2704300	42.46	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.64	264	2215363	32.67	ng/ul	0.00


Target Compounds					Qvalue
21) Isophorone	9.80	82	34877	1.216 ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010447.D
Acq On : 09 Jun 2017 11:16
Operator : SJ/MA
Sample : PB99575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Time: Jun 10 01:46:54 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 10 01:45:50 2017
Response via : Initial Calibration

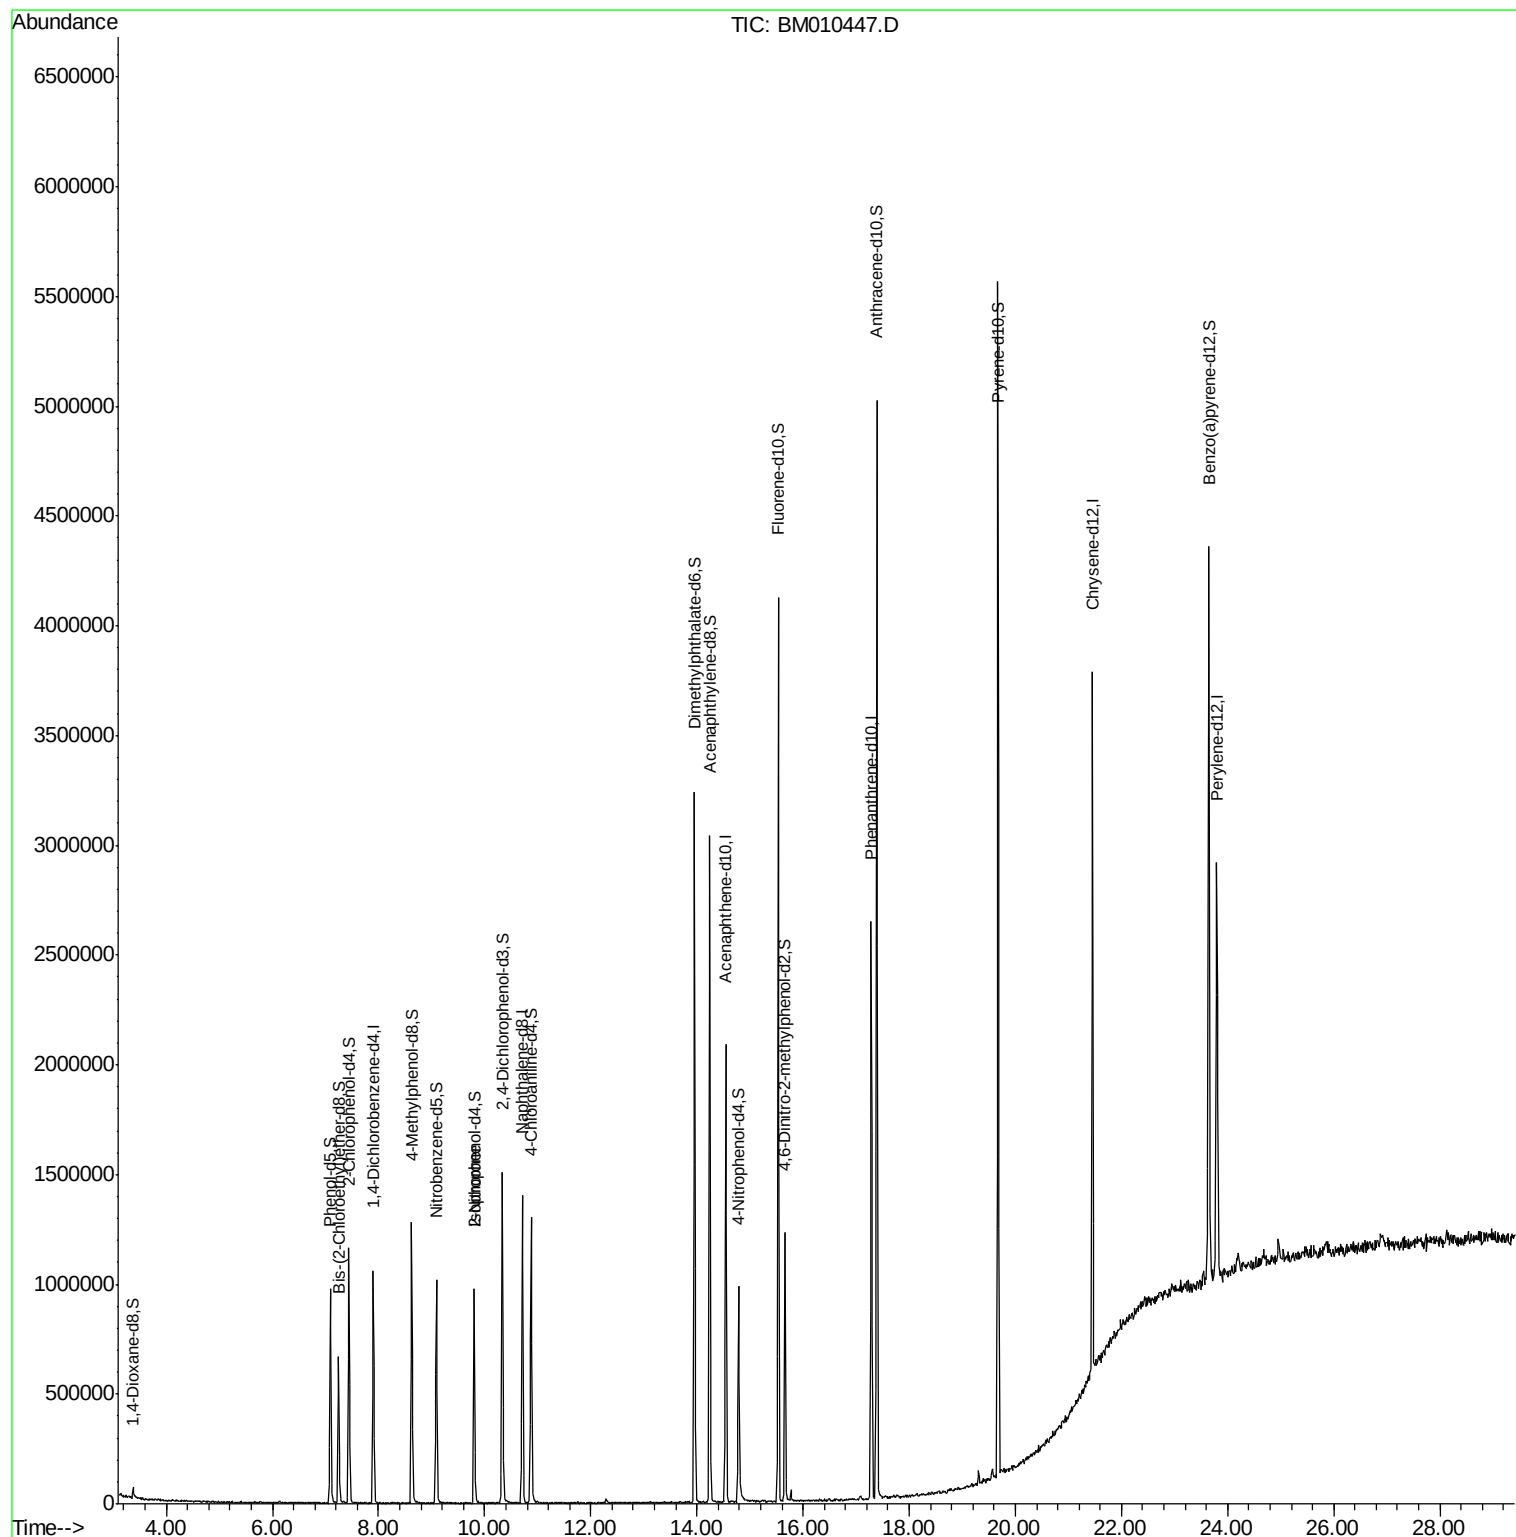

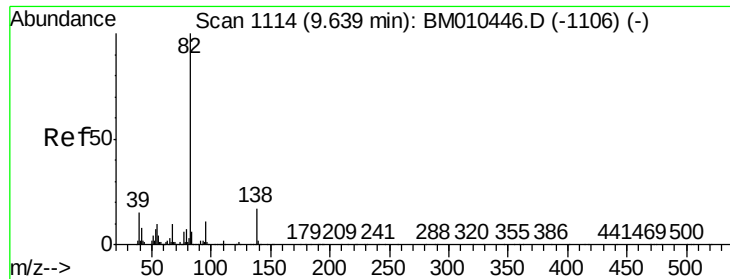

#21

Isophorone

Concen: 1.216 ng/ul

RT: 9.80 min Scan# 1142

Delta R.T. 0.16 min

Lab File: BM010447.D


Acq: 09 Jun 2017 11:16

Instrument :

BNA_M

ClientSampleId :

SBLK75

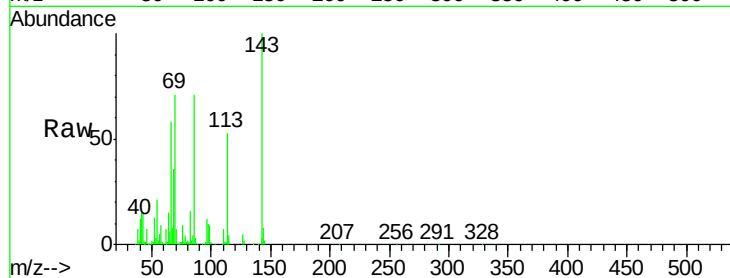

Tgt Ion:	82	Resp:	34877
Ion	Ratio	Lower	Upper
82	100		
95	5.8	7.8	11.8#
138	0.0	11.9	17.9#

