

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010453.D
 Acq On : 09 Jun 2017 14:51
 Operator : SJ/MA
 Sample : PB99573BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK73

Quant Time: Jun 10 01:48:07 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 10 01:45:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	254934	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	943897	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.54	164	639021	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	1466642	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1506743	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1520884	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	33464	5.39	ng/uL	0.00
5) Phenol-d5	7.09	99	485462	25.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	277070	25.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	429082	27.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	407618	26.15	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	204976	29.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	251091	31.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	499079	30.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	539731	34.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	1807673	34.05	ng/ul	0.00
46) Acenaphthylene-d8	14.24	160	1909112	30.82	ng/ul	0.00
51) 4-Nitrophenol-d4	14.78	143	194843	24.53	ng/ul	0.00
57) Fluorene-d10	15.53	176	1485388	31.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	294345	28.33	ng/ul	0.00
70) Anthracene-d10	17.39	188	2365144	33.14	ng/ul	0.00
76) Pyrene-d10	19.67	212	2547723	40.89	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.64	264	2346001	33.13	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.63	70	16832	1.324	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010453.D
Acq On : 09 Jun 2017 14:51
Operator : SJ/MA
Sample : PB99573BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Time: Jun 10 01:48:07 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 10 01:45:58 2017
Response via : Initial Calibration

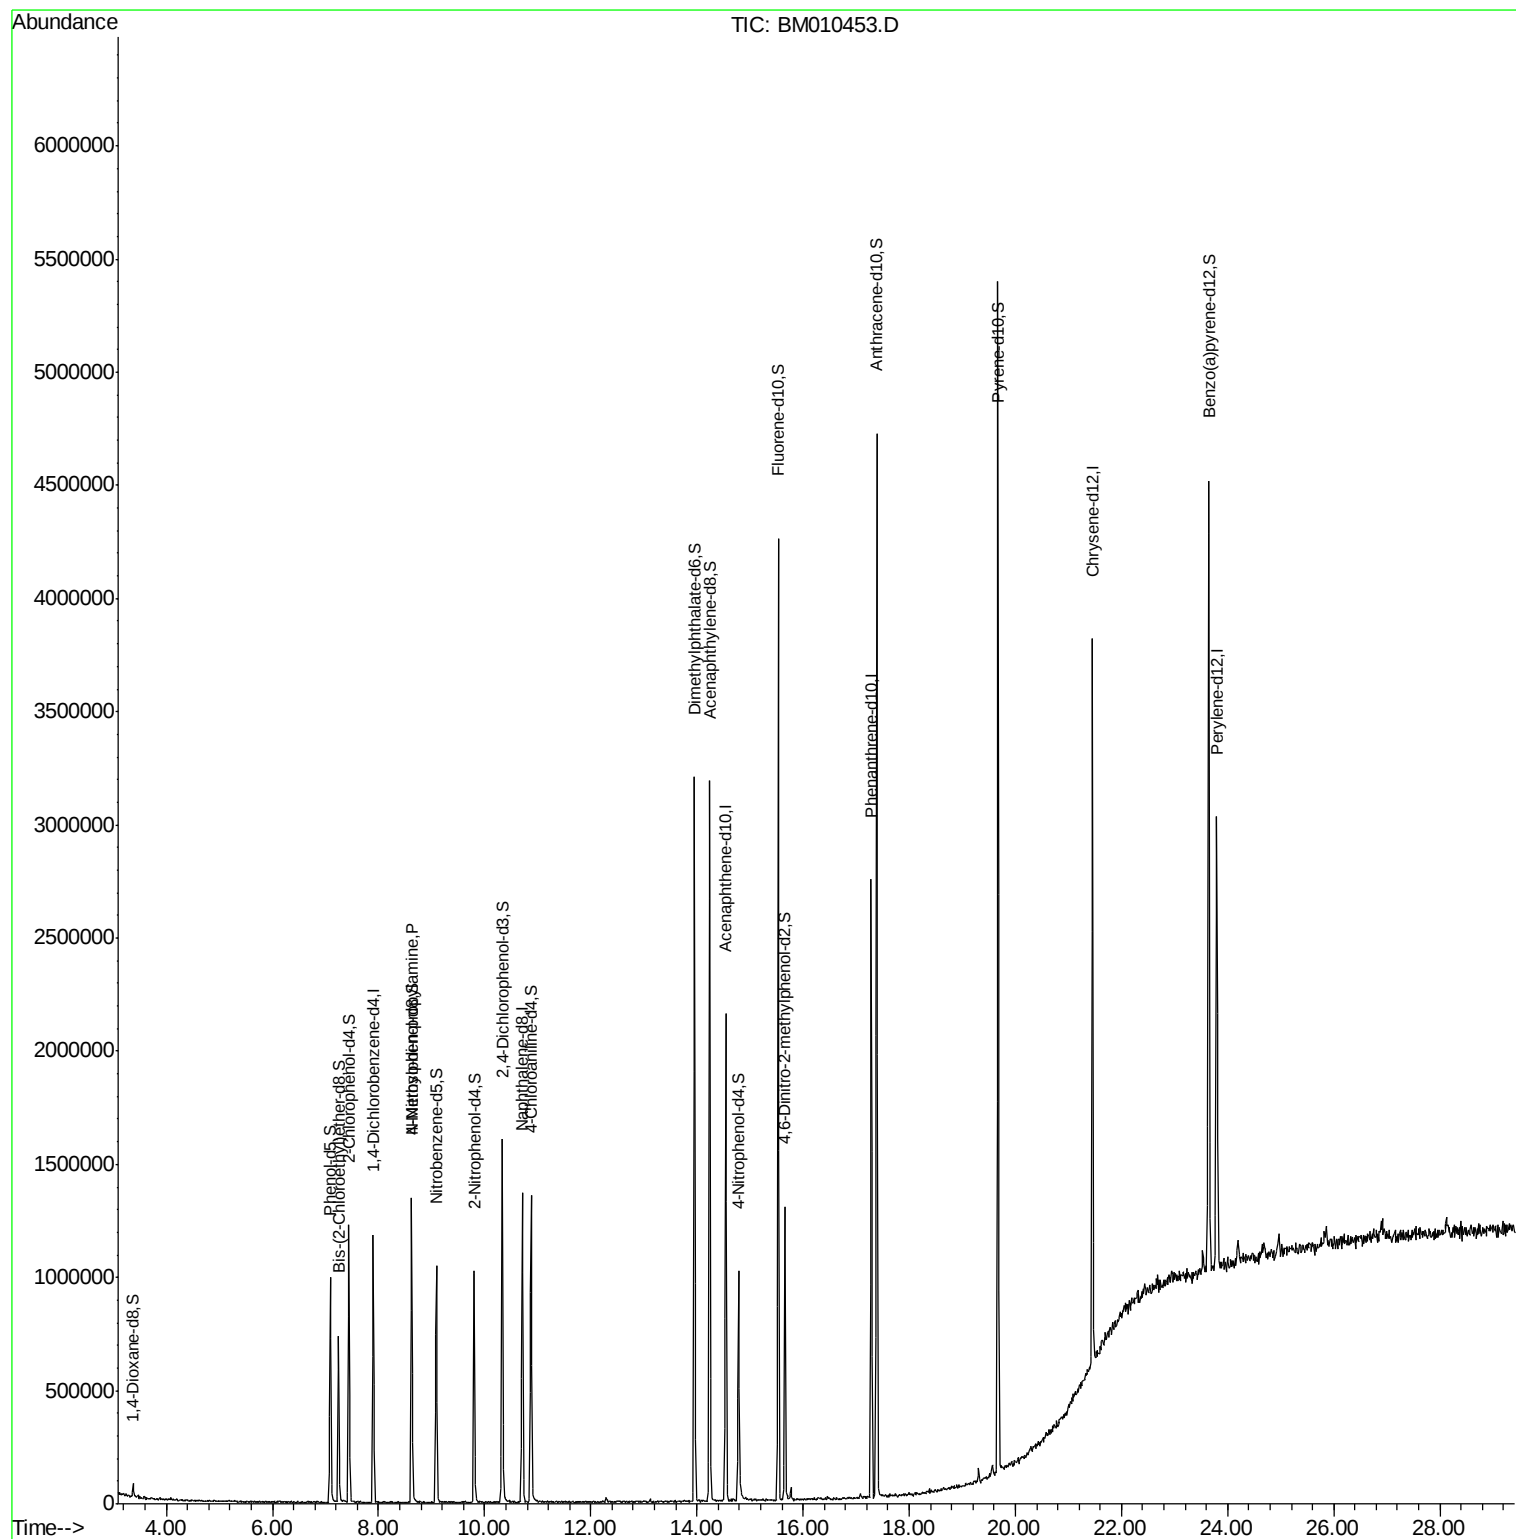

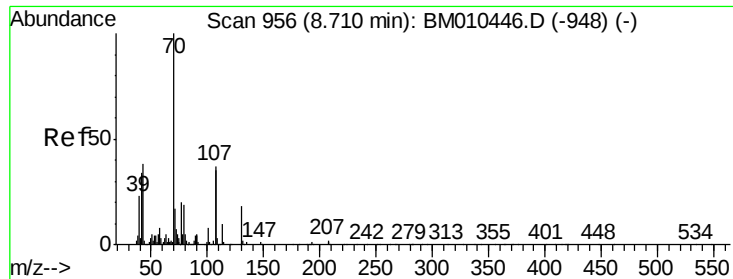

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.324 ng/ul
 RT: 8.63 min Scan# 942
 Delta R.T. -0.08 min
 Lab File: BM010453.D
 Acq: 09 Jun 2017 14:51

Instrument :
 BNA_M
 ClientSampleId :
 SBLK73

Tgt Ion:	70	Resp:	16832
Ion	Ratio	Lower	Upper
70	100		
42	247.9	41.1	61.7#
101	0.0	6.7	10.1#
130	0.0	14.6	22.0#

