

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010468.D
 Acq On : 09 Jun 2017 23:51
 Operator : SJ/MA
 Sample : I3520-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5B11

Quant Time: Jun 10 02:34:26 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 10 02:32:05 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	282369	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	1081583	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.54	164	742878	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	1827445	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1935808	20.00	ng/ul	0.00
83) Perylene-d12	23.79	264	1759121	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.37	96	30585	4.44	ng/uL	0.00
5) Phenol-d5	7.09	99	573706	26.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	320630	26.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.44	132	501969	29.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	493195	28.57	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	238452	30.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	303601	33.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	607753	32.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	643528	35.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	2177739	35.28	ng/ul	0.00
46) Acenaphthylene-d8	14.24	160	2341551	32.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.78	143	254240	27.53	ng/ul	0.00
57) Fluorene-d10	15.53	176	1852930	34.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	373045	28.82	ng/ul	0.00
70) Anthracene-d10	17.39	188	3059877	34.41	ng/ul	0.00
76) Pyrene-d10	19.67	212	3567883	44.57	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.64	264	2871021	35.05	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	7.12	94	33600	1.532	ng/ul	89
15) N-Nitroso-di-n-propylamine	8.62	70	21773	1.546	ng/ul#	1
21) Isophorone	9.80	82	45107	1.295	ng/ul#	76
44) Dimethylphthalate	14.00	163	524238	8.636	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010468.D
Acq On : 09 Jun 2017 23:51
Operator : SJ/MA
Sample : I3520-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5B11

Quant Time: Jun 10 02:34:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 10 02:32:05 2017
Response via : Initial Calibration

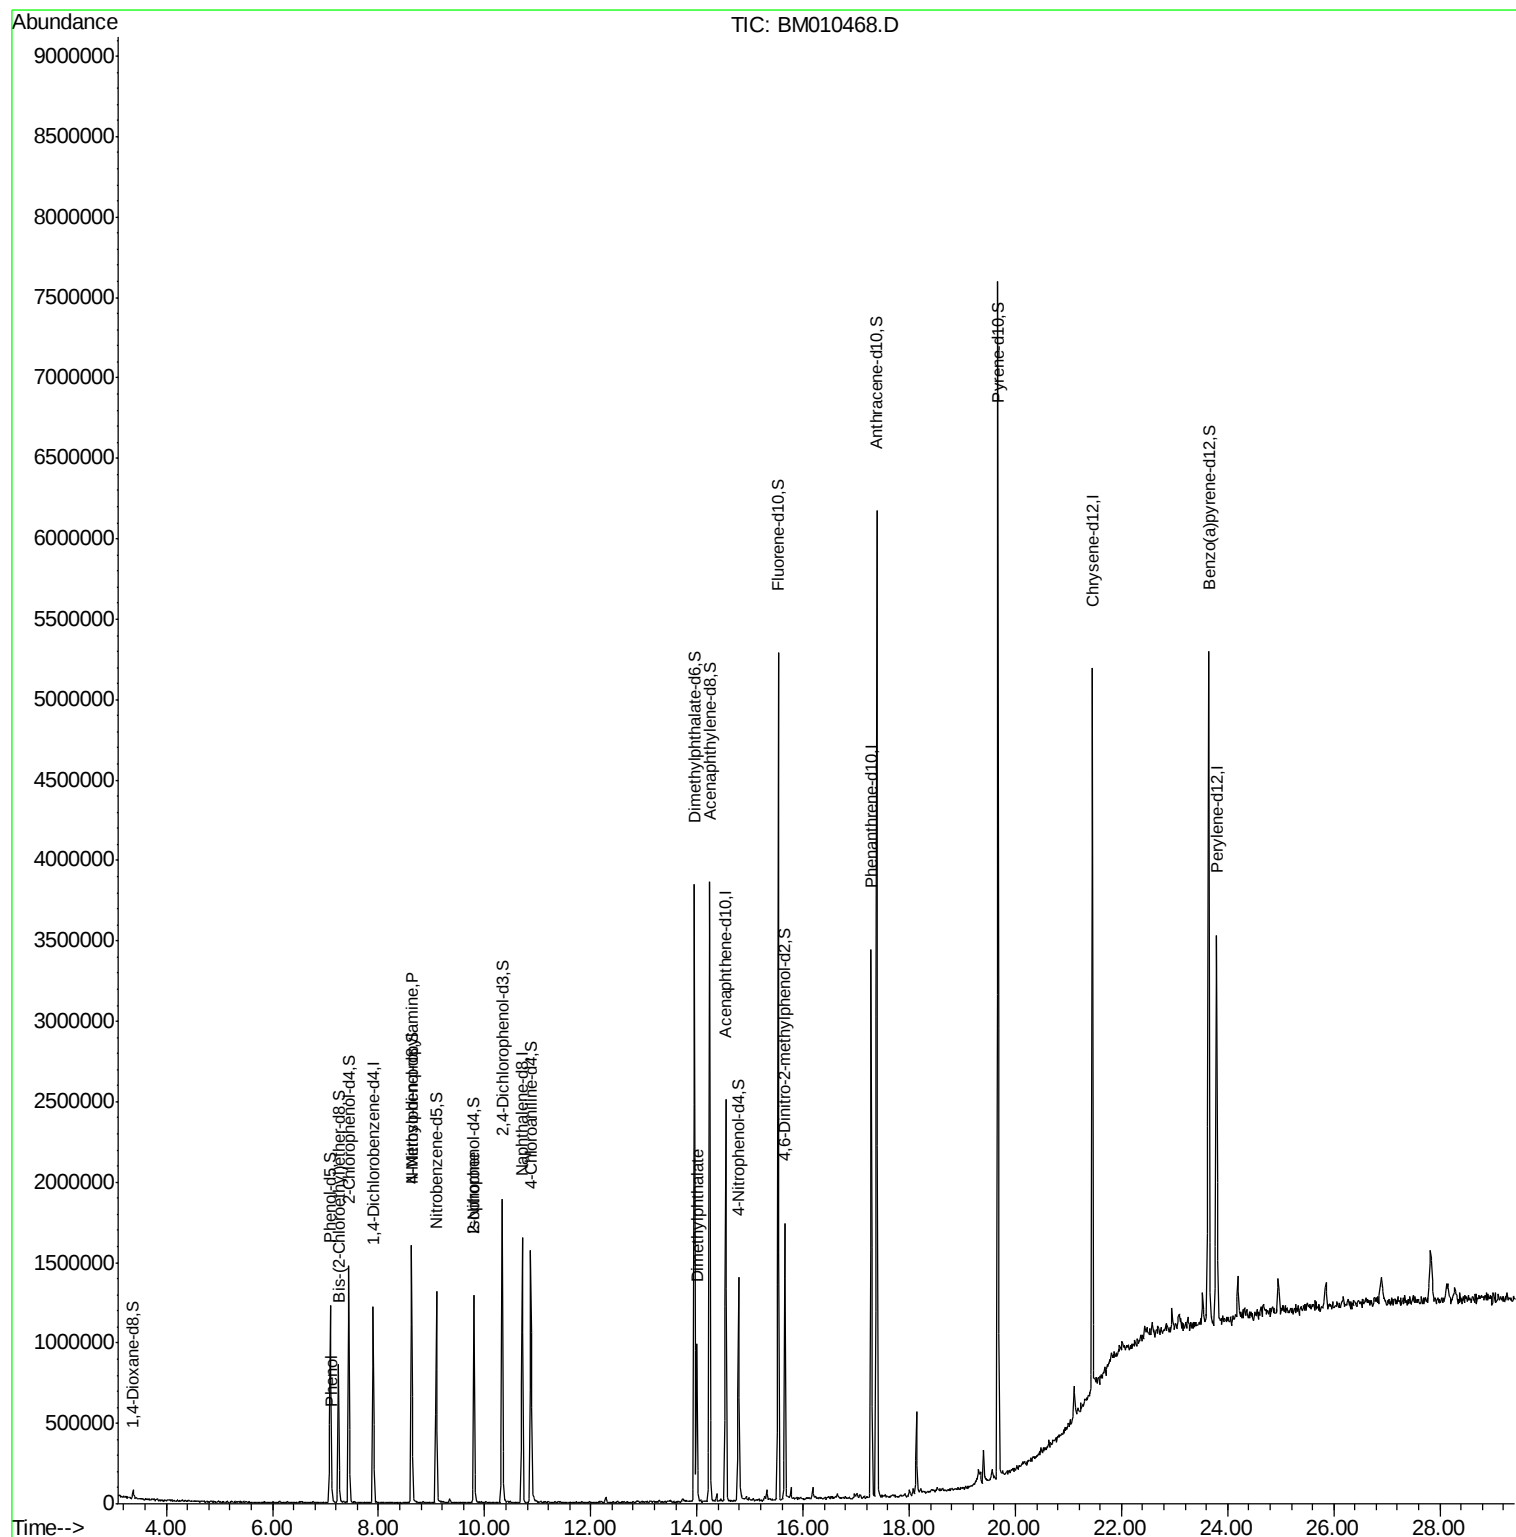

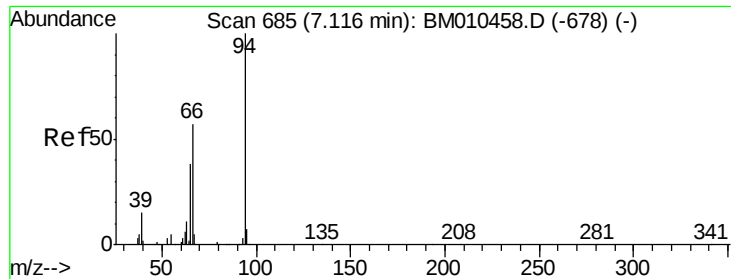

#6

Phenol

Concen: 1.532 ng/ul

RT: 7.12 min Scan# 685

Delta R.T. -0.00 min

Lab File: BM010468.D

Acq: 09 Jun 2017 23:51

Instrument :

BNA_M

ClientSampled :

F5B11


Tgt Ion: 94 Resp: 33600

Ion Ratio Lower Upper

94 100

65 40.8 28.2 42.4




66 67.9 47.2 70.8

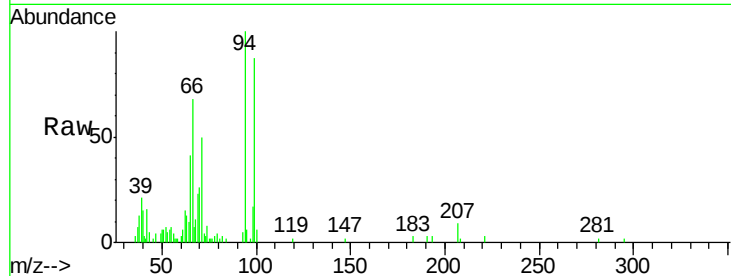

Abundance Ion 94.00 (93.70 to 94.70): BM010458.D (-678) (-)

Ion 65.00 (64.70 to 65.70): BM010458.D (-678) (-)

Ion 66.00 (65.70 to 66.70): BM010458.D (-678) (-)

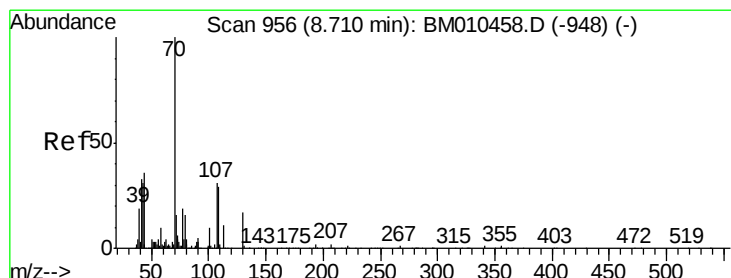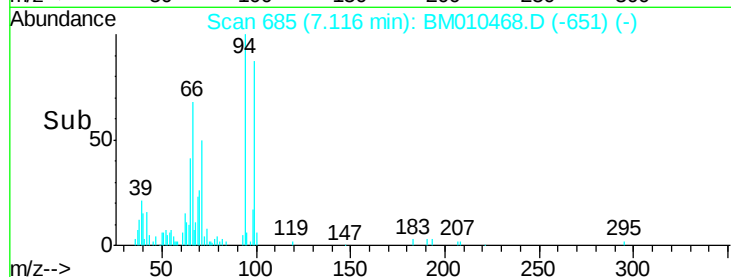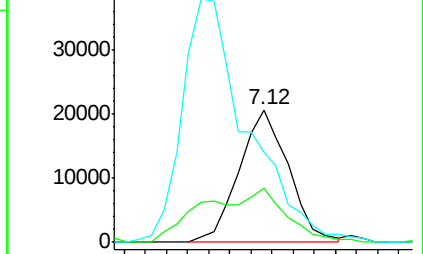

#15

N-Nitroso-di-n-propylamine

Concen: 1.546 ng/ul

RT: 8.62 min Scan# 941

Delta R.T. -0.09 min

Lab File: BM010468.D

Acq: 09 Jun 2017 23:51

Tgt Ion: 70 Resp: 21773


Ion Ratio Lower Upper

70 100

42 173.2 41.1 61.7#

101 0.0 6.7 10.1#

130 0.0 14.6 22.0#


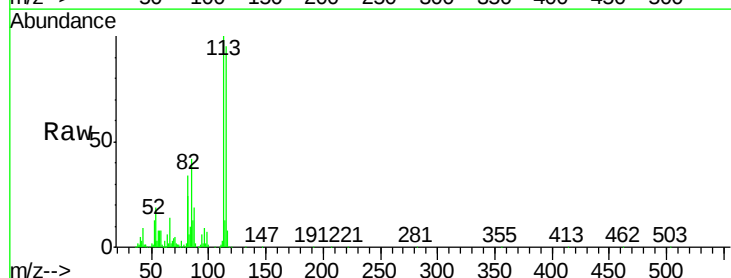



Abundance Ion 70.00 (69.70 to 70.70): BM010458.D (-948) (-)

Ion 42.00 (41.70 to 42.70): BM010458.D (-948) (-)

Ion 101.00 (100.70 to 101.70): BM010458.D (-948) (-)

Ion 130.00 (129.70 to 130.70): BM010458.D (-948) (-)

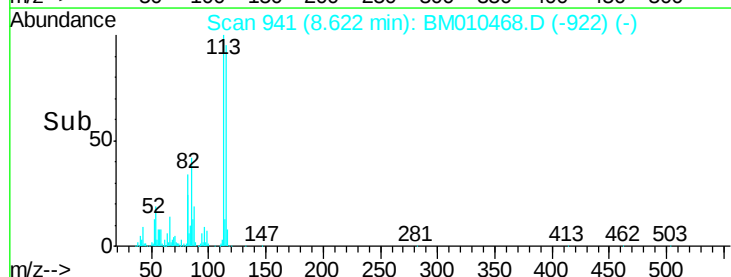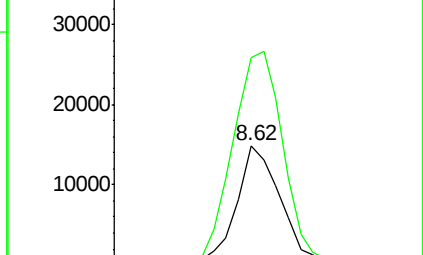

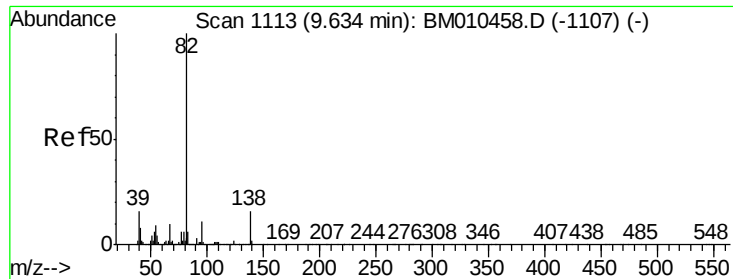

#21

Isophorone

Concen: 1.295 ng/ul

RT: 9.80 min Scan# 1141

Delta R.T. 0.16 min

Lab File: BM010468.D

Acq: 09 Jun 2017 23:51

Instrument :

BNA_M

ClientSampleId :

F5B11





Tgt Ion: 82 Resp: 45107

Ion Ratio Lower Upper

82 100

95 6.3 7.8 11.8#

138 0.9 11.9 17.9#

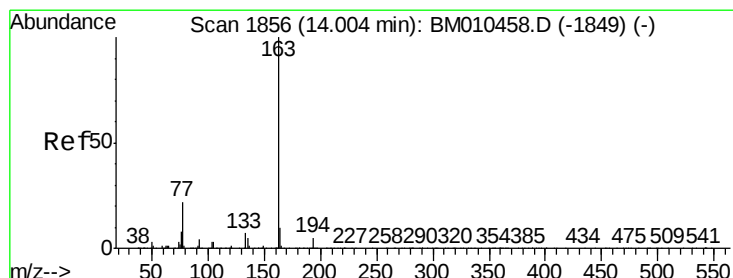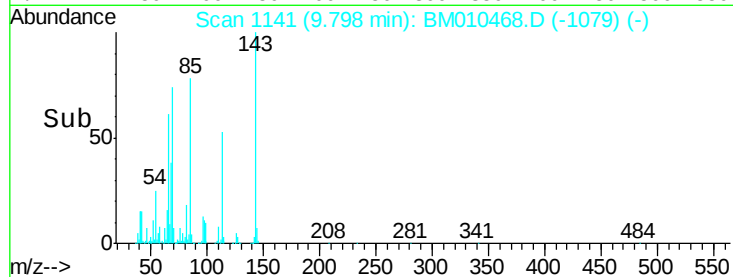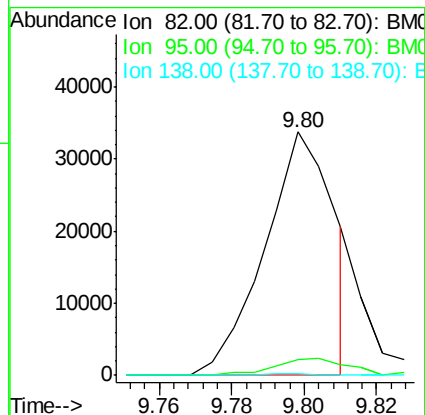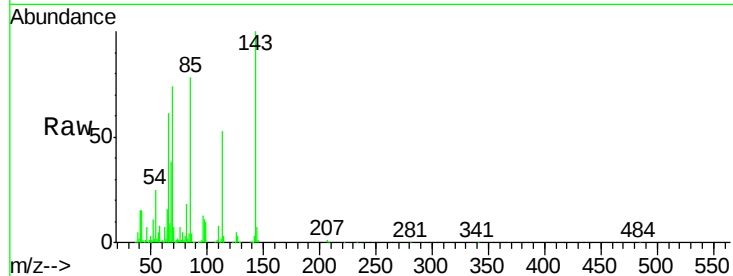

#44

Dimethylphthalate

Concen: 8.636 ng/ul

RT: 14.00 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BM010468.D

Acq: 09 Jun 2017 23:51

Tgt Ion: 163 Resp: 524238

Ion Ratio Lower Upper

163 100

194 5.0 3.5 5.3

164 10.3 8.2 12.4

